

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026334.D
 Acq On : 16 Jun 2022 15:22
 Operator : SY/MD
 Sample : N3275-07
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0BD9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026334.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.121	20	25	34	rVB2	10011	10638	1.79%	0.199%
2	1.224	51	57	62	rBV	5515	6073	1.02%	0.114%
3	1.317	79	86	107	rBV	95552	105834	17.83%	1.983%
4	1.580	160	168	180	rBV	89812	100627	16.95%	1.886%
5	1.764	217	225	237	rBV	21531	28796	4.85%	0.540%
6	2.121	325	336	351	rBV	177674	255393	43.02%	4.786%
7	2.207	351	363	364	rBV	17236	23022	3.88%	0.431%
8	2.442	399	436	438	rBV2	29894	128727	21.69%	2.412%
9	3.924	885	897	944	rBV2	35136	169009	28.47%	3.167%
10	4.362	1016	1033	1065	rBV2	110306	284354	47.90%	5.329%
11	5.056	1234	1249	1281	rBV3	238105	593603	100.00%	11.125%
12	5.625	1412	1426	1449	rBV	226962	464644	78.28%	8.708%
13	5.921	1506	1518	1543	rBV2	115877	238512	40.18%	4.470%
14	6.075	1551	1566	1589	rBV	137261	284117	47.86%	5.325%
15	6.992	1841	1851	1872	rBV2	53581	100720	16.97%	1.888%
16	7.320	1938	1953	1971	rBV	260064	465307	78.39%	8.720%
17	7.628	2040	2049	2067	rBV2	28989	53214	8.96%	0.997%
18	7.940	2132	2146	2150	rBV3	4017	6337	1.07%	0.119%
19	7.982	2150	2159	2172	rVB3	26200	45189	7.61%	0.847%
20	8.095	2184	2194	2229	rBV2	177976	384992	64.86%	7.215%
21	8.854	2418	2430	2451	rBV	347469	569865	96.00%	10.680%
22	10.217	2841	2854	2869	rBV	85989	136919	23.07%	2.566%
23	10.381	2896	2905	2919	rVB2	9817	15524	2.62%	0.291%
24	11.249	3164	3175	3194	rBV	294984	454437	76.56%	8.516%
25	11.532	3254	3263	3280	rBV3	22484	43366	7.31%	0.813%
26	11.625	3280	3292	3311	rVB	228273	366764	61.79%	6.873%




Sum of corrected areas: 5335983

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026334.D
Acq On : 16 Jun 2022 15:22
Operator : SY/MD
Sample : N3275-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

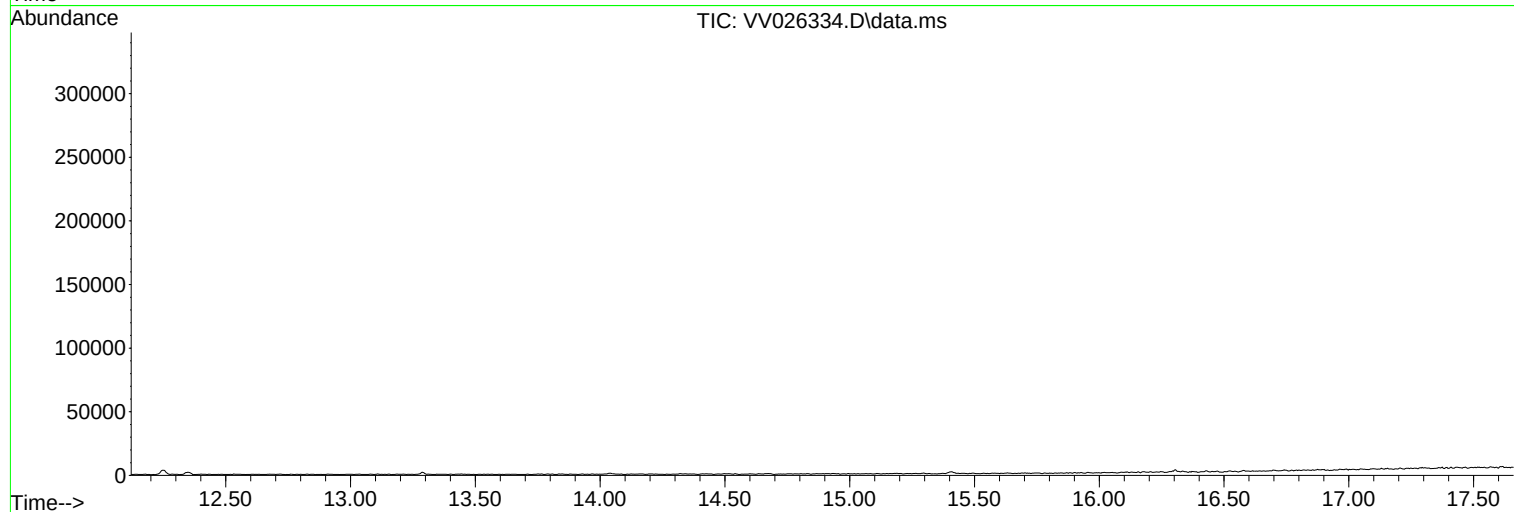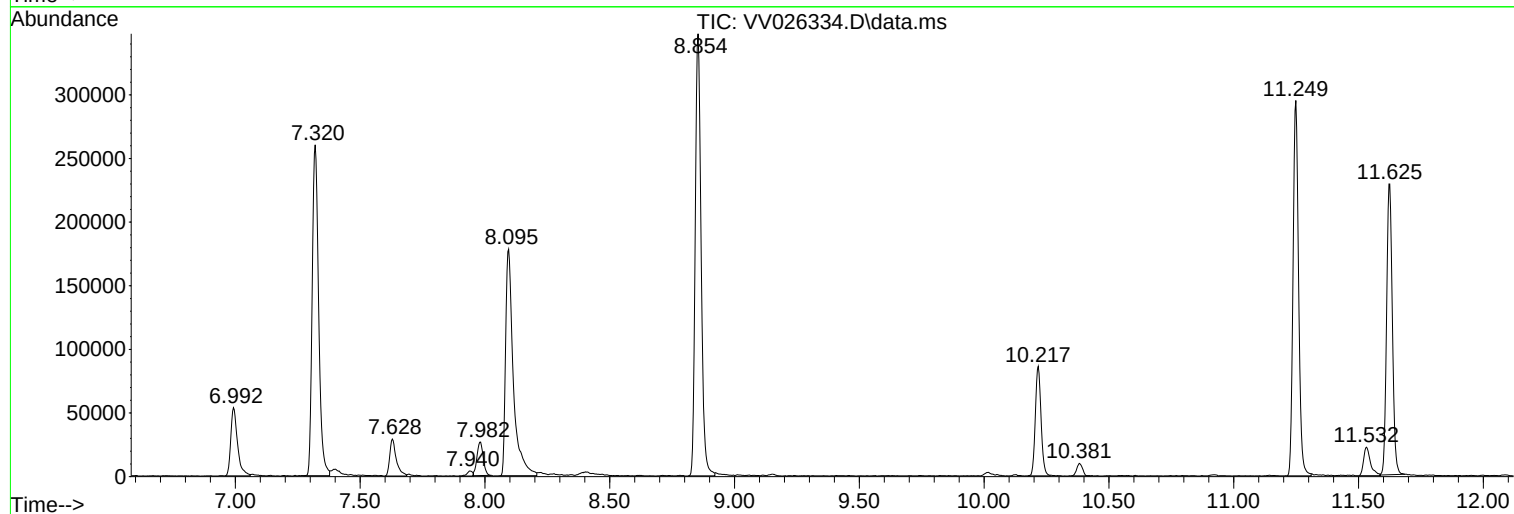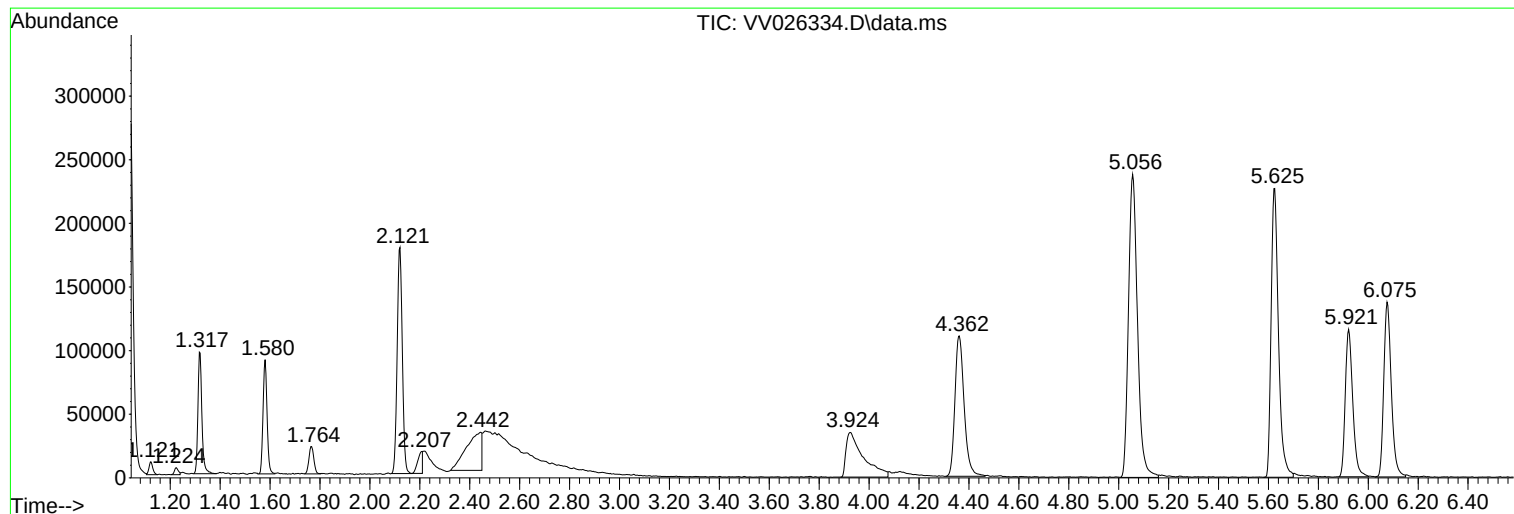

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026334.D
Acq On : 16 Jun 2022 15:22
Operator : SY/MD
Sample : N3275-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD9










Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

Peak Number 1 Isopropyl Alcohol Concentration Rank 1

R.T.	EstConc	Area	Relative to ISTD	R.T.
2.442	1.39 ug/L	128727	1,4-Difluorobenzene	5.625

Hit#	of	5	Tentative ID	MW	MolForm	CAS#	Qual
1			Isopropyl Alcohol	60	C3H8O	000067-63-0	86
2			Isopropyl Alcohol	60	C3H8O	000067-63-0	78
3			Isopropyl Alcohol	60	C3H8O	000067-63-0	64
4			Isopropyl Alcohol	60	C3H8O	000067-63-0	56
5			Isopropyl Alcohol	60	C3H8O	000067-63-0	9

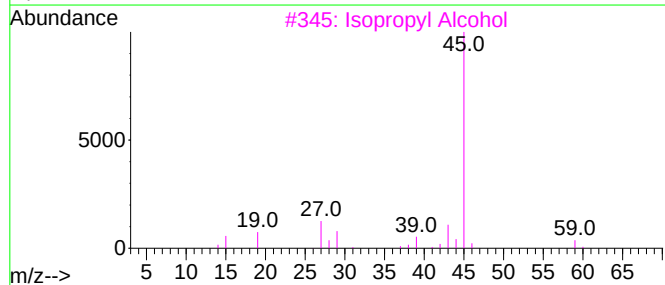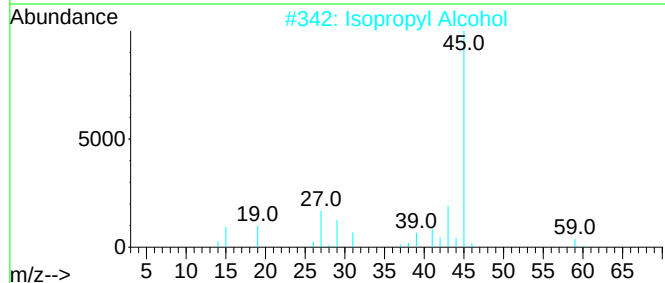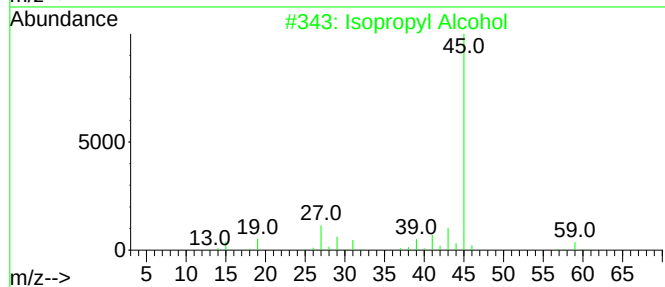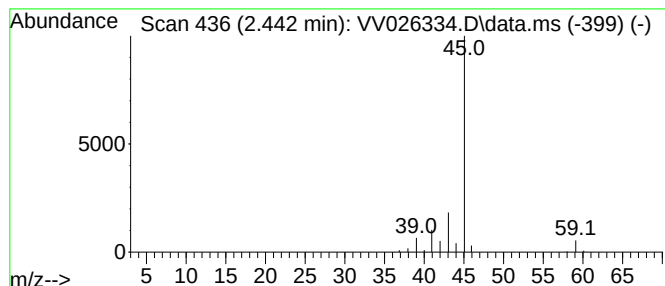

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026334.D
Acq On : 16 Jun 2022 15:22
Operator : SY/MD
Sample : N3275-07
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 16 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BD9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
Isopropyl Alcohol	2.442	1.4	ug/L	128727	1	5.625	464644	5.0