

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026336.D
 Acq On : 16 Jun 2022 16:09
 Operator : SY/MD
 Sample : N3275-08
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 COBE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV026336.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.124	20	26	38	rVB2	14065	14858	2.46%	0.282%
2	1.224	52	57	63	rBV	6023	7143	1.18%	0.135%
3	1.320	79	87	98	rBV	99642	107591	17.83%	2.039%
4	1.581	161	168	181	rVB	90229	104361	17.30%	1.978%
5	1.767	218	226	238	rBV5	3700	6533	1.08%	0.124%
6	2.121	325	336	350	rBV	178415	256152	42.45%	4.856%
7	2.214	350	365	398	rBV2	44138	179615	29.77%	3.405%
8	3.924	885	897	940	rBV2	35437	160015	26.52%	3.033%
9	4.362	1017	1033	1058	rBV	113626	288768	47.86%	5.474%
10	5.059	1232	1250	1293	rBV2	241584	603405	100.00%	11.438%
11	5.625	1412	1426	1453	rBV	207589	429544	71.19%	8.142%
12	5.921	1505	1518	1545	rBV	134453	277356	45.97%	5.257%
13	6.075	1553	1566	1593	rBV	139017	290014	48.06%	5.497%
14	6.992	1841	1851	1867	rBV	52613	100010	16.57%	1.896%
15	7.143	1888	1898	1913	rVB7	3449	6338	1.05%	0.120%
16	7.320	1942	1953	1971	rBV	268754	472444	78.30%	8.955%
17	7.400	1971	1978	1990	rVB	8497	16896	2.80%	0.320%
18	7.628	2038	2049	2077	rBV	27920	54428	9.02%	1.032%
19	7.982	2151	2159	2172	rVB4	9207	15788	2.62%	0.299%
20	8.095	2183	2194	2216	rBV2	182598	374000	61.98%	7.089%
21	8.854	2419	2430	2458	rBV	316453	521104	86.36%	9.878%
22	9.143	2508	2520	2534	rBV3	7431	14271	2.37%	0.271%
23	10.217	2840	2854	2870	rBV2	86964	135797	22.51%	2.574%
24	10.381	2891	2905	2914	rVB3	5314	8586	1.42%	0.163%
25	11.249	3161	3175	3196	rBV	273333	426997	70.76%	8.094%
26	11.532	3253	3263	3280	rBV	19310	35815	5.94%	0.679%
27	11.625	3280	3292	3310	rVV	232897	367649	60.93%	6.969%




Sum of corrected areas: 5275478

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026336.D
Acq On : 16 Jun 2022 16:09
Operator : SY/MD
Sample : N3275-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

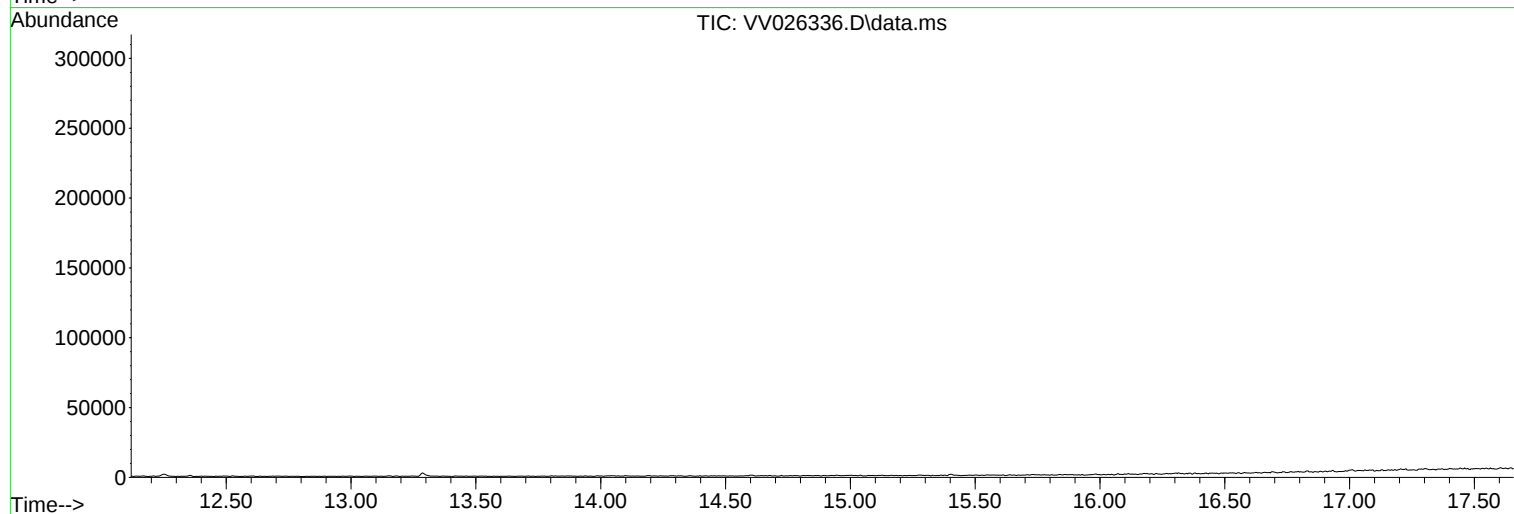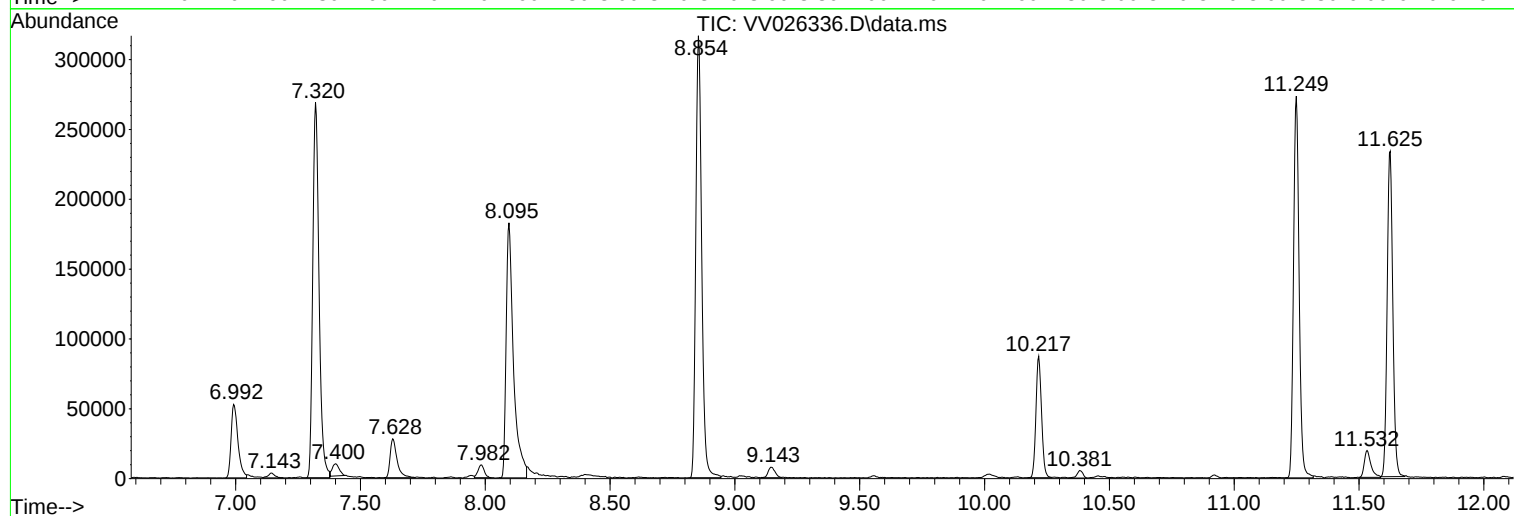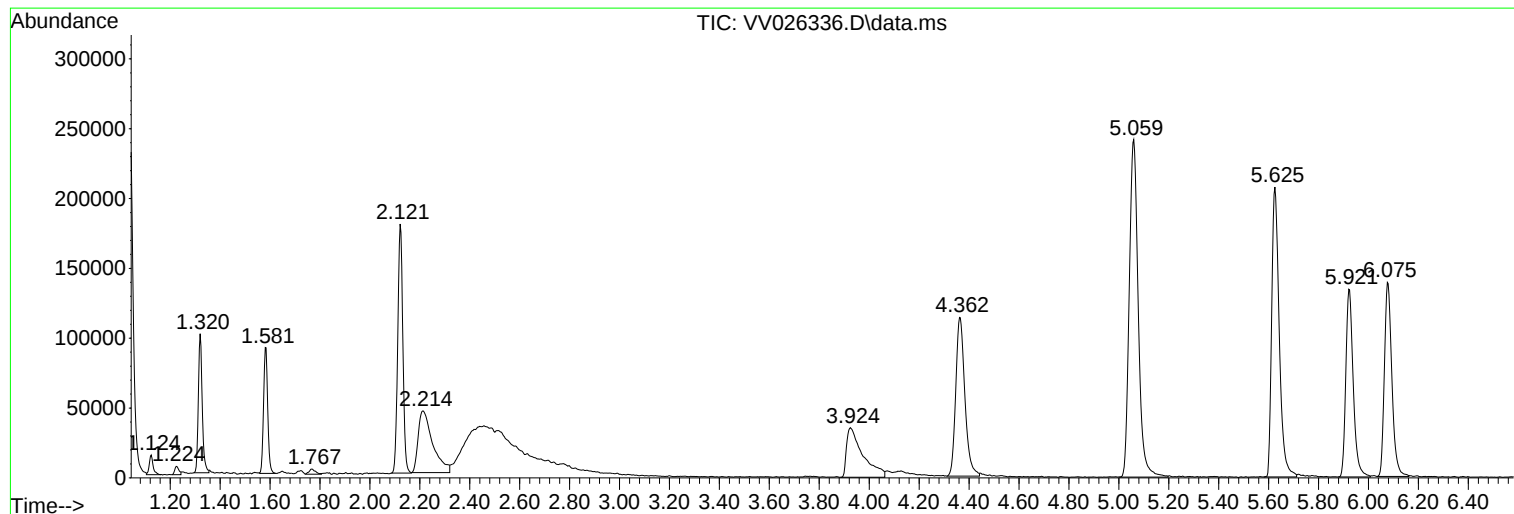

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026336.D
Acq On : 16 Jun 2022 16:09
Operator : SY/MD
Sample : N3275-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026336.D
Acq On : 16 Jun 2022 16:09
Operator : SY/MD
Sample : N3275-08
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0BE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
