

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026359.D
 Acq On : 17 Jun 2022 02:04
 Operator : SY/MD
 Sample : N3318-14
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 43 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ68

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026359.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.320	78	87	101	rVB2	105383	128925	16.63%	1.986%
2	1.552	140	159	161	rBV	28776	73631	9.50%	1.134%
3	1.580	162	168	185	rVB	95936	137962	17.80%	2.125%
4	2.127	327	338	356	rVB3	265965	459901	59.33%	7.083%
5	2.786	528	543	567	rBV2	42121	94938	12.25%	1.462%
6	3.204	658	673	696	rBV	115809	248457	32.05%	3.827%
7	3.928	886	898	925	rBV3	57773	193943	25.02%	2.987%
8	4.362	1017	1033	1063	rBV	113381	303402	39.14%	4.673%
9	5.059	1231	1250	1282	rBV2	231718	584055	75.34%	8.995%
10	5.625	1411	1426	1451	rBV	211453	434860	56.10%	6.698%
11	5.918	1504	1517	1550	rBV	386665	775179	100.00%	11.939%
12	6.075	1553	1566	1595	rVB2	136799	286971	37.02%	4.420%
13	6.992	1840	1851	1878	rBV2	41364	82582	10.65%	1.272%
14	7.320	1942	1953	1972	rBV	260082	459887	59.33%	7.083%
15	7.632	2041	2050	2067	rBV	22018	40146	5.18%	0.618%
16	7.979	2139	2158	2174	rBV	213126	363858	46.94%	5.604%
17	8.095	2184	2194	2229	rBV2	176963	371876	47.97%	5.728%
18	8.853	2415	2430	2459	rBV	326252	532979	68.76%	8.209%
19	10.217	2843	2854	2873	rBV	88373	142062	18.33%	2.188%
20	11.249	3164	3175	3192	rBV	276528	430717	55.56%	6.634%
21	11.622	3280	3291	3310	rBV	221636	346455	44.69%	5.336%




Sum of corrected areas: 6492786

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026359.D
Acq On : 17 Jun 2022 02:04
Operator : SY/MD
Sample : N3318-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

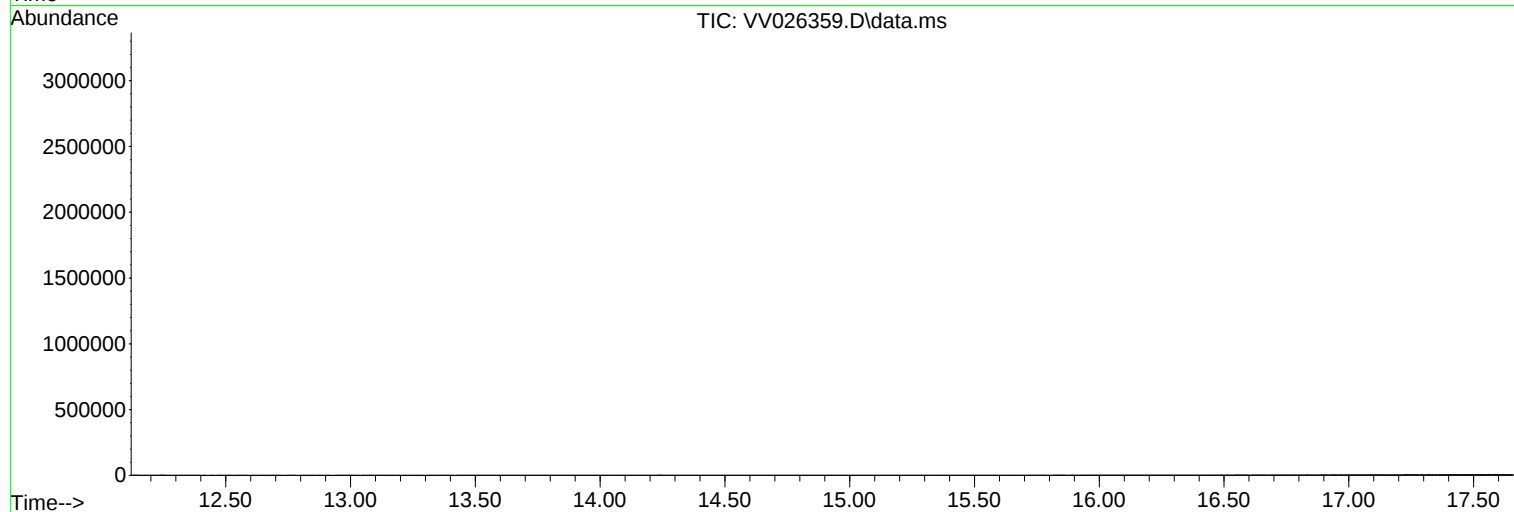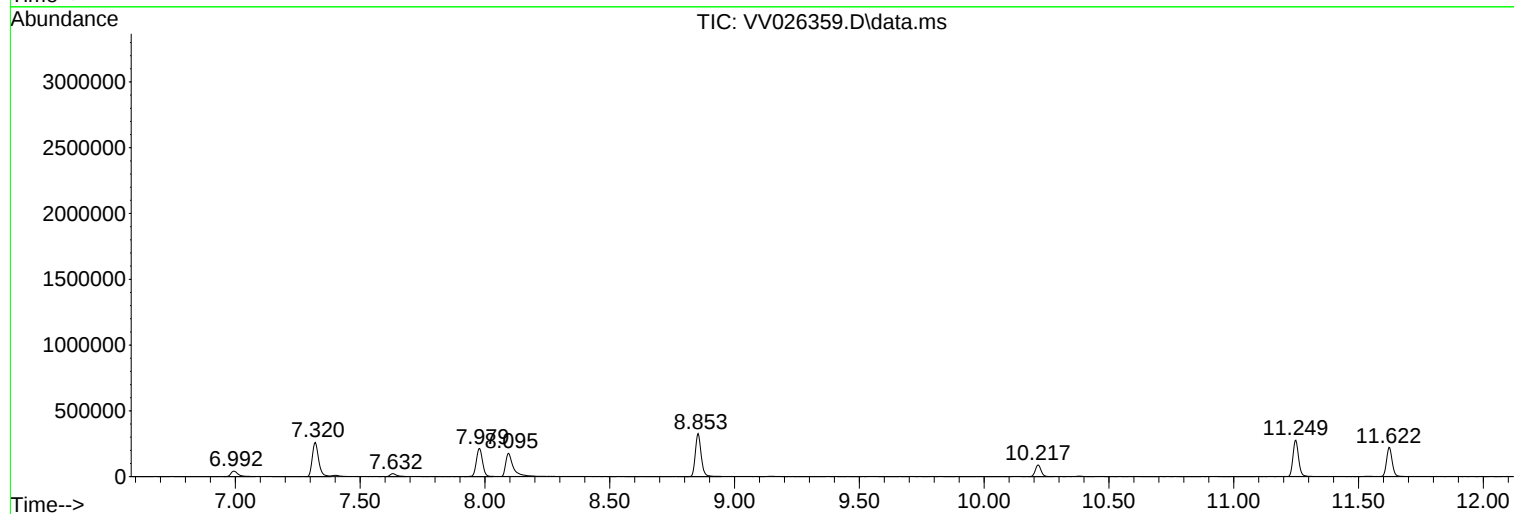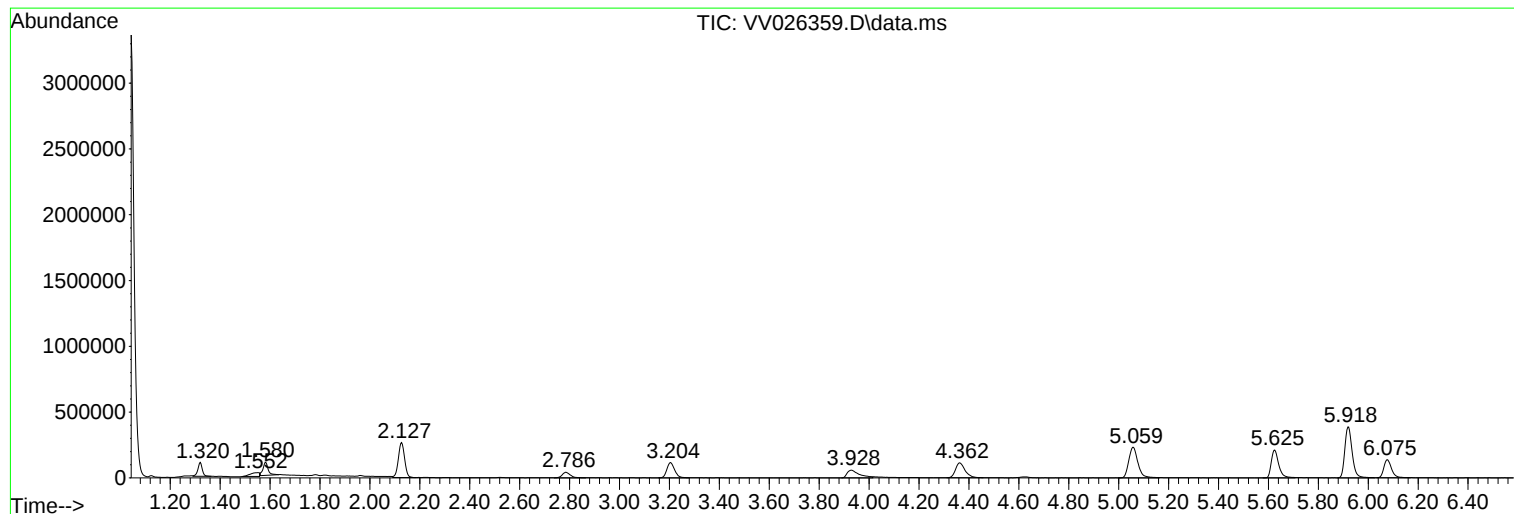

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026359.D
Acq On : 17 Jun 2022 02:04
Operator : SY/MD
Sample : N3318-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026359.D
Acq On : 17 Jun 2022 02:04
Operator : SY/MD
Sample : N3318-14
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 43 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ68

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
