

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
 Data File : VV026363.D
 Acq On : 17 Jun 2022 03:39
 Operator : SY/MD
 Sample : N3320-16 10X
 Misc : 25mL/MSVOA_V/WATER
 ALS Vial : 47 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BGJ91

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV026363.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.288	53	77	79	rBV3	9489	27539	4.70%	0.567%
2	1.323	81	88	100	rVB	96862	110732	18.89%	2.280%
3	1.542	135	156	161	rBV	36799	118752	20.26%	2.445%
4	1.584	163	169	184	rVB	99071	139205	23.75%	2.866%
5	2.124	327	337	354	rVB	174463	260812	44.50%	5.370%
6	2.526	451	462	475	rBV2	11719	19235	3.28%	0.396%
7	3.937	878	901	945	rBV4	47470	231566	39.51%	4.768%
8	4.365	1017	1034	1054	rBV2	110757	273633	46.69%	5.634%
9	5.060	1233	1250	1286	rBV2	234777	586094	100.00%	12.068%
10	5.625	1414	1426	1454	rBV	211003	436682	74.51%	8.992%
11	5.931	1509	1521	1538	rBV6	11979	26786	4.57%	0.552%
12	6.076	1554	1566	1589	rBV	135094	282094	48.13%	5.809%
13	6.992	1841	1851	1881	rBV2	40550	78942	13.47%	1.625%
14	7.320	1939	1953	1973	rBV	264967	458399	78.21%	9.439%
15	7.632	2039	2050	2069	rBV2	21178	40853	6.97%	0.841%
16	8.095	2183	2194	2225	rBV2	159438	338467	57.75%	6.969%
17	8.854	2417	2430	2453	rBV	318261	524458	89.48%	10.799%
18	10.217	2841	2854	2873	rBV	86870	136094	23.22%	2.802%
19	11.249	3164	3175	3197	rBV	274890	423442	72.25%	8.719%
20	11.622	3279	3291	3315	rBV	215862	342746	58.48%	7.057%




Sum of corrected areas: 4856531

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026363.D
Acq On : 17 Jun 2022 03:39
Operator : SY/MD
Sample : N3320-16 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

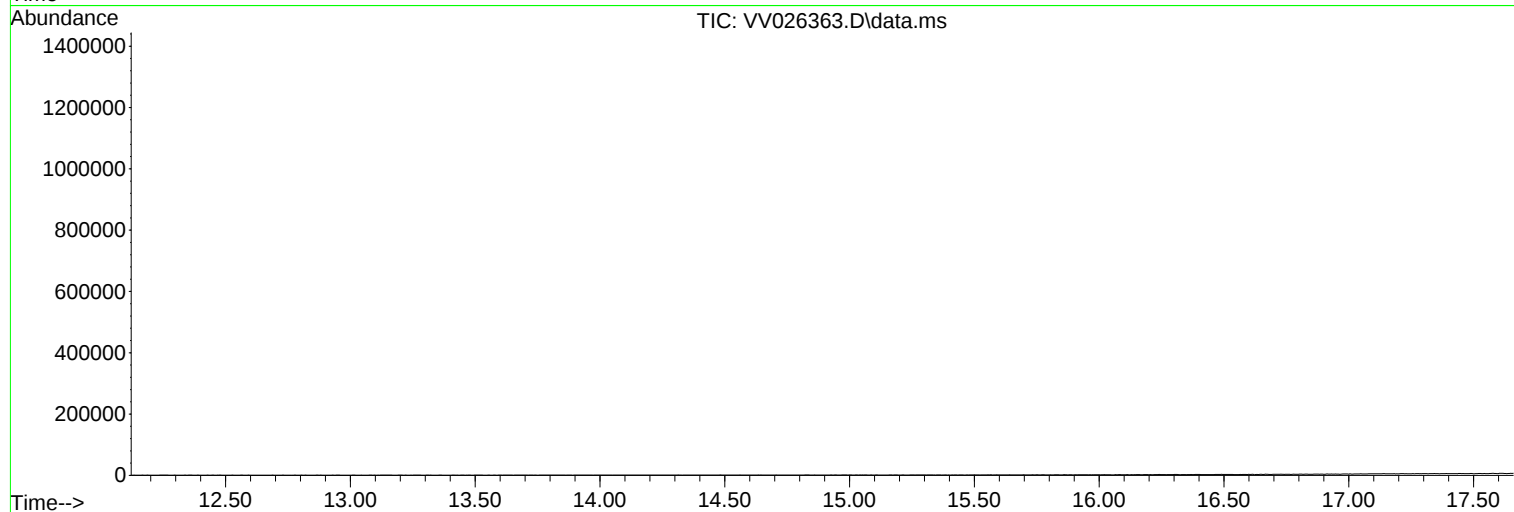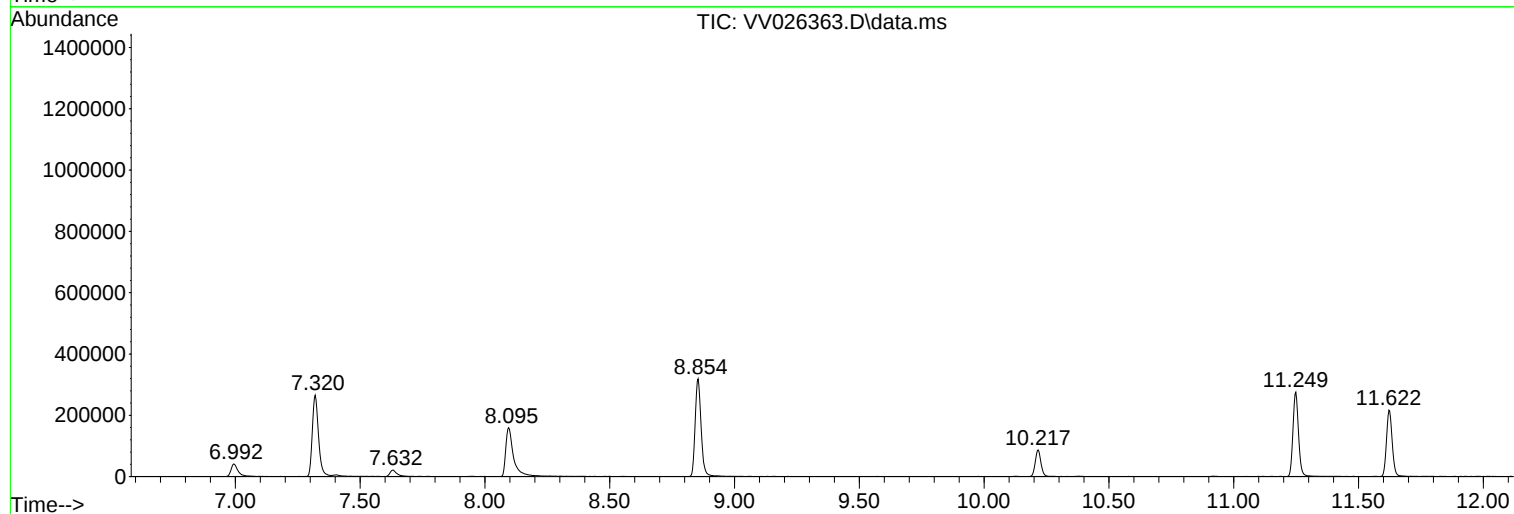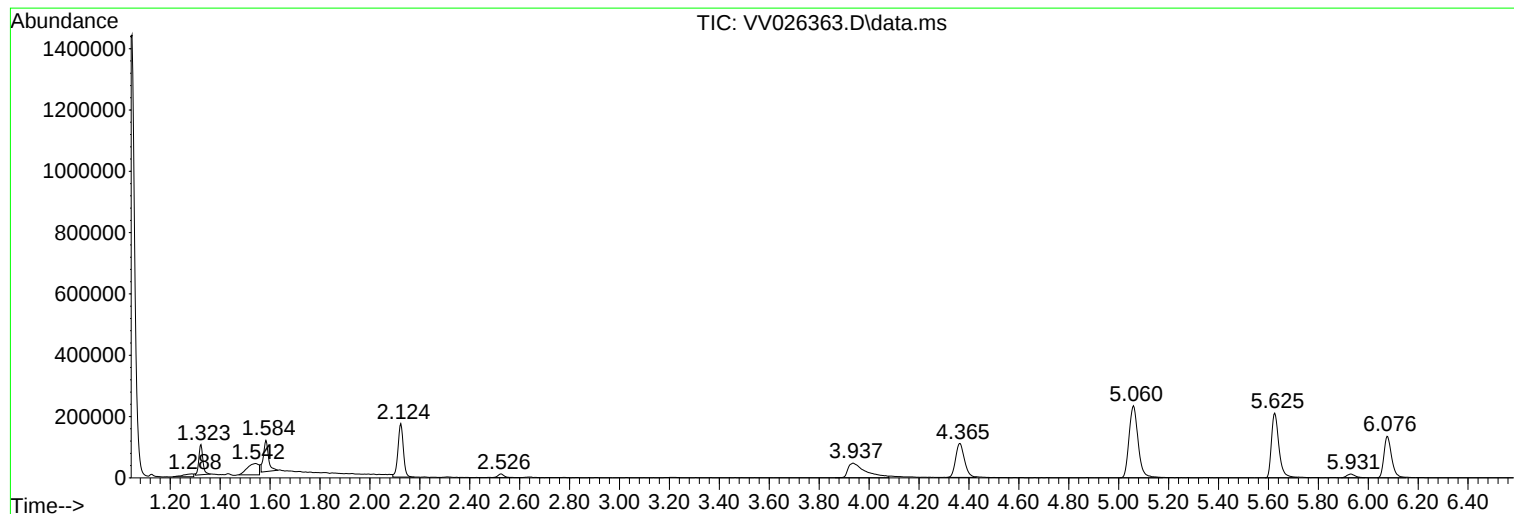

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026363.D
Acq On : 17 Jun 2022 03:39
Operator : SY/MD
Sample : N3320-16 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV061622\
Data File : VV026363.D
Acq On : 17 Jun 2022 03:39
Operator : SY/MD
Sample : N3320-16 10X
Misc : 25mL/MSVOA_V/WATER
ALS Vial : 47 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BGJ91

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR061522WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------