

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081722\
 Data File : VV027417.D
 Acq On : 17 Aug 2022 12:29
 Operator : SY/MD
 Sample : N4192-03
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Quant Time: Aug 18 01:42:15 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Thu Aug 18 01:40:54 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	132837	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	134739	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	56289	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.304	65	39167	3.394	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	67.800%	
7) Chloroethane-d5	1.565	69	35760	4.266	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	85.400%	
11) 1,1-Dichloroethene-d2	2.105	63	66218	3.164	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	63.200%	
20) 2-Butanone-d5	3.886	46	75781	38.772	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	77.540%	
24) Chloroform-d	4.343	84	108649	5.133	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	102.600%	
26) 1,2-Dichloroethane-d4	5.027	65	56993	5.652	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	113.000%	
32) Benzene-d6	5.043	84	190971	4.805	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	96.000%	
36) 1,2-Dichloropropane-d6	6.066	67	68023	5.535	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	110.800%	
41) Toluene-d8	7.313	98	139262	3.827	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	76.600%	
43) trans-1,3-Dichloroprop...	7.622	79	20210	4.748	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	95.000%	
46) 2-Hexanone-d5	8.088	63	88317	53.610	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	107.220%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	49999	5.624	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	112.400%	
66) 1,2-Dichlorobenzene-d4	11.622	152	54575	5.617	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	112.400%	
Target Compounds						Qvalue
16) Methylene chloride	2.503	84	6629	0.432	ug/L	98


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081722\
Data File : VV027417.D
Acq On : 17 Aug 2022 12:29
Operator : SY/MD
Sample : N4192-03
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Time: Aug 18 01:42:15 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Thu Aug 18 01:40:54 2022
Response via : Initial Calibration

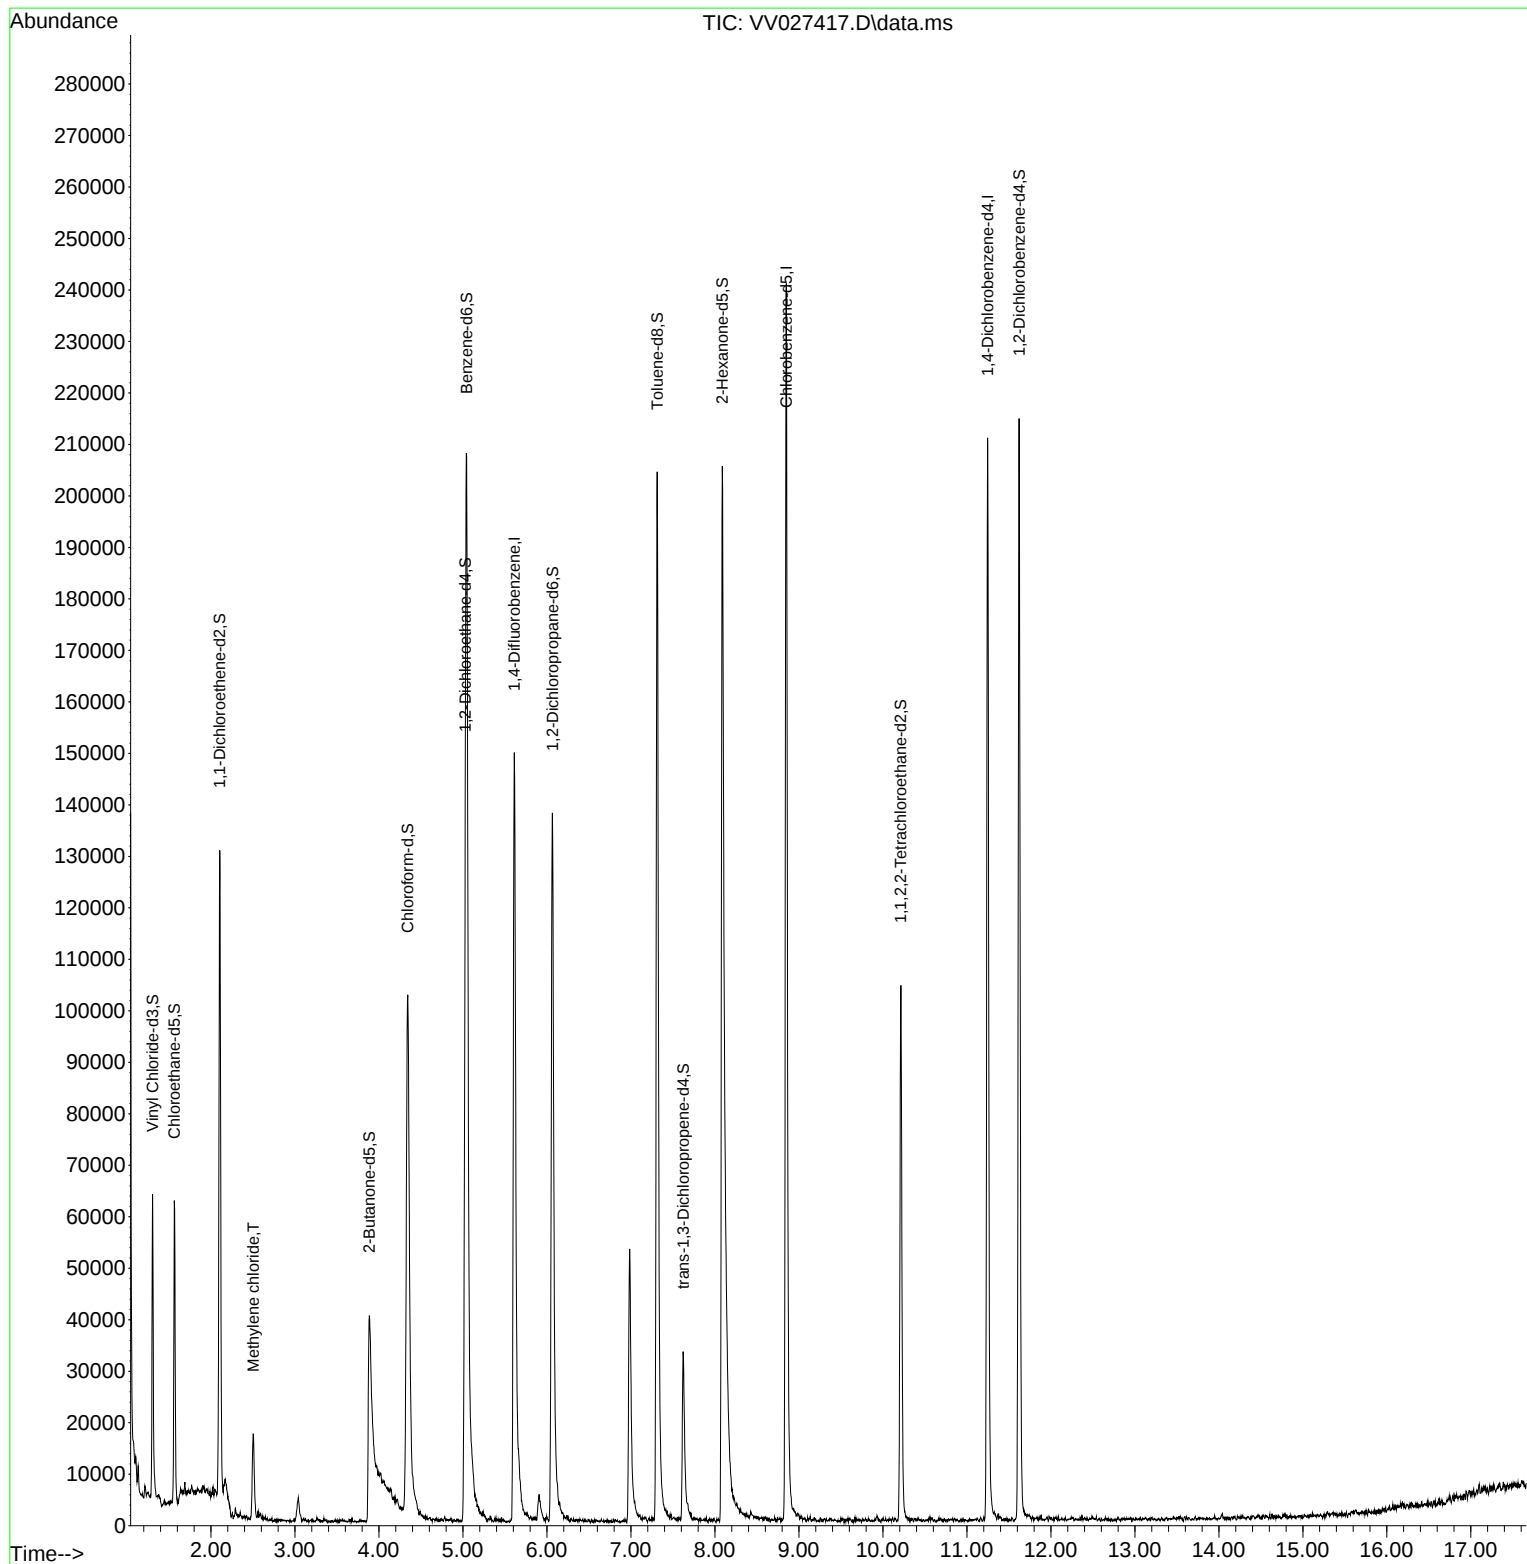

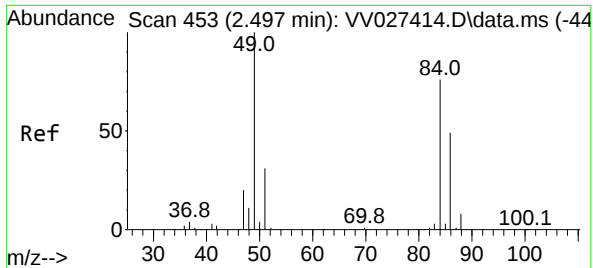

#16
Methylene chloride
Concen: 0.432 ug/L
RT: 2.503 min Scan# 4
Delta R.T. 0.007 min
Lab File: VV027417.D
Acq: 17 Aug 2022 12:29

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Tgt Ion:	84	Resp:	6629
Ion	Ratio	Lower	Upper
84	100		
86	64.8	45.1	83.9
49	134.2	91.2	169.4

