
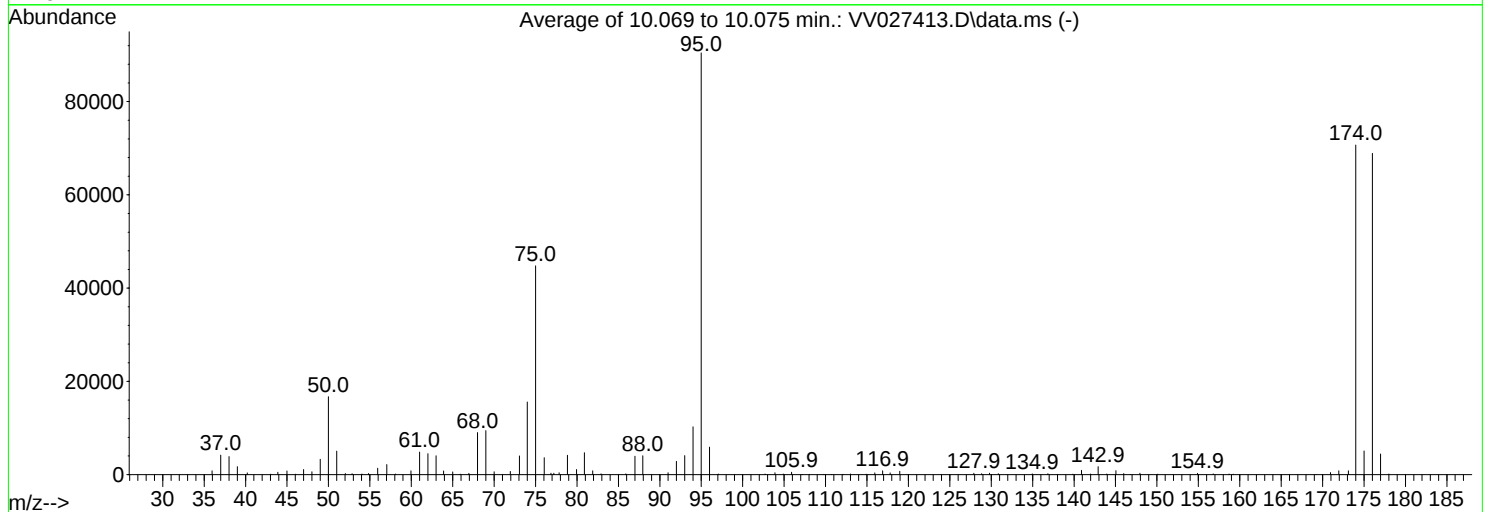


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV081722\
Data File : VV027413.D
Acq On : 17 Aug 2022 09:10
Operator : SY/MD
Sample : BFB355
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 1 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
BFB355

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR081122WMA.M
Title : TRACE VOA SFAM1.0
Last Update : Thu Aug 18 01:40:54 2022

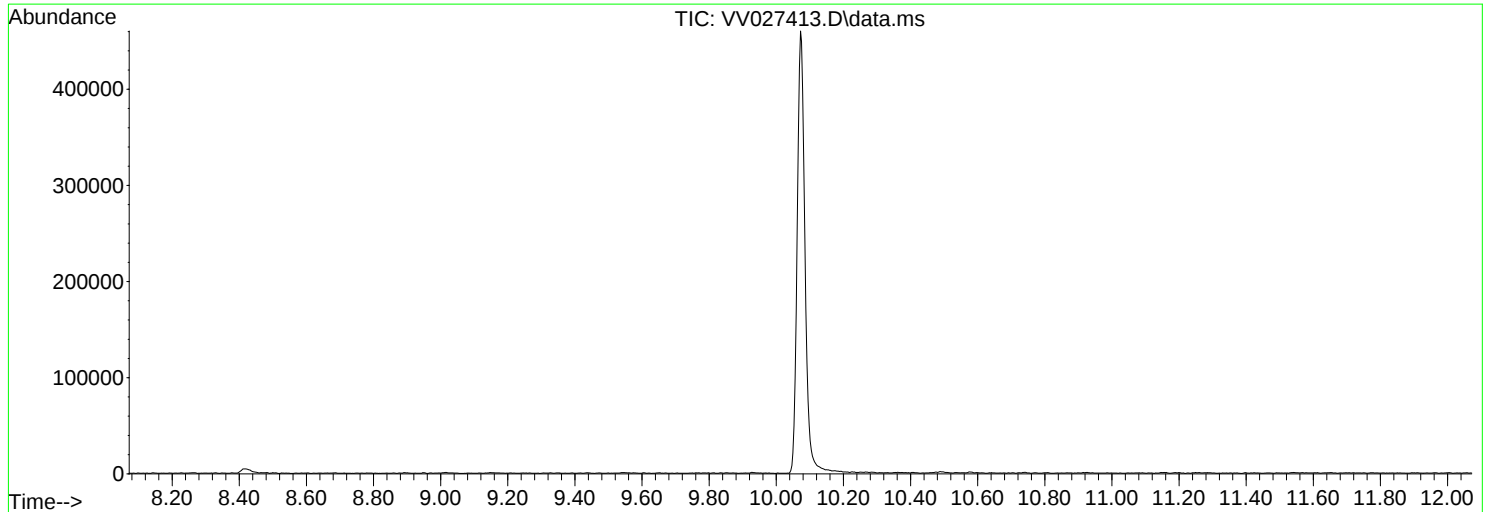

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2796

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	18.5	16720	PASS
75	95	30	80	49.5	44792	PASS
95	95	100	100	100.0	90453	PASS
96	95	5	9	6.5	5911	PASS
173	174	0.00	2	1.2	828	PASS
174	95	50	120	78.1	70669	PASS
175	174	5	9	7.2	5086	PASS
176	174	95	105	97.5	68907	PASS
177	176	5	10	6.4	4421	PASS

m/z	Abundance
35.70	117.0
39.80	268.0
44.00	305.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

m/z	Abundance
36.00	813.0
37.00	4164.0
38.00	3941.0
39.00	1692.0
40.20	358.0
43.10	120.0
43.90	850.0
45.00	698.0
46.00	184.0
47.00	1168.0
48.00	586.0
49.00	3275.0
50.00	15952.0
51.00	4928.0
52.10	289.0
52.90	189.0
54.10	105.0
54.90	241.0
56.00	1390.0
57.00	2110.0
58.10	164.0
59.90	833.0
61.00	4701.0
62.00	4510.0
63.00	3831.0
63.90	750.0
65.00	516.0
66.90	246.0
68.00	8841.0
69.00	9035.0
70.00	574.0
71.90	593.0
73.00	4041.0
74.00	15045.0
75.00	42808.0
76.00	3498.0
77.90	411.0
78.80	3899.0
80.00	969.0
80.90	4419.0
81.90	810.0
82.90	126.0
86.00	194.0
87.00	3675.0
88.00	4097.0
91.00	428.0
92.00	2679.0
93.00	3879.0
94.00	9804.0
95.00	86648.0
96.00	5583.0
97.10	142.0
102.70	139.0
103.90	387.0
104.90	135.0
105.90	457.0
108.00	127.0
112.10	125.0
113.00	168.0
116.00	330.0
116.90	818.0
117.80	338.0
119.00	689.0
127.90	332.0
128.90	193.0
129.80	300.0
130.80	185.0
135.10	169.0
136.80	248.0
139.80	109.0
140.90	864.0
142.00	102.0
142.90	1555.0
143.90	124.0
145.10	832.0
146.00	271.0
146.80	105.0
147.90	301.0
154.90	268.0
156.80	130.0
158.70	159.0
169.20	108.0
170.90	426.0
172.00	773.0
173.10	1227.0
174.00	66224.0
175.00	4830.0
176.00	64088.0
177.00	4135.0
178.00	104.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

m/z	Abundance
35.90	846.0
37.00	4357.0
38.00	4062.0
39.00	1819.0
40.20	349.0
43.00	112.0
43.90	832.0
45.00	834.0
46.10	183.0
47.00	1118.0
48.00	622.0
49.00	3368.0
50.00	17384.0
51.00	5176.0
52.10	212.0
52.80	228.0
54.10	153.0
54.90	221.0
56.00	1419.0
57.00	2259.0
58.10	161.0
60.00	836.0
61.00	5067.0
62.00	4654.0
63.00	4174.0
63.90	786.0
65.00	564.0
65.90	118.0
66.90	315.0
68.00	9341.0
69.00	9815.0
70.00	642.0
71.90	715.0
73.10	4184.0
74.00	16203.0
75.00	46432.0
76.00	3725.0
76.80	476.0
77.20	437.0
77.80	436.0
78.90	4284.0
79.90	1148.0
80.90	4830.0
81.90	836.0
82.90	166.0
85.90	194.0
87.00	4089.0
87.90	4226.0
91.00	449.0
92.00	2955.0
93.00	4214.0
94.00	10496.0
95.00	93744.0
96.00	6158.0
97.10	126.0
102.70	129.0
103.90	447.0
104.90	153.0
105.90	542.0
108.10	112.0
109.80	108.0
112.10	104.0
113.00	156.0
114.90	119.0
116.00	388.0
116.90	837.0
117.80	416.0
119.00	753.0
127.90	334.0
128.80	214.0
129.80	334.0
130.90	237.0
134.90	176.0
136.80	223.0
139.90	111.0
140.90	954.0
142.00	131.0
142.90	1779.0
143.90	153.0
145.10	902.0
146.00	261.0
147.90	322.0
150.10	127.0
154.90	287.0
156.80	166.0
158.70	137.0
159.20	141.0
171.00	469.0
172.00	831.0
173.10	1256.0
174.00	72768.0
175.00	5265.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

176.00	71496.0
177.00	4556.0
178.00	153.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

m/z	Abundance
35.90	819.0
37.00	4091.0
38.00	3674.0
39.00	1661.0
40.20	390.0
43.00	106.0
43.90	783.0
45.00	810.0
47.00	989.0
48.00	621.0
49.00	3213.0
50.00	16824.0
51.00	5042.0
52.00	203.0
52.80	238.0
54.00	198.0
54.80	247.0
55.90	1352.0
57.10	2134.0
58.10	115.0
59.90	823.0
61.00	4721.0
62.00	4374.0
63.00	4186.0
63.90	857.0
65.00	672.0
65.90	160.0
67.00	311.0
68.00	8871.0
69.00	9423.0
70.00	665.0
72.00	730.0
73.00	3865.0
74.00	15488.0
75.00	45136.0
76.10	3676.0
76.90	455.0
77.20	473.0
77.80	388.0
78.90	4237.0
79.90	1208.0
80.90	4841.0
81.90	846.0
82.90	233.0
85.80	163.0
87.00	4094.0
87.90	3819.0
91.00	405.0
92.00	2875.0
93.00	4180.0
94.00	10449.0
95.00	90968.0
96.00	5993.0
97.00	118.0
102.70	117.0
103.90	455.0
104.90	140.0
105.90	518.0
107.20	103.0
109.80	108.0
110.70	108.0
113.00	110.0
114.90	175.0
115.90	419.0
116.90	793.0
117.80	424.0
118.90	696.0
127.90	303.0
128.80	219.0
129.80	301.0
130.90	186.0
134.80	166.0
136.90	185.0
139.90	111.0
140.90	994.0
142.00	149.0
142.90	1825.0
144.00	179.0
145.00	894.0
146.00	218.0
148.00	270.0
150.10	148.0
154.90	283.0
156.80	212.0
158.70	103.0
159.20	131.0
171.00	412.0
171.90	847.0
174.00	73016.0
175.00	5163.0
176.00	71136.0
177.00	4571.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355

178.00

181.0

Instrument :
MSVOA_V
ClientSampleId :
BFB355