

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027947.D
 Acq On : 20 Sep 2022 00:21
 Operator : SY/MD
 Sample : N4658-13
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :

Quant Time: Sep 20 02:12:06 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Sep 20 01:54:53 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	101299	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	104722	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	52801	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	45306	5.728	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	= 114.600%		
7) Chloroethane-d5	1.564	69	41042	5.898	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	= 118.000%		
11) 1,1-Dichloroethene-d2	2.101	63	57399	4.389	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	= 87.800%		
20) 2-Butanone-d5	3.889	46	80869	63.986	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	= 127.980%		
24) Chloroform-d	4.343	84	81095	6.124	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 122.400%		
26) 1,2-Dichloroethane-d4	5.027	65	36051	6.580	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 131.600%#		
32) Benzene-d6	5.043	84	145438	5.857	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	= 117.200%		
36) 1,2-Dichloropropane-d6	6.066	67	45909	5.631	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	= 112.600%		
41) Toluene-d8	7.313	98	108556	4.870	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	= 97.400%		
43) trans-1,3-Dichloroprop...	7.622	79	12937	4.791	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	= 95.800%		
46) 2-Hexanone-d5	8.088	63	66132	55.468	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	= 110.940%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	39793	5.967	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	= 119.400%		
66) 1,2-Dichlorobenzene-d4	11.622	152	49073	5.971	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	= 119.400%		
Target Compounds						Qvalue
12) 1,1-Dichloroethene	2.098	96	624	0.085	ug/L #	1
35) Methylcyclohexane	6.063	83	11112	1.109	ug/L #	21
37) 1,2-Dichloropropane	6.066	63	4670	0.617	ug/L #	85
61) 1,2,3-Trichloropropane	11.249	75	5784	1.495	ug/L #	63
71) Naphthalene	13.506	128	3400	0.228	ug/L #	80


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027947.D
Acq On : 20 Sep 2022 00:21
Operator : SY/MD
Sample : N4658-13
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :

Quant Time: Sep 20 02:12:06 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 20 01:54:53 2022
Response via : Initial Calibration

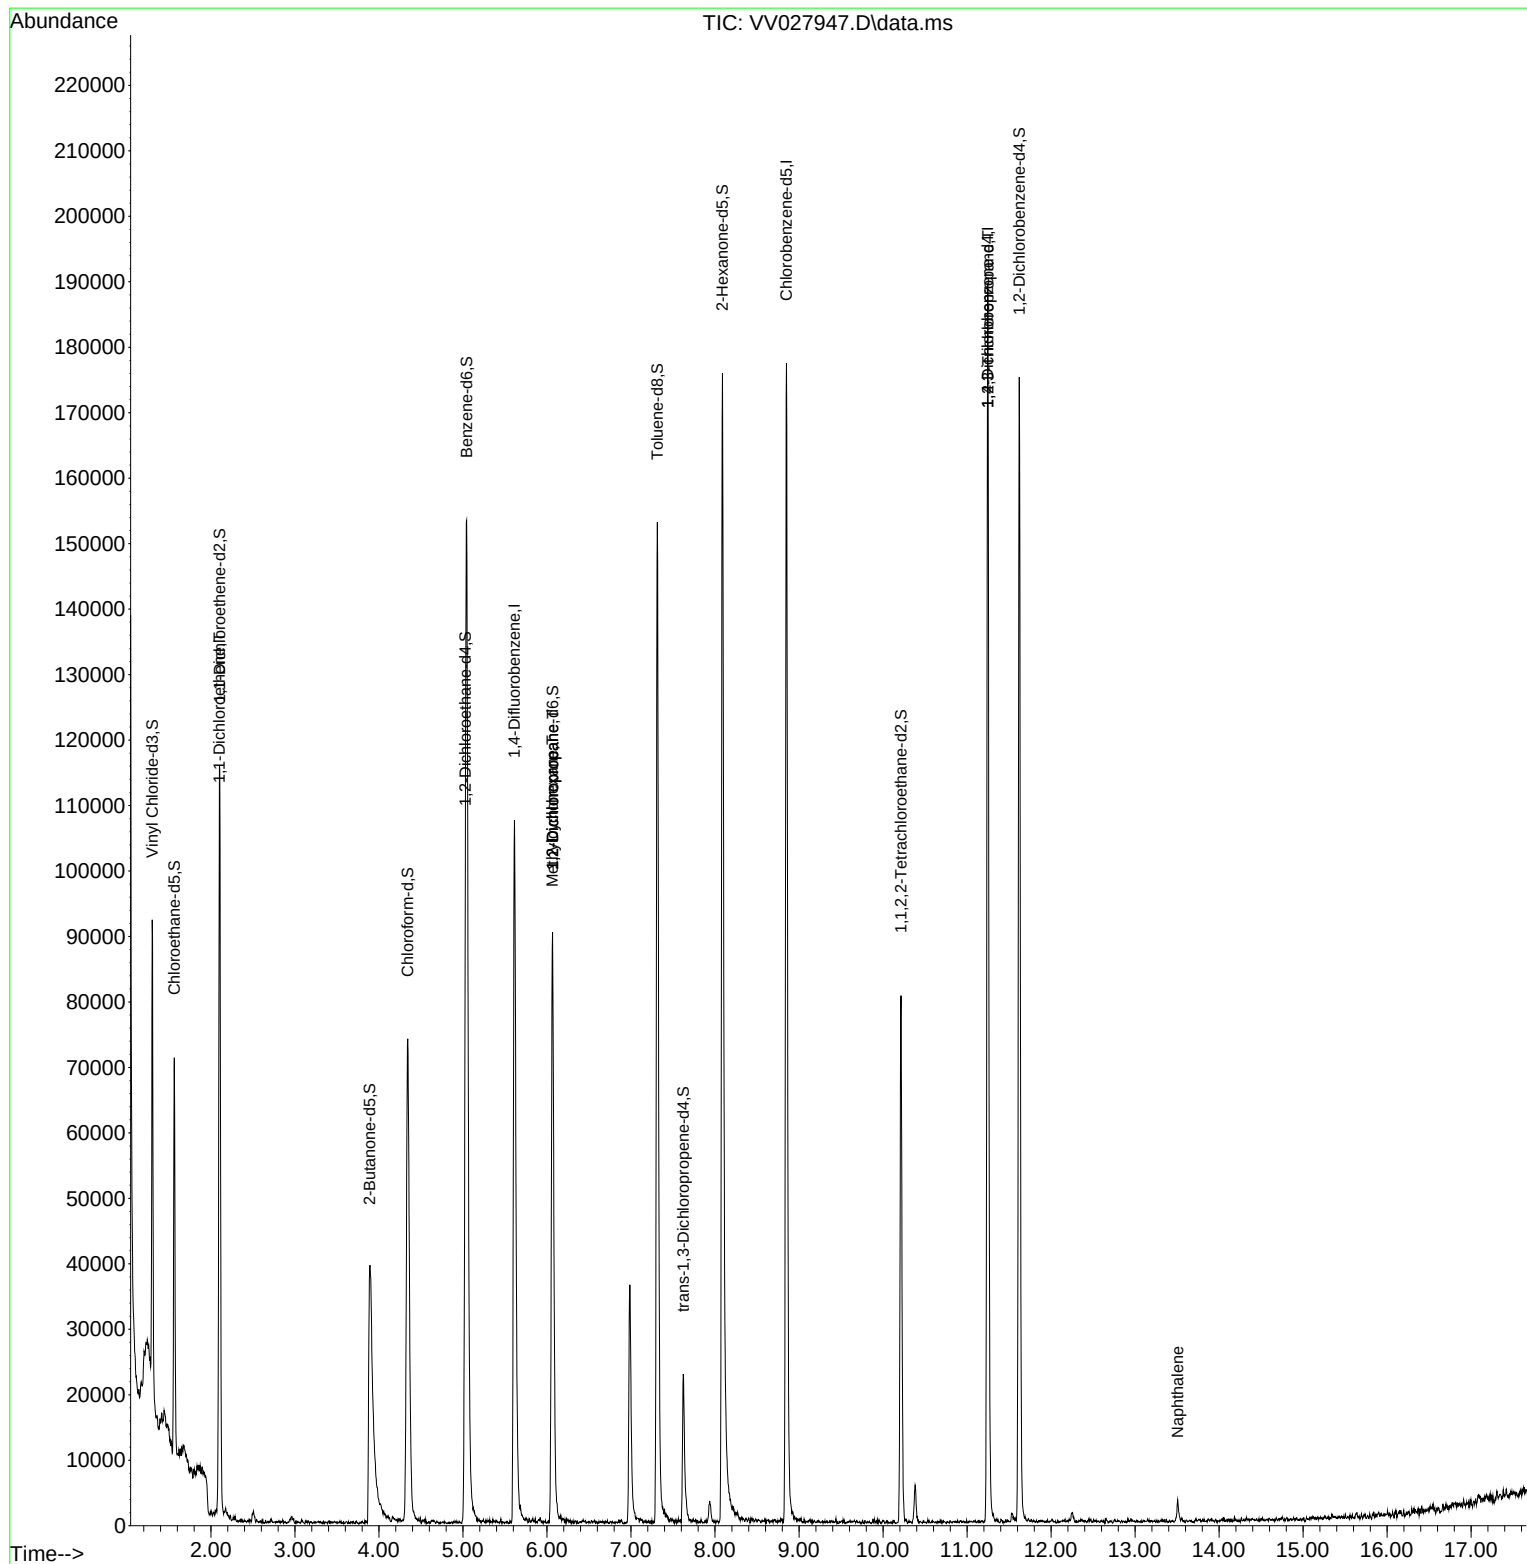

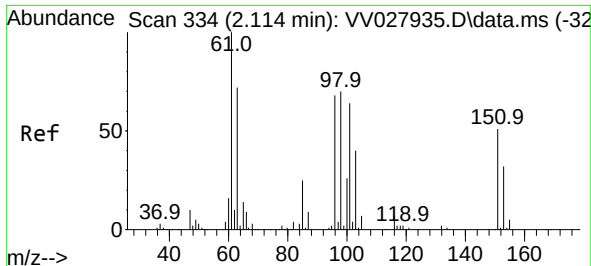

#12

1,1-Dichloroethene

Concen: 0.085 ug/L

RT: 2.098 min Scan# 31

Delta R.T. -0.016 min

Lab File: VV027947.D

Acq: 20 Sep 2022 00:21





Instrument :

MSVOA_V

ClientSampleId :

Tgt Ion: 96 Resp: 624

Ion	Ratio	Lower	Upper
96	100		
61	898.9	106.2	197.2#
63	8253.5	85.0	158.0#

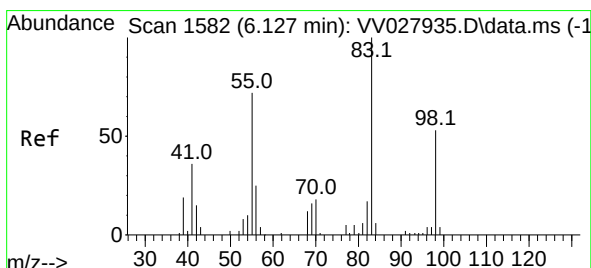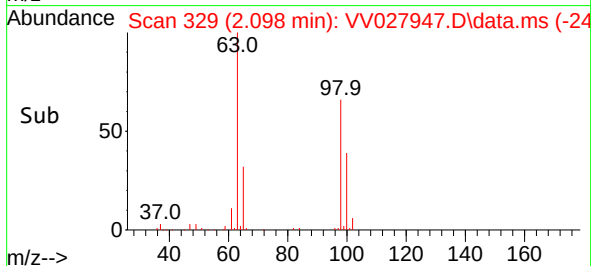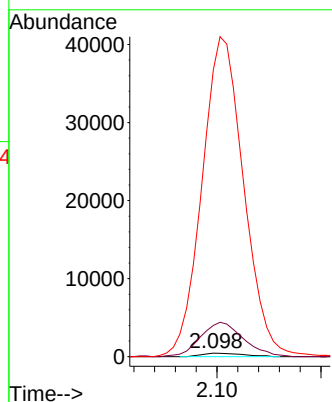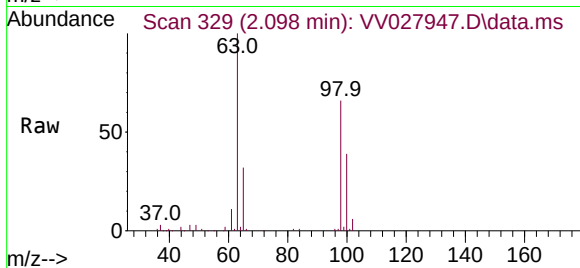

#35

Methylcyclohexane

Concen: 1.109 ug/L

RT: 6.063 min Scan# 1562




Delta R.T. -0.064 min


Lab File: VV027947.D

Acq: 20 Sep 2022 00:21

Tgt Ion: 83 Resp: 11112

Ion	Ratio	Lower	Upper
83	100		
55	0.0	54.5	81.7#
98	0.4	39.6	59.4#

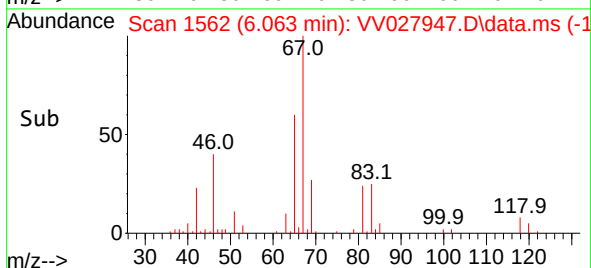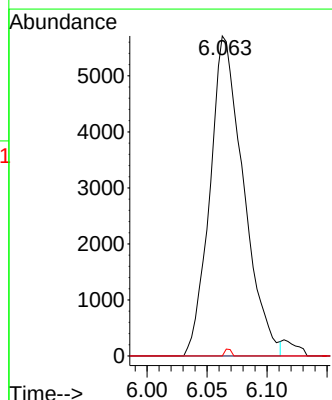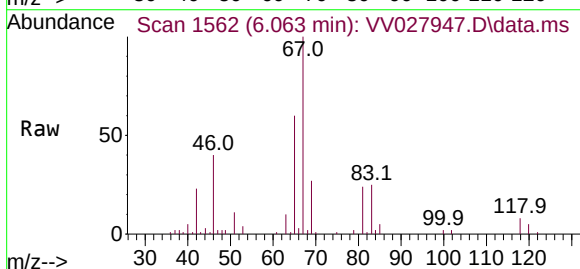

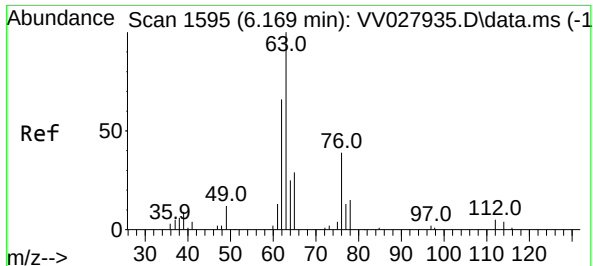

#37

1,2-Dichloropropane

Concen: 0.617 ug/L

RT: 6.066 min Scan# 1

Delta R.T. -0.103 min

Lab File: VV027947.D

Acq: 20 Sep 2022 00:21

Instrument :

MSVOA_V





ClientSampleId :

Tgt Ion: 63 Resp: 4670

Ion Ratio Lower Upper

63 100

112 0.0 3.8 5.8#

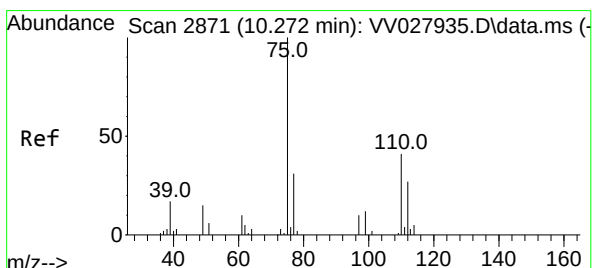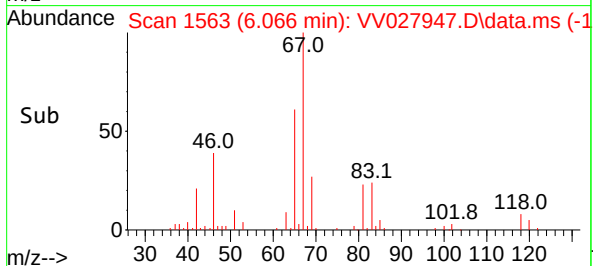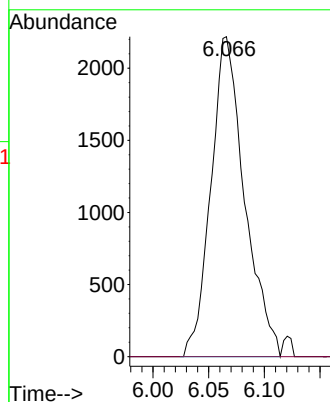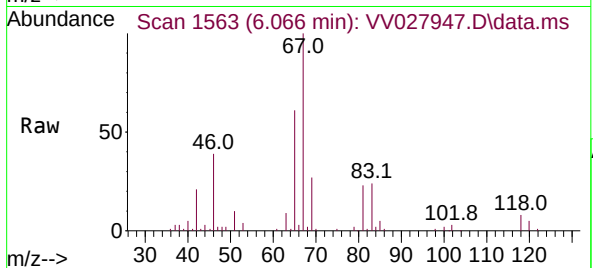

#61

1,2,3-Trichloropropane

Concen: 1.495 ug/L

RT: 11.249 min Scan# 3175

Delta R.T. 0.977 min

Lab File: VV027947.D

Acq: 20 Sep 2022 00:21




Tgt Ion: 75 Resp: 5784


Ion Ratio Lower Upper

75 100

77 34.6 26.1 39.1


110 0.0 31.3 46.9#

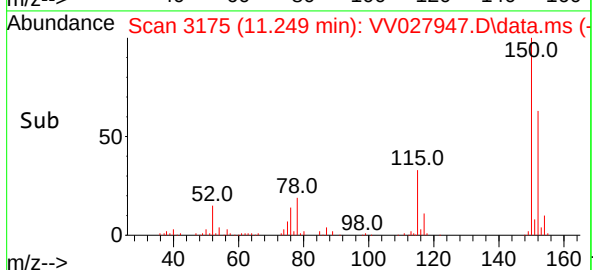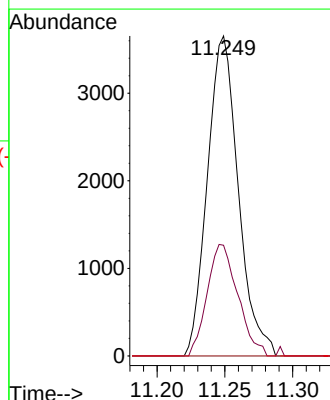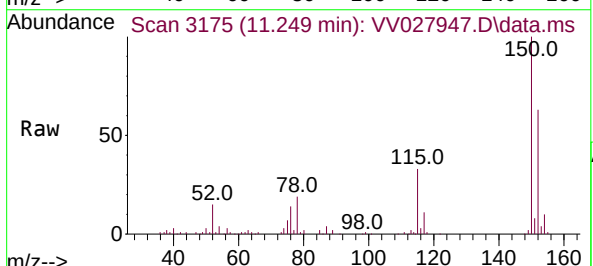

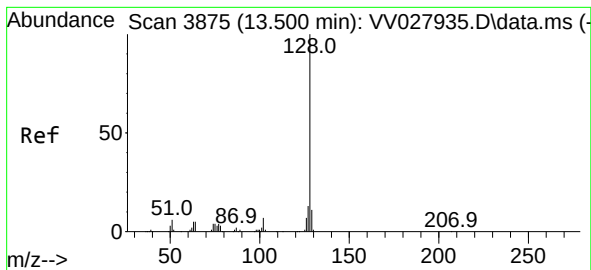

#71
Naphthalene
Concen: 0.228 ug/L
RT: 13.506 min Scan# 3877
Delta R.T. 0.006 min
Lab File: VV027947.D
Acq: 20 Sep 2022 00:21

Instrument :
MSVOA_V
ClientSampleId :

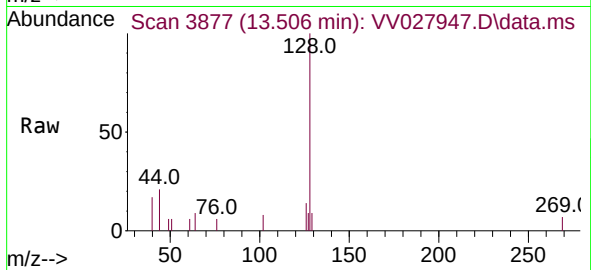

Tgt Ion:128 Resp: 3400
Ion Ratio Lower Upper
128 100
129 4.7 8.2 12.2#
127 3.3 10.2 15.2#

