

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027949.D
 Acq On : 20 Sep 2022 01:10
 Operator : SY/MD
 Sample : N4658-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED9

Quant Time: Sep 20 02:12:30 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Quant Title : TRACE VOA SFAM1.0
 QLast Update : Tue Sep 20 01:54:53 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	112861	5.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	105794	5.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	47280	5.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	45613	5.176	ug/L	0.00
Spiked Amount	5.000	Range 40 - 130	Recovery	=	103.600%	
7) Chloroethane-d5	1.565	69	40133	5.177	ug/L	0.00
Spiked Amount	5.000	Range 65 - 130	Recovery	=	103.600%	
11) 1,1-Dichloroethene-d2	2.105	63	56942	3.908	ug/L	0.00
Spiked Amount	5.000	Range 60 - 125	Recovery	=	78.200%	
20) 2-Butanone-d5	3.892	46	78669	55.869	ug/L	0.00
Spiked Amount	50.000	Range 40 - 130	Recovery	=	111.740%	
24) Chloroform-d	4.343	84	78359	5.311	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	106.200%	
26) 1,2-Dichloroethane-d4	5.031	65	34842	5.707	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	114.200%	
32) Benzene-d6	5.044	84	146510	5.840	ug/L	0.00
Spiked Amount	5.000	Range 70 - 125	Recovery	=	116.800%	
36) 1,2-Dichloropropane-d6	6.066	67	47563	5.775	ug/L	0.00
Spiked Amount	5.000	Range 60 - 140	Recovery	=	115.400%	
41) Toluene-d8	7.314	98	103821	4.611	ug/L	0.00
Spiked Amount	5.000	Range 70 - 130	Recovery	=	92.200%	
43) trans-1,3-Dichloroprop...	7.622	79	13088	4.798	ug/L	0.00
Spiked Amount	5.000	Range 55 - 130	Recovery	=	96.000%	
46) 2-Hexanone-d5	8.088	63	60512	50.240	ug/L	0.00
Spiked Amount	50.000	Range 45 - 130	Recovery	=	100.480%	
56) 1,1,2,2-Tetrachloroeth...	10.214	84	36255	5.381	ug/L	0.00
Spiked Amount	5.000	Range 65 - 120	Recovery	=	107.600%	
66) 1,2-Dichlorobenzene-d4	11.622	152	44030	5.983	ug/L	0.00
Spiked Amount	5.000	Range 80 - 120	Recovery	=	119.600%	
Target Compounds					Qvalue	
25) Chloroform	4.372	83	5070	0.322	ug/L	85


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027949.D
Acq On : 20 Sep 2022 01:10
Operator : SY/MD
Sample : N4658-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED9

Quant Time: Sep 20 02:12:30 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0
QLast Update : Tue Sep 20 01:54:53 2022
Response via : Initial Calibration

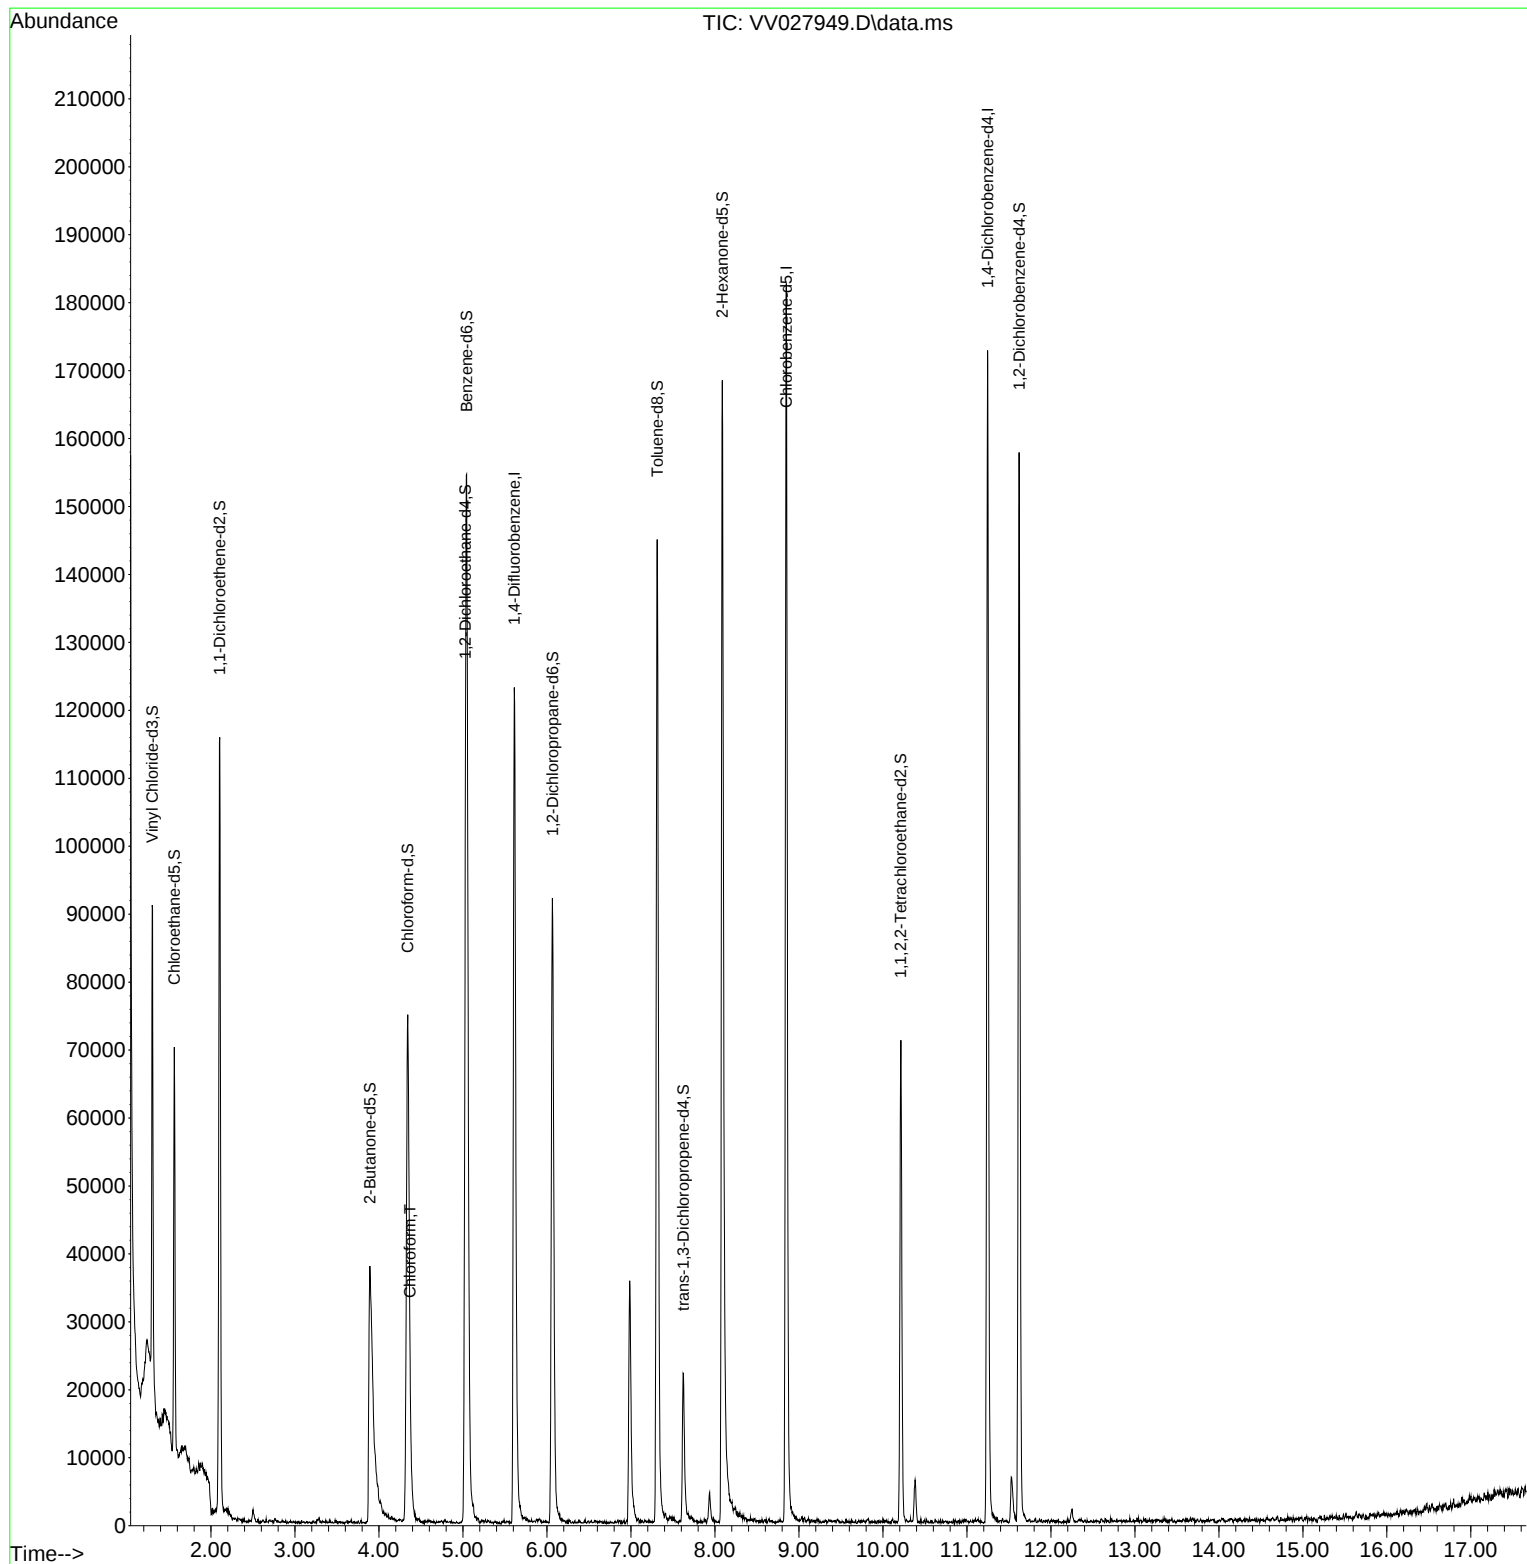

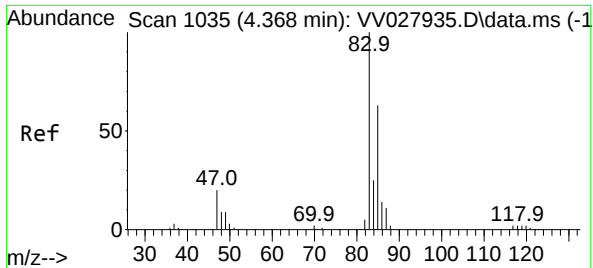

#25

Chloroform

Concen: 0.322 ug/L

RT: 4.372 min Scan# 10

Delta R.T. 0.003 min

Lab File: VV027949.D

Acq: 20 Sep 2022 01:10

Instrument :

MSVOA_V

ClientSampleId :

C0ED9

Tgt Ion: 83 Resp: 5070

Ion Ratio Lower Upper

83 100

85 74.5 44.0 81.8

