

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027936.D
 Acq On : 19 Sep 2022 19:49
 Operator : SY/MD
 Sample : VV0919WBL01
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK232

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027936.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	94	rVB	81908	94776	24.24%	2.890%
2	1.564	156	163	171	rVB	60198	65991	16.88%	2.012%
3	2.105	321	331	342	rBV2	118985	174764	44.70%	5.328%
4	2.503	444	455	463	rBV4	2491	4372	1.12%	0.133%
5	3.889	876	886	919	rBV2	44255	146766	37.54%	4.475%
6	4.342	1012	1027	1049	rBV	74627	185941	47.56%	5.669%
7	5.043	1228	1245	1271	rBV4	157686	390999	100.00%	11.921%
8	5.612	1411	1422	1456	rBV	125046	260437	66.61%	7.940%
9	6.066	1550	1563	1587	rBV2	93828	194150	49.65%	5.919%
10	6.664	1741	1749	1758	rBV4	2447	4535	1.16%	0.138%
11	6.985	1839	1849	1868	rBV	40880	76977	19.69%	2.347%
12	7.313	1940	1951	1974	rBV	168101	294666	75.36%	8.984%
13	7.622	2036	2047	2066	rBV	23691	44108	11.28%	1.345%
14	8.088	2182	2192	2221	rBV	187036	353317	90.36%	10.772%
15	8.850	2414	2429	2444	rBV	202240	323709	82.79%	9.869%
16	10.214	2839	2853	2868	rBV	71321	112114	28.67%	3.418%
17	10.381	2895	2905	2915	rBV2	4877	7330	1.87%	0.223%
18	11.246	3163	3174	3195	rBV	179336	280806	71.82%	8.561%
19	11.535	3255	3264	3272	rBV6	4644	8179	2.09%	0.249%
20	11.622	3280	3291	3307	rBV	164006	255964	65.46%	7.804%




Sum of corrected areas: 3279901

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027936.D
Acq On : 19 Sep 2022 19:49
Operator : SY/MD
Sample : VV0919WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

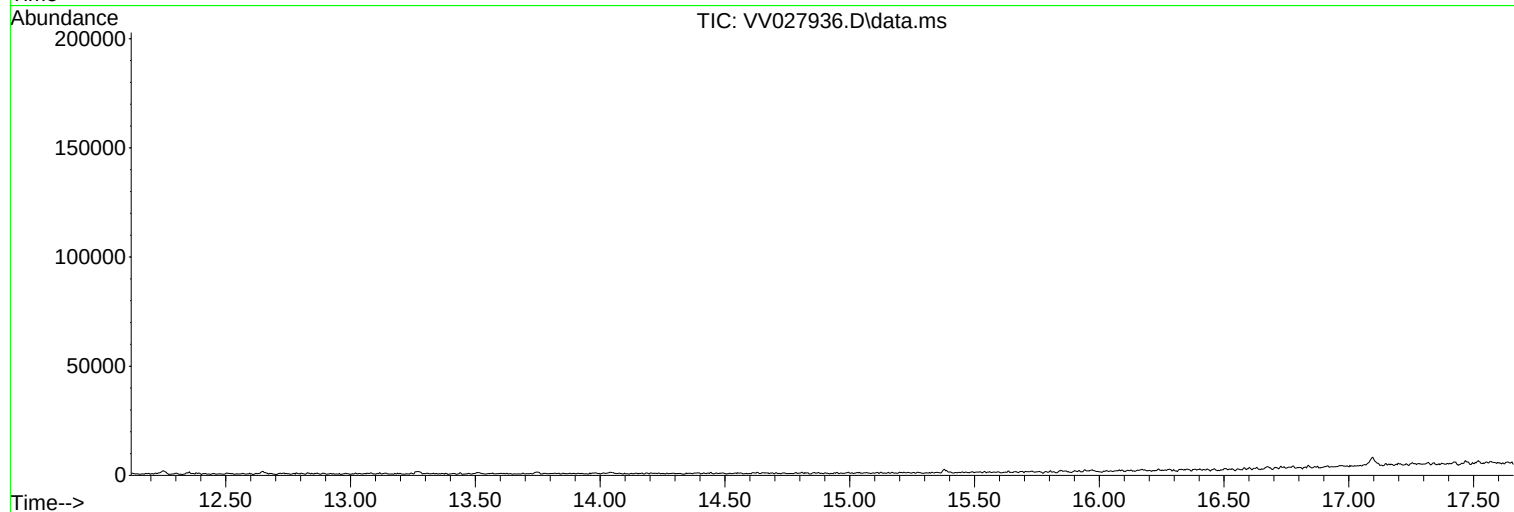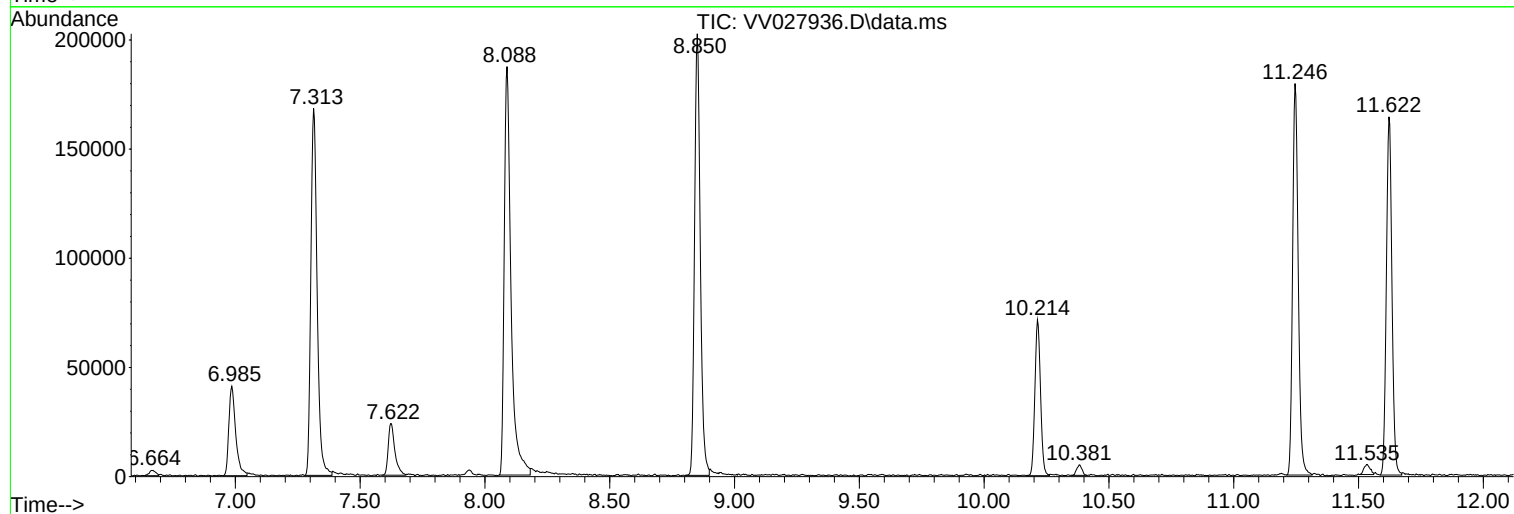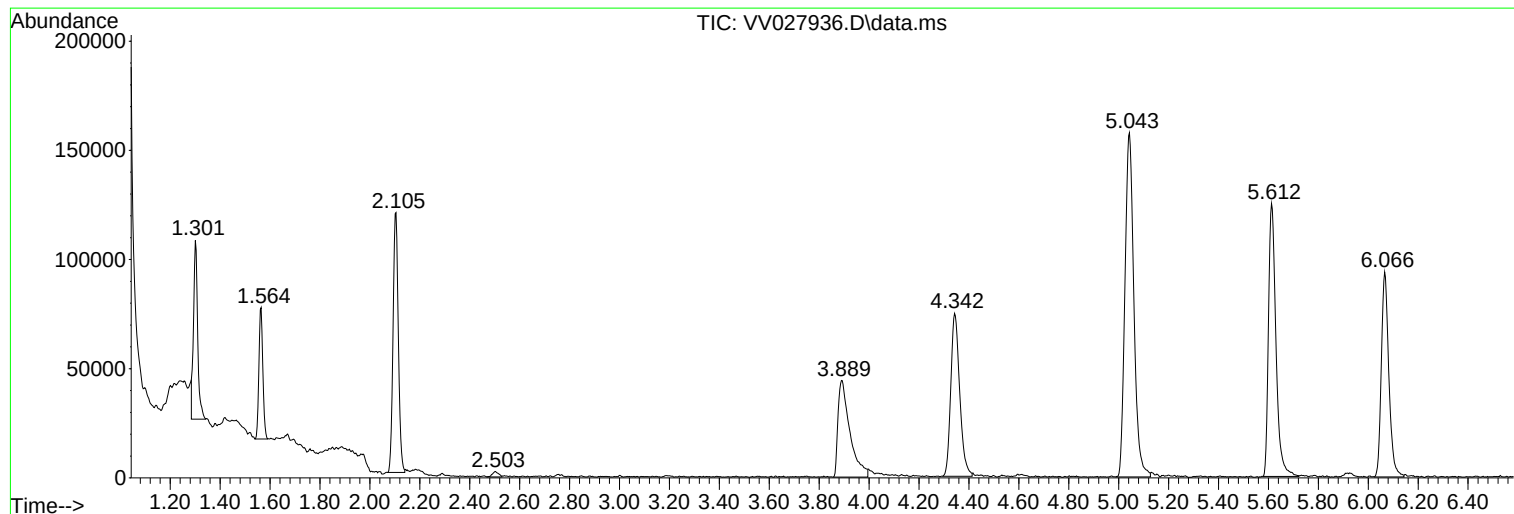

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027936.D
Acq On : 19 Sep 2022 19:49
Operator : SY/MD
Sample : VV0919WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027936.D
Acq On : 19 Sep 2022 19:49
Operator : SY/MD
Sample : VV0919WBL01
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK232

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc