

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027937.D
 Acq On : 19 Sep 2022 20:14
 Operator : SY/MD
 Sample : N4618-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027937.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	91	rVB	79841	85835	21.82%	2.593%
2	1.561	156	162	175	rVB	63254	73474	18.68%	2.220%
3	2.101	316	330	345	rBV	119250	171517	43.61%	5.182%
4	2.500	446	454	465	rBV5	4252	6991	1.78%	0.211%
5	3.889	875	886	908	rBV2	39656	121072	30.78%	3.658%
6	4.342	1011	1027	1050	rBV3	69634	175364	44.59%	5.298%
7	5.043	1229	1245	1266	rBV2	158331	393311	100.00%	11.883%
8	5.612	1410	1422	1445	rBV	120347	251817	64.02%	7.608%
9	6.066	1550	1563	1587	rBV2	91770	195148	49.62%	5.896%
10	6.985	1839	1849	1866	rBV	42023	77815	19.78%	2.351%
11	7.313	1940	1951	1970	rBV	176200	310336	78.90%	9.376%
12	7.622	2036	2047	2065	rBV2	25843	46199	11.75%	1.396%
13	7.937	2137	2145	2157	rVB2	6685	11241	2.86%	0.340%
14	8.088	2182	2192	2217	rBV	198302	367598	93.46%	11.106%
15	8.850	2418	2429	2448	rBV	202156	332629	84.57%	10.049%
16	10.213	2842	2853	2869	rBV	71794	113964	28.98%	3.443%
17	10.381	2895	2905	2915	rBV	10527	18394	4.68%	0.556%
18	11.249	3163	3175	3190	rBV	179011	279225	70.99%	8.436%
19	11.529	3255	3262	3273	rBV8	7060	13474	3.43%	0.407%
20	11.622	3280	3291	3307	rBV	166682	264508	67.25%	7.991%




Sum of corrected areas: 3309912

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027937.D
Acq On : 19 Sep 2022 20:14
Operator : SY/MD
Sample : N4618-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

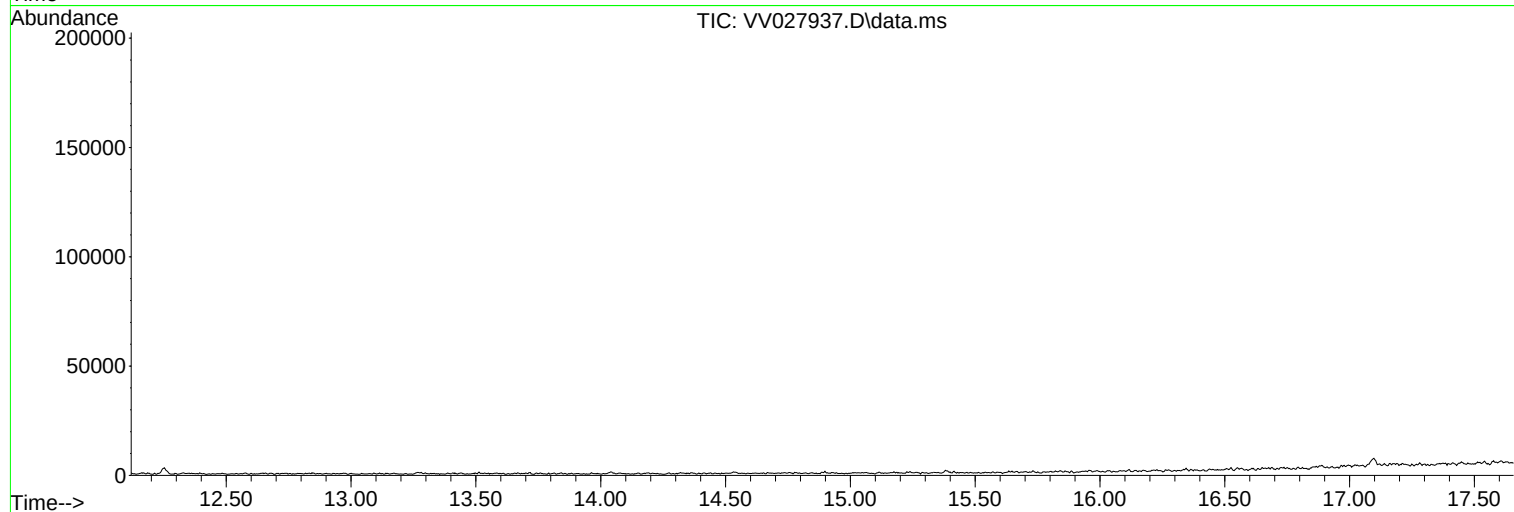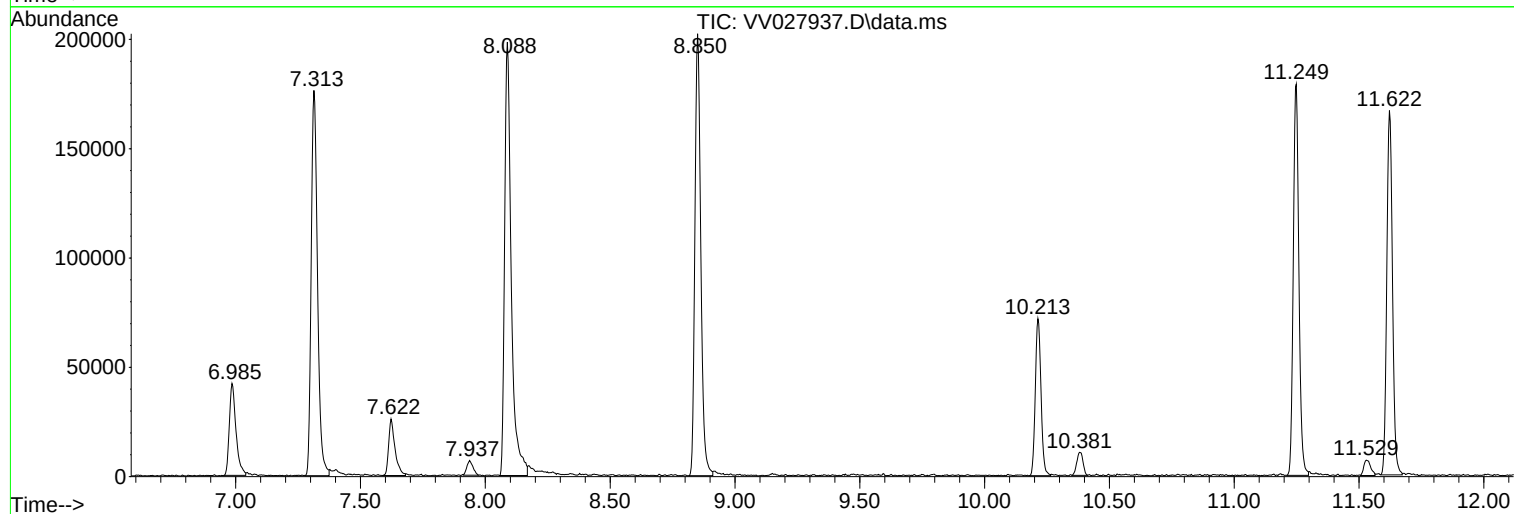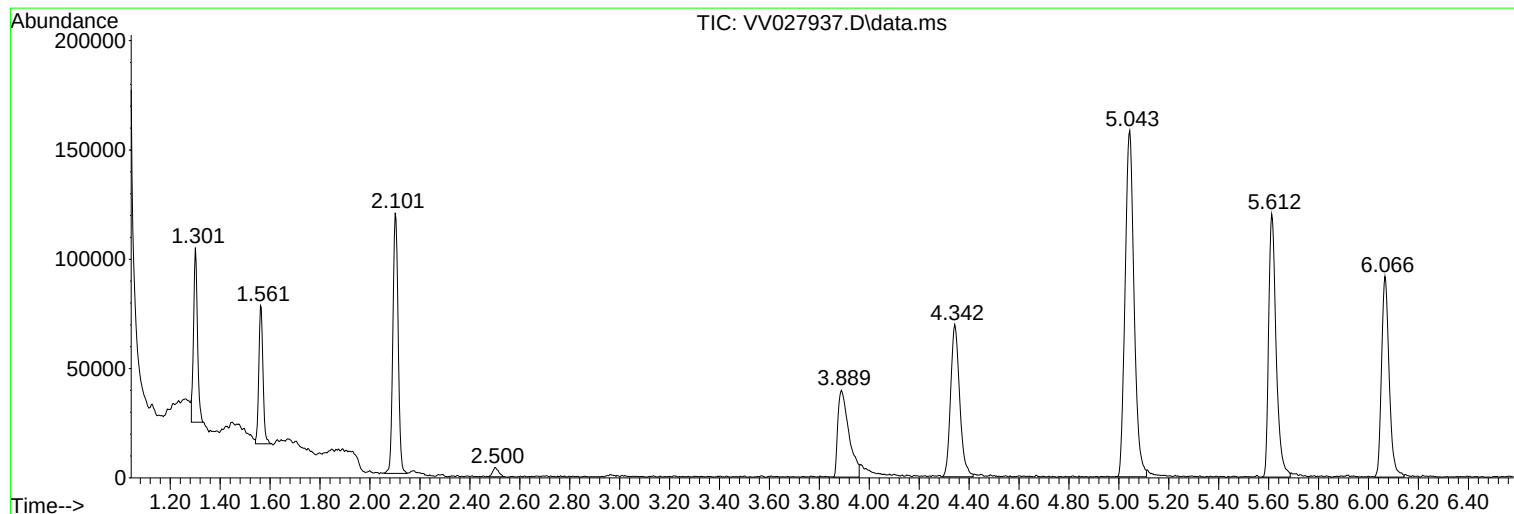

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027937.D
Acq On : 19 Sep 2022 20:14
Operator : SY/MD
Sample : N4618-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027937.D
Acq On : 19 Sep 2022 20:14
Operator : SY/MD
Sample : N4618-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
