

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027939.D
 Acq On : 19 Sep 2022 21:03
 Operator : SY/MD
 Sample : N4658-05
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E84

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027939.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	96	rVB2	80045	95469	24.64%	2.860%
2	1.564	156	163	173	rVB	59417	70192	18.12%	2.103%
3	2.101	319	330	345	rVB	116871	164937	42.57%	4.941%
4	2.503	446	455	466	rVB7	2021	4174	1.08%	0.125%
5	3.892	875	887	911	rBV	37166	126910	32.76%	3.802%
6	4.342	1010	1027	1050	rBV2	72812	187321	48.35%	5.611%
7	5.043	1228	1245	1276	rBV2	153703	387427	100.00%	11.605%
8	5.613	1410	1422	1445	rBV	123291	253406	65.41%	7.591%
9	6.066	1548	1563	1585	rBV	91482	191520	49.43%	5.737%
10	6.985	1836	1849	1868	rBV	38385	75633	19.52%	2.266%
11	7.313	1939	1951	1970	rBV	164278	291144	75.15%	8.721%
12	7.622	2036	2047	2067	rBV2	23322	44809	11.57%	1.342%
13	7.937	2135	2145	2154	rBV2	8437	14203	3.67%	0.425%
14	8.088	2182	2192	2219	rBV	185537	354361	91.47%	10.615%
15	8.850	2417	2429	2454	rBV	204357	335951	86.71%	10.063%
16	10.214	2843	2853	2866	rBV	75101	119019	30.72%	3.565%
17	10.381	2894	2905	2917	rVB2	14343	23269	6.01%	0.697%
18	11.246	3163	3174	3194	rBV	195128	308861	79.72%	9.252%
19	11.535	3254	3264	3272	rBV7	4742	8419	2.17%	0.252%
20	11.622	3279	3291	3307	rBV	172179	275214	71.04%	8.244%
21	12.252	3472	3487	3495	rBV2	3498	6167	1.59%	0.185%




Sum of corrected areas: 3338406

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027939.D
Acq On : 19 Sep 2022 21:03
Operator : SY/MD
Sample : N4658-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

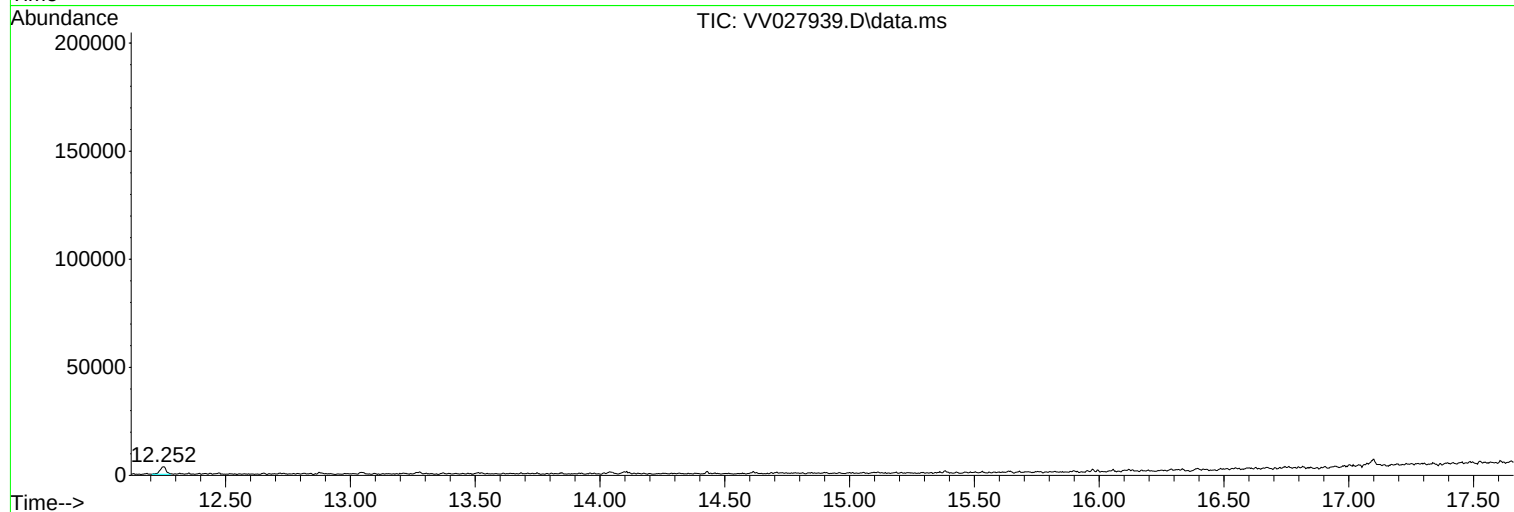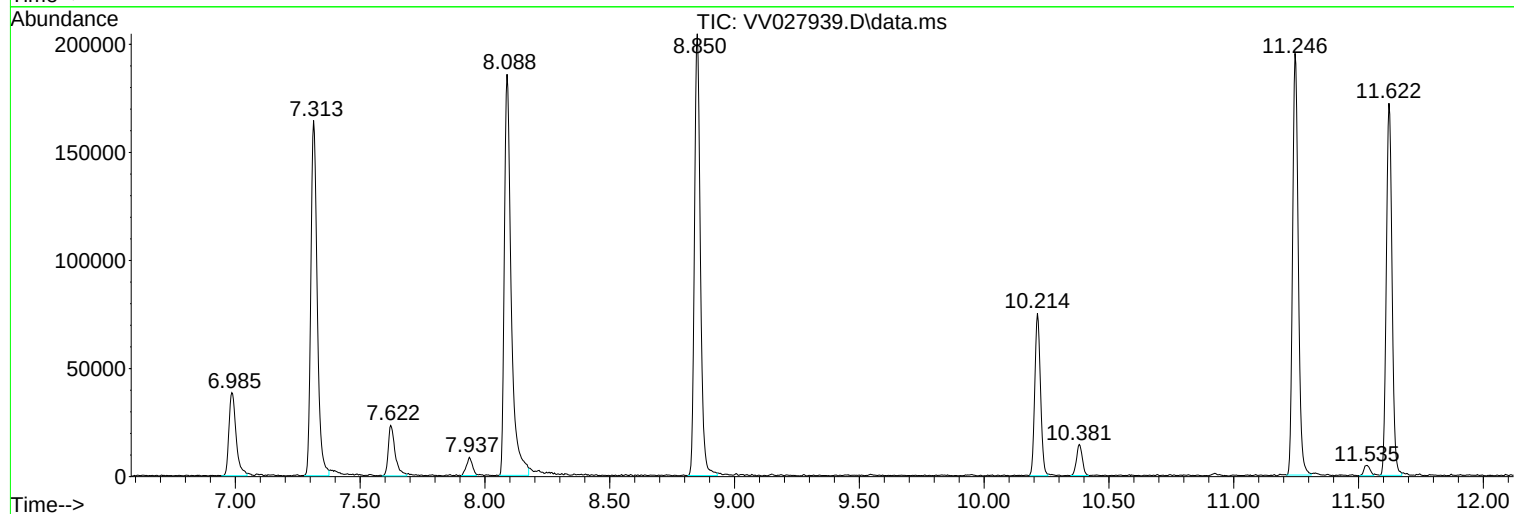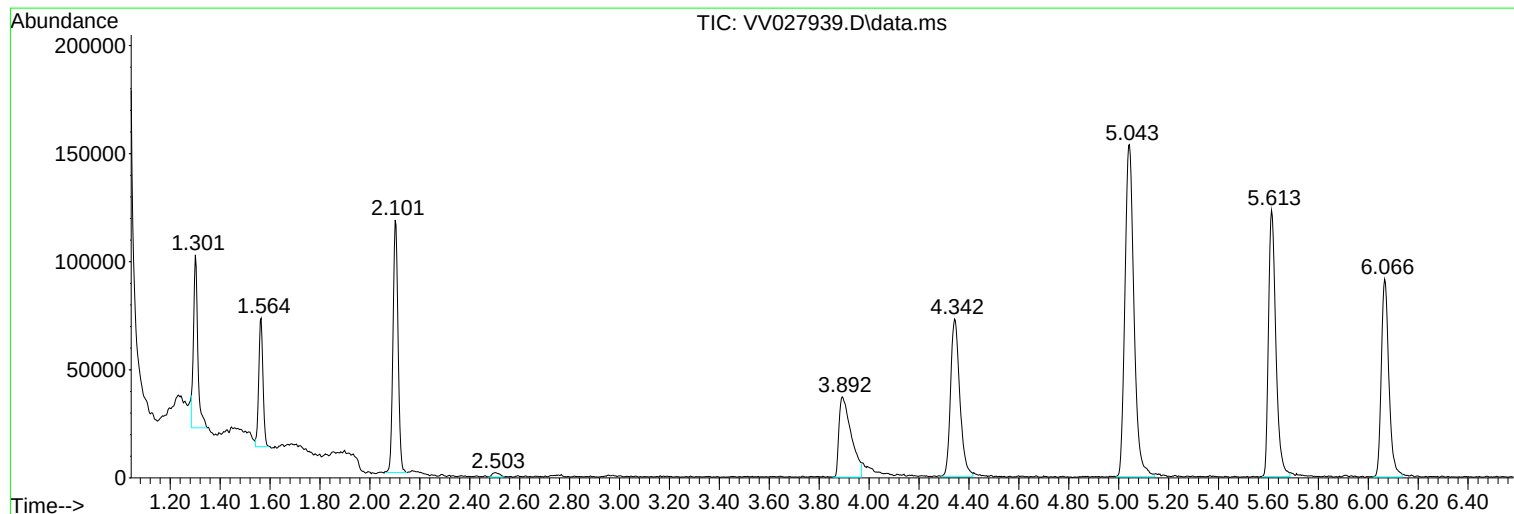

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027939.D
Acq On : 19 Sep 2022 21:03
Operator : SY/MD
Sample : N4658-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027939.D
Acq On : 19 Sep 2022 21:03
Operator : SY/MD
Sample : N4658-05
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E84

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
