

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027940.D
 Acq On : 19 Sep 2022 21:28
 Operator : SY/MD
 Sample : N4658-06
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E87

Integration Parameters: rteint.p
 Integrator: RTE
 Smoothing : ON Filtering: 5
 Sampling : 1 Min Area: 3 % of largest Peak
 Start Thrs: 0.1 Max Peaks: 100
 Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
 Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027940.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	81403	92241	24.31%	2.849%
2	1.564	156	163	173	rBV	59119	67244	17.72%	2.077%
3	2.101	320	330	349	rVB	114148	164360	43.32%	5.076%
4	2.500	448	454	466	rVB7	2725	4557	1.20%	0.141%
5	3.889	873	886	912	rBV2	40044	128936	33.98%	3.982%
6	4.342	1012	1027	1051	rBV2	71424	173991	45.85%	5.374%
7	5.043	1230	1245	1268	rBV2	152508	379447	100.00%	11.719%
8	5.612	1411	1422	1441	rBV	124093	249888	65.86%	7.718%
9	6.066	1551	1563	1587	rBV2	90257	188593	49.70%	5.825%
10	6.985	1838	1849	1868	rBV2	39175	75195	19.82%	2.322%
11	7.313	1940	1951	1974	rBV	159645	284196	74.90%	8.777%
12	7.625	2038	2048	2064	rBV2	23452	42759	11.27%	1.321%
13	7.940	2135	2146	2155	rBV4	6206	11021	2.90%	0.340%
14	8.088	2182	2192	2218	rBV	181297	345660	91.10%	10.675%
15	8.850	2419	2429	2450	rBV	201807	329261	86.77%	10.169%
16	10.214	2842	2853	2865	rBV2	74076	115775	30.51%	3.576%
17	10.384	2895	2906	2918	rBV3	6365	11099	2.93%	0.343%
18	11.246	3164	3174	3196	rBV	196712	302585	79.74%	9.345%
19	11.622	3280	3291	3311	rBV2	169944	271106	71.45%	8.373%




Sum of corrected areas: 3237914

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027940.D
Acq On : 19 Sep 2022 21:28
Operator : SY/MD
Sample : N4658-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

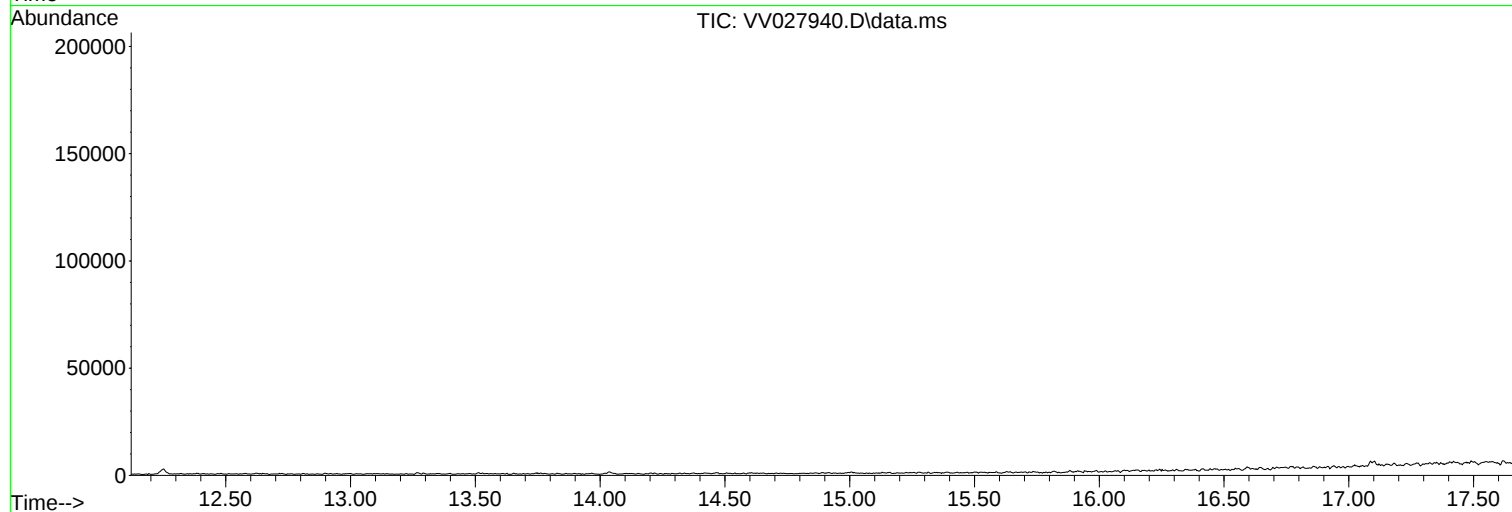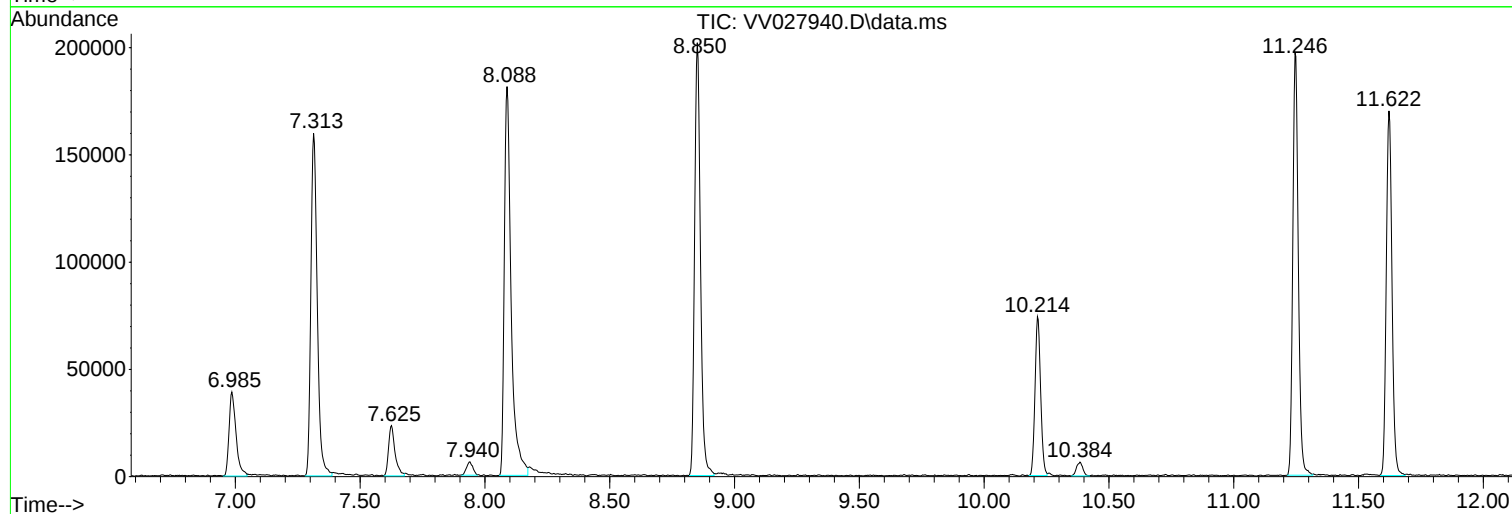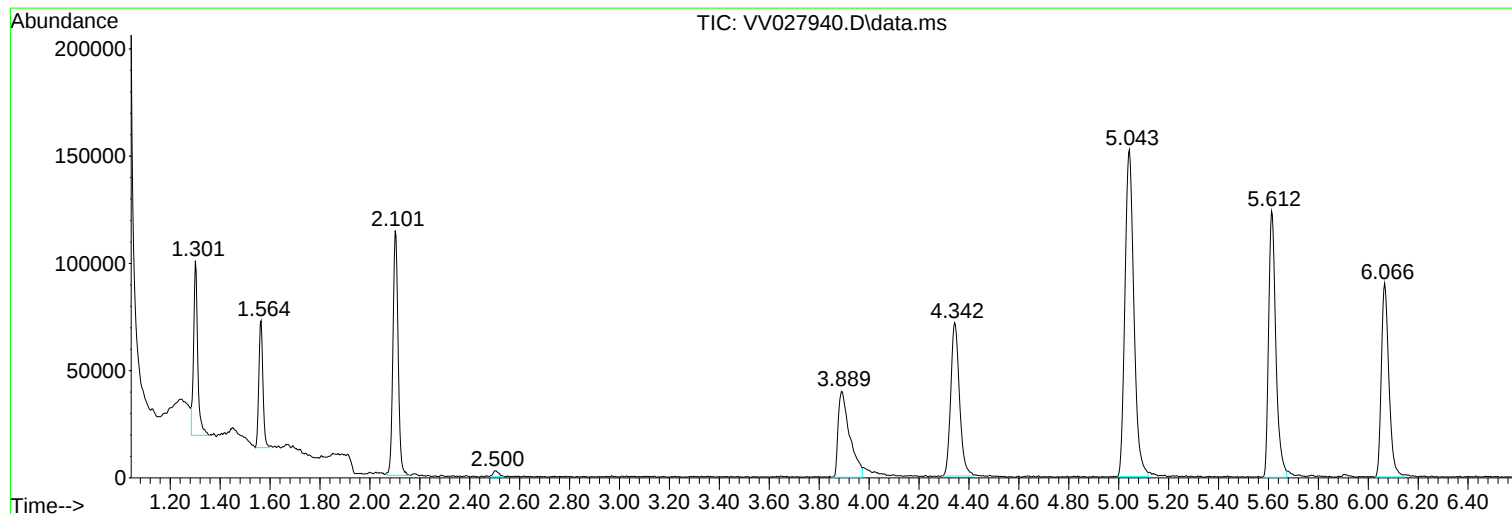

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027940.D
Acq On : 19 Sep 2022 21:28
Operator : SY/MD
Sample : N4658-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027940.D
Acq On : 19 Sep 2022 21:28
Operator : SY/MD
Sample : N4658-06
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E87

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc