

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027942.D
 Acq On : 19 Sep 2022 22:18
 Operator : SY/MD
 Sample : N4658-08
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E93

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027942.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	104	rVB2	81592	103012	27.43%	3.182%
2	1.564	156	163	173	rVB	60261	67902	18.08%	2.097%
3	2.101	321	330	343	rBV	111115	157234	41.87%	4.857%
4	3.889	877	886	920	rBV2	40249	135073	35.97%	4.172%
5	4.342	1010	1027	1050	rBV2	70359	172990	46.07%	5.344%
6	5.043	1228	1245	1272	rBV2	150806	375527	100.00%	11.600%
7	5.613	1410	1422	1448	rBV	123651	251727	67.03%	7.776%
8	6.066	1549	1563	1582	rBV	91390	187573	49.95%	5.794%
9	6.985	1838	1849	1871	rBV	38485	73571	19.59%	2.273%
10	7.313	1937	1951	1972	rBV	157247	278181	74.08%	8.593%
11	7.622	2037	2047	2069	rBV2	22712	42981	11.45%	1.328%
12	7.940	2134	2146	2157	rBV3	5302	9916	2.64%	0.306%
13	8.088	2182	2192	2220	rBV	178217	340232	90.60%	10.510%
14	8.850	2418	2429	2448	rBV	201392	325499	86.68%	10.054%
15	10.214	2841	2853	2873	rBV	73711	116760	31.09%	3.607%
16	10.384	2895	2906	2918	rBV2	8251	14491	3.86%	0.448%
17	11.246	3164	3174	3192	rBV	195974	304146	80.99%	9.395%
18	11.532	3255	3263	3272	rBV3	4451	7956	2.12%	0.246%
19	11.622	3280	3291	3314	rVB	168971	267604	71.26%	8.266%
20	12.249	3477	3486	3494	rBV3	3100	4985	1.33%	0.154%




Sum of corrected areas: 3237360

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027942.D
Acq On : 19 Sep 2022 22:18
Operator : SY/MD
Sample : N4658-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

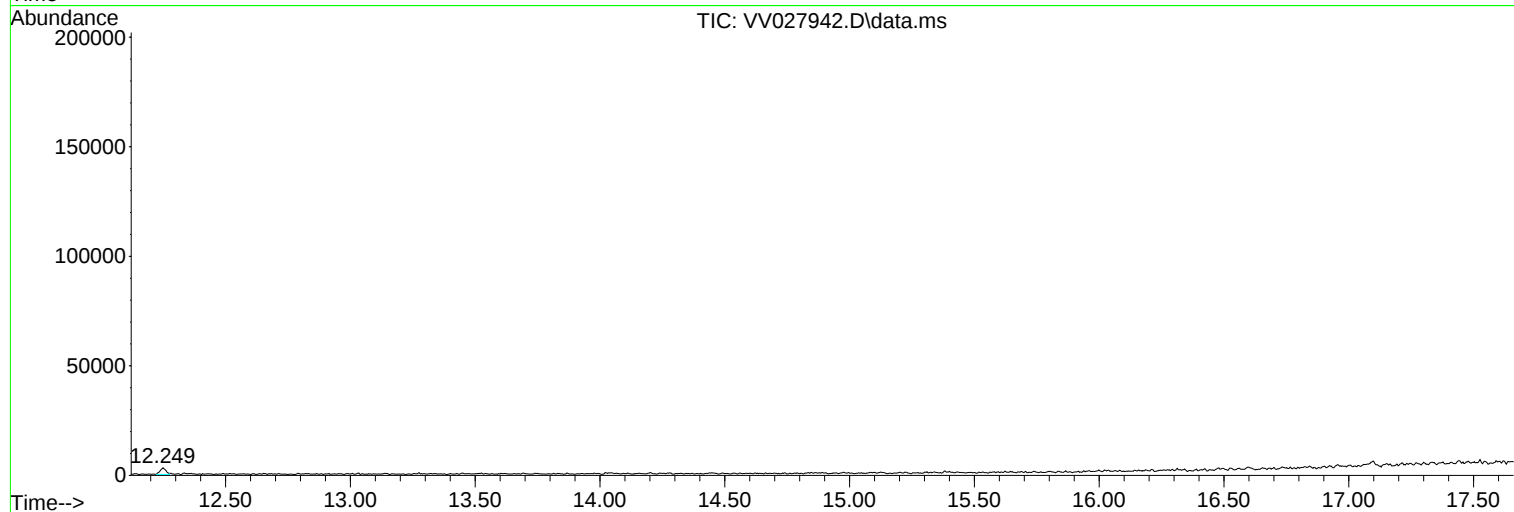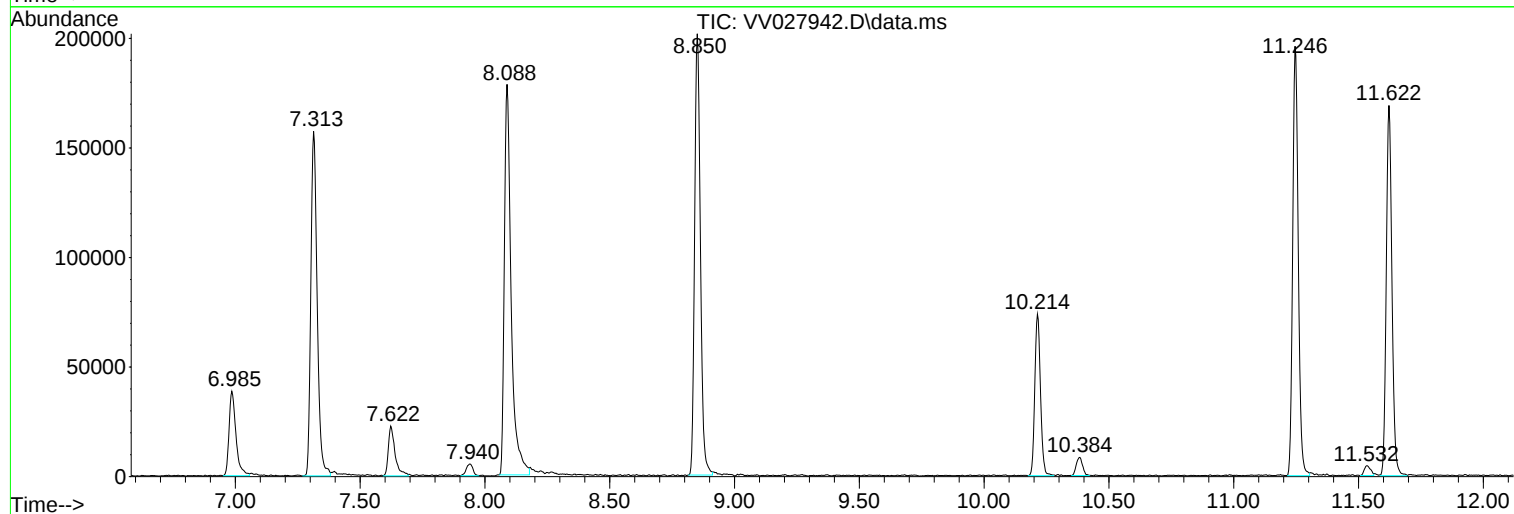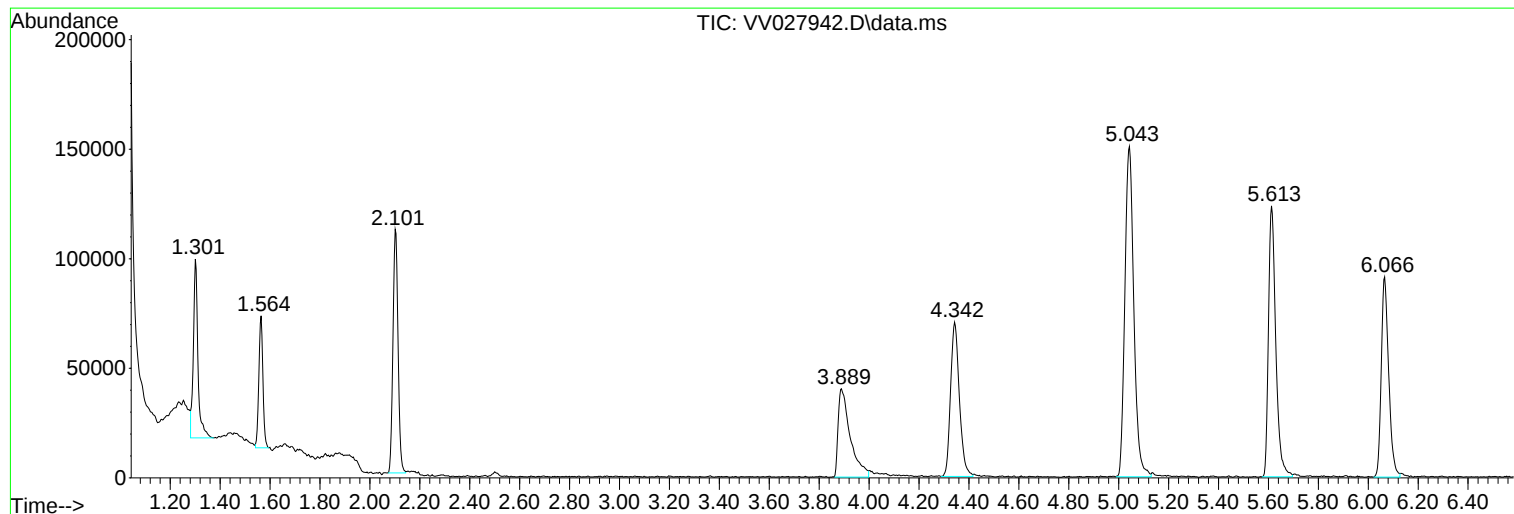

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027942.D
Acq On : 19 Sep 2022 22:18
Operator : SY/MD
Sample : N4658-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027942.D
Acq On : 19 Sep 2022 22:18
Operator : SY/MD
Sample : N4658-08
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E93

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
