

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027943.D
 Acq On : 19 Sep 2022 22:42
 Operator : SY/MD
 Sample : N4658-09
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E96

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027943.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	96	rVB	78173	92486	24.91%	2.900%
2	1.561	156	162	174	rVB	57594	68861	18.54%	2.159%
3	2.101	319	330	346	rBV	107714	156419	42.12%	4.905%
4	2.503	448	455	467	rBV7	2354	3894	1.05%	0.122%
5	3.889	876	886	919	rBV2	37879	126928	34.18%	3.980%
6	4.343	1012	1027	1047	rBV	69621	172268	46.39%	5.402%
7	5.040	1229	1244	1275	rBV2	149131	371345	100.00%	11.644%
8	5.613	1410	1422	1453	rBV	120673	251798	67.81%	7.896%
9	6.066	1550	1563	1584	rBV2	86734	185167	49.86%	5.806%
10	6.986	1839	1849	1874	rBV2	36388	70019	18.86%	2.196%
11	7.313	1940	1951	1974	rBV	155427	276092	74.35%	8.657%
12	7.622	2039	2047	2059	rBV2	22486	39365	10.60%	1.234%
13	7.944	2138	2147	2158	rVB2	4704	8346	2.25%	0.262%
14	8.088	2180	2192	2221	rBV	176965	339805	91.51%	10.655%
15	8.850	2418	2429	2451	rBV	201565	328775	88.54%	10.309%
16	10.214	2841	2853	2871	rBV	73258	117069	31.53%	3.671%
17	10.381	2894	2905	2916	rBV4	8970	14365	3.87%	0.450%
18	11.246	3164	3174	3192	rBV	189723	297739	80.18%	9.336%
19	11.538	3255	3265	3273	rBV6	3936	6804	1.83%	0.213%
20	11.622	3280	3291	3312	rBV2	164873	261514	70.42%	8.200%




Sum of corrected areas: 3189059

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027943.D
Acq On : 19 Sep 2022 22:42
Operator : SY/MD
Sample : N4658-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

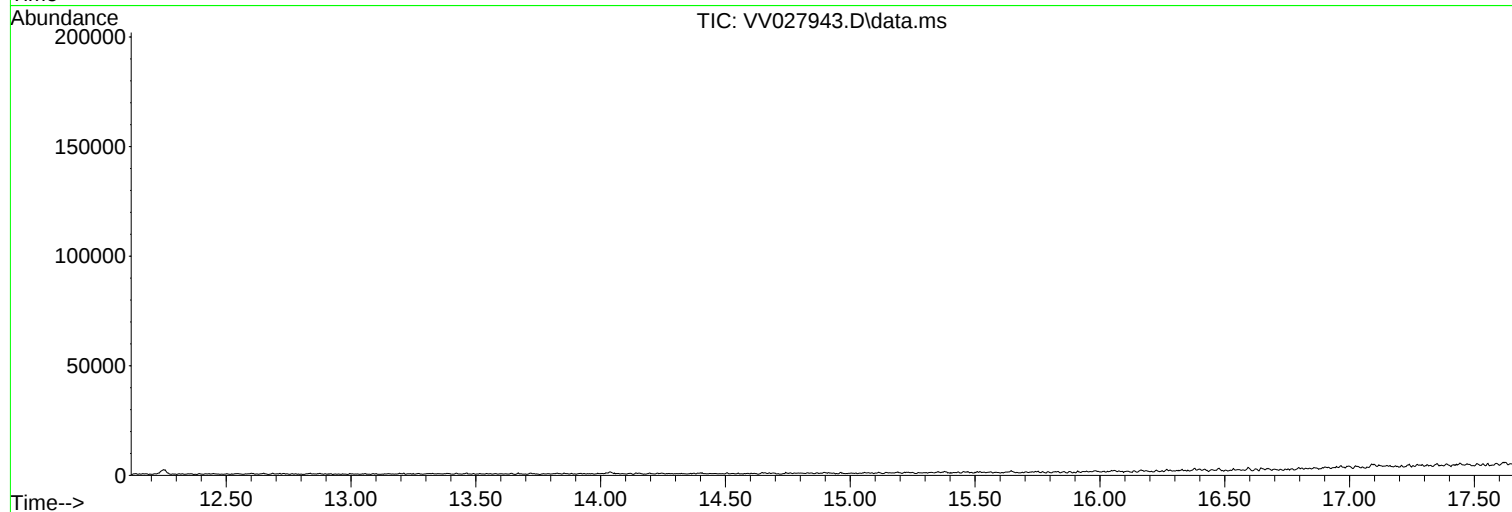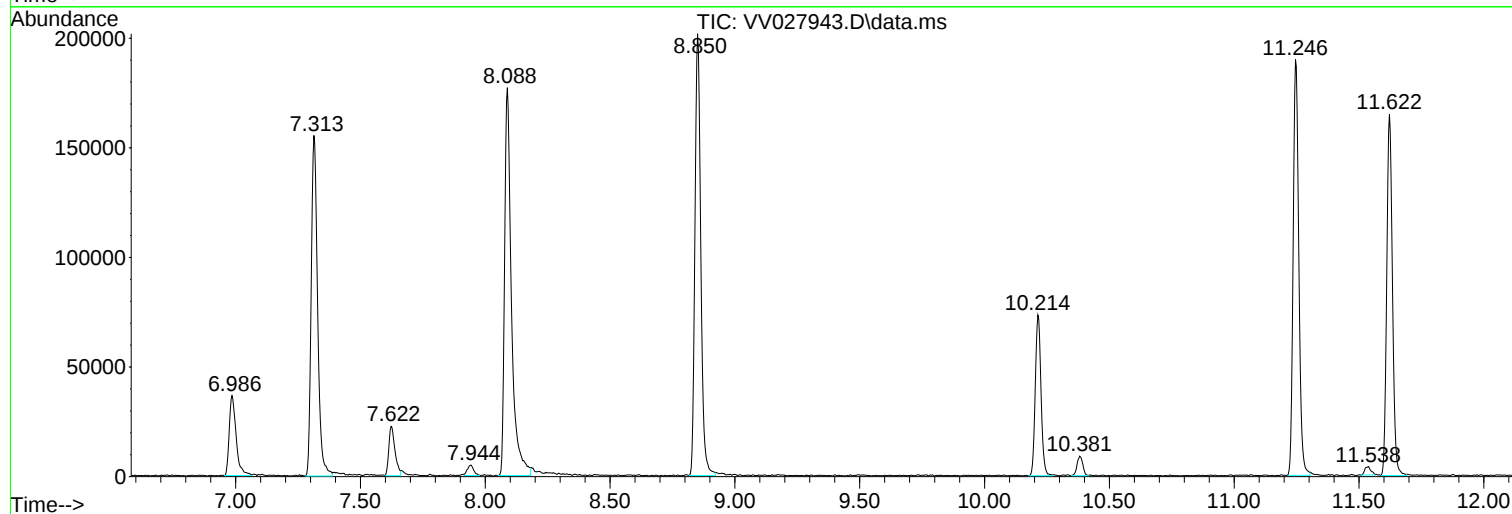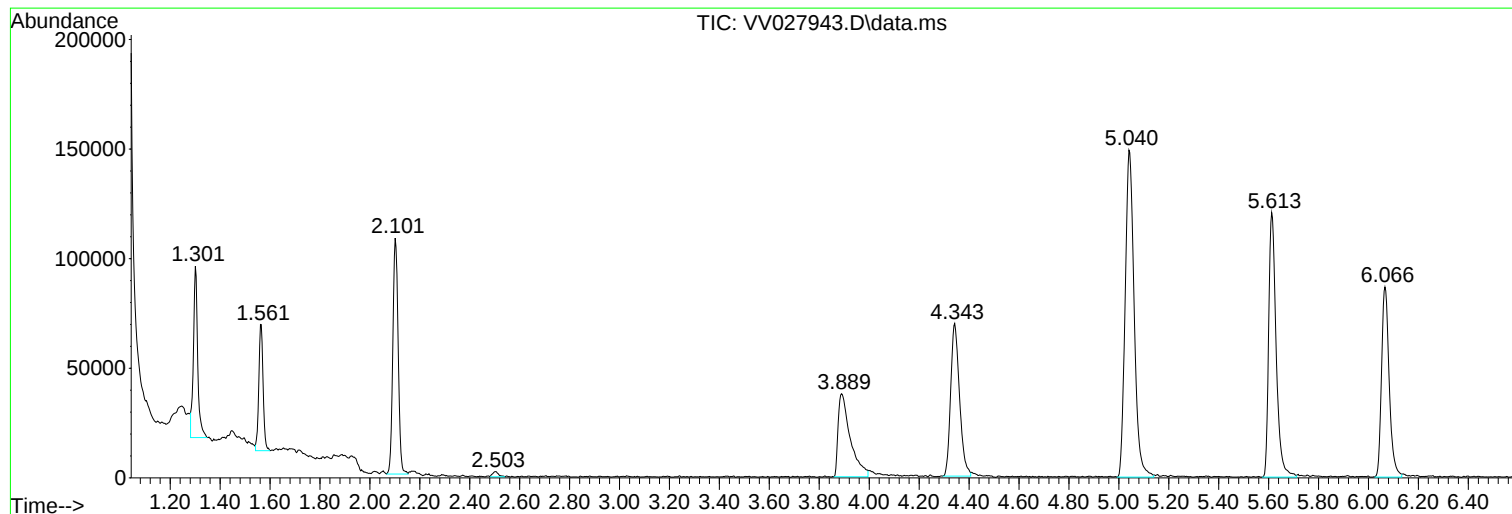

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027943.D
Acq On : 19 Sep 2022 22:42
Operator : SY/MD
Sample : N4658-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027943.D
Acq On : 19 Sep 2022 22:42
Operator : SY/MD
Sample : N4658-09
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E96

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc