

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027944.D
 Acq On : 19 Sep 2022 23:07
 Operator : SY/MD
 Sample : N4658-10
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E99

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027944.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	95	rVB	75477	87286	25.44%	2.904%
2	1.565	156	163	173	rVB	58252	67926	19.80%	2.260%
3	2.102	319	330	342	rBV	109710	156535	45.63%	5.208%
4	2.497	448	453	465	rVB7	2082	3558	1.04%	0.118%
5	3.892	877	887	913	rBV2	33331	116656	34.00%	3.881%
6	4.343	1012	1027	1050	rBV2	63558	161786	47.16%	5.382%
7	5.044	1229	1245	1269	rBV3	138374	343063	100.00%	11.413%
8	5.613	1411	1422	1443	rBV	111484	228711	66.67%	7.609%
9	6.066	1550	1563	1584	rBV2	81725	172069	50.16%	5.725%
10	6.986	1839	1849	1864	rBV2	35576	67220	19.59%	2.236%
11	7.314	1940	1951	1977	rBV	152601	275853	80.41%	9.177%
12	7.625	2036	2048	2062	rBV3	20866	38760	11.30%	1.290%
13	7.941	2135	2146	2153	rBV3	3311	5234	1.53%	0.174%
14	8.088	2178	2192	2219	rBV	174510	334925	97.63%	11.143%
15	8.850	2418	2429	2448	rBV	186872	306158	89.24%	10.186%
16	10.214	2841	2853	2867	rBV	68666	108309	31.57%	3.603%
17	10.384	2896	2906	2917	rVB3	5363	8874	2.59%	0.295%
18	11.249	3164	3175	3194	rBV	174032	272780	79.51%	9.075%
19	11.532	3257	3263	3279	rVB7	4149	7544	2.20%	0.251%
20	11.622	3279	3291	3311	rBV	149169	238663	69.57%	7.940%
21	12.252	3474	3487	3493	rBV5	2013	3904	1.14%	0.130%




Sum of corrected areas: 3005814

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027944.D
Acq On : 19 Sep 2022 23:07
Operator : SY/MD
Sample : N4658-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

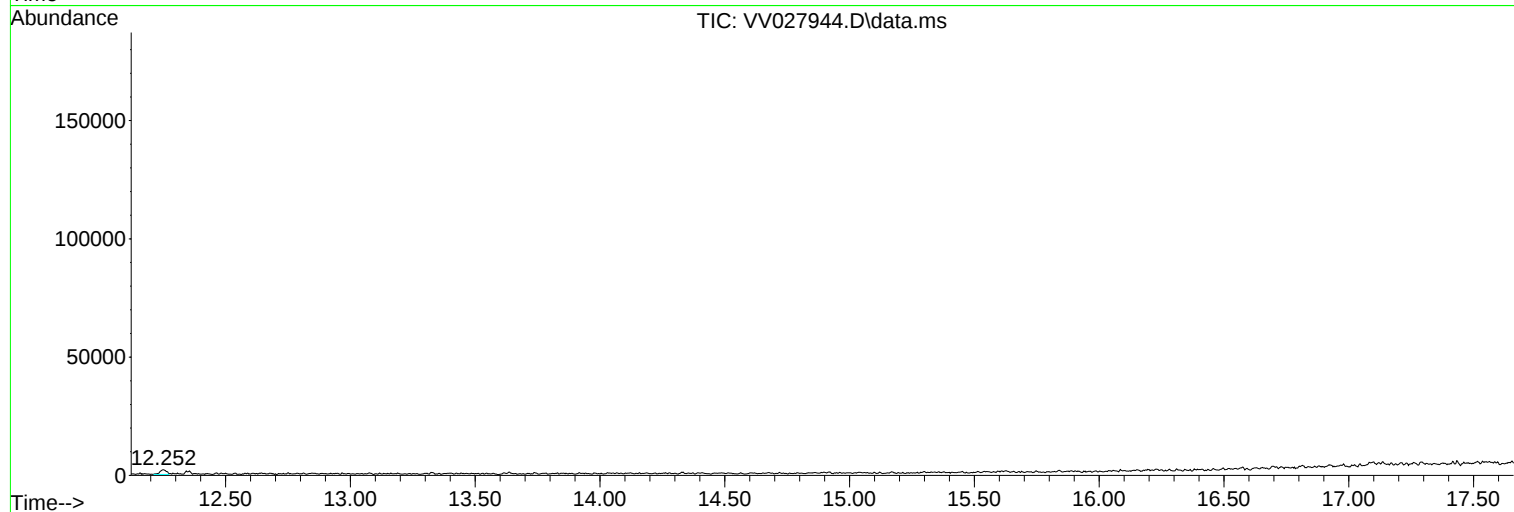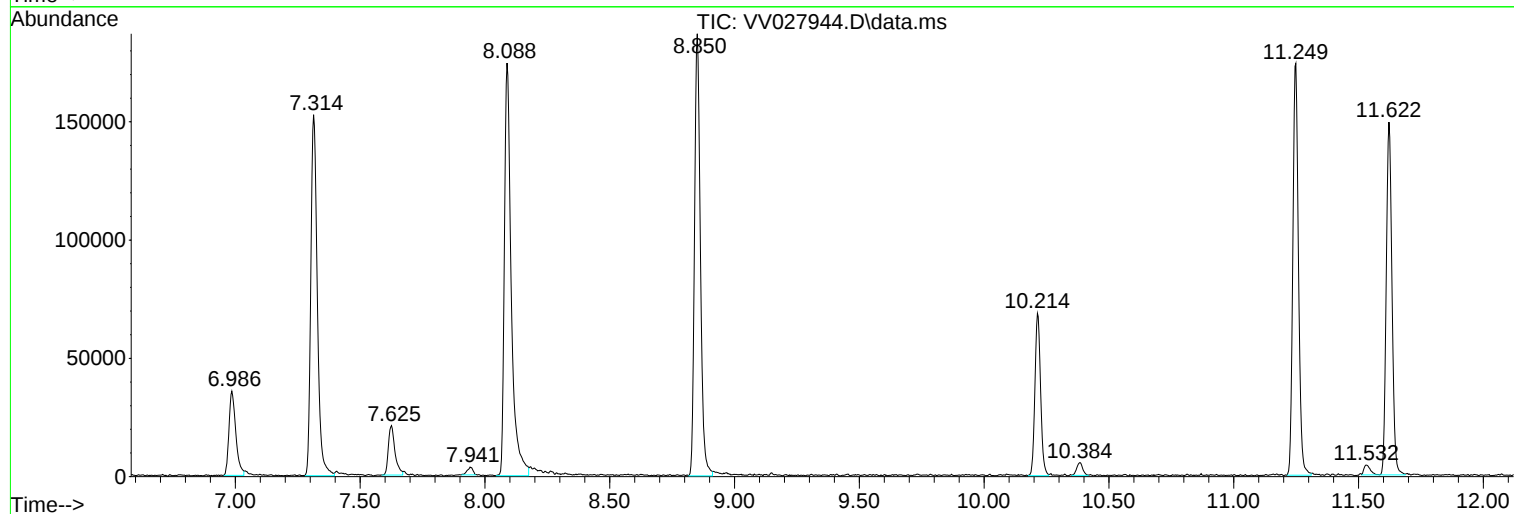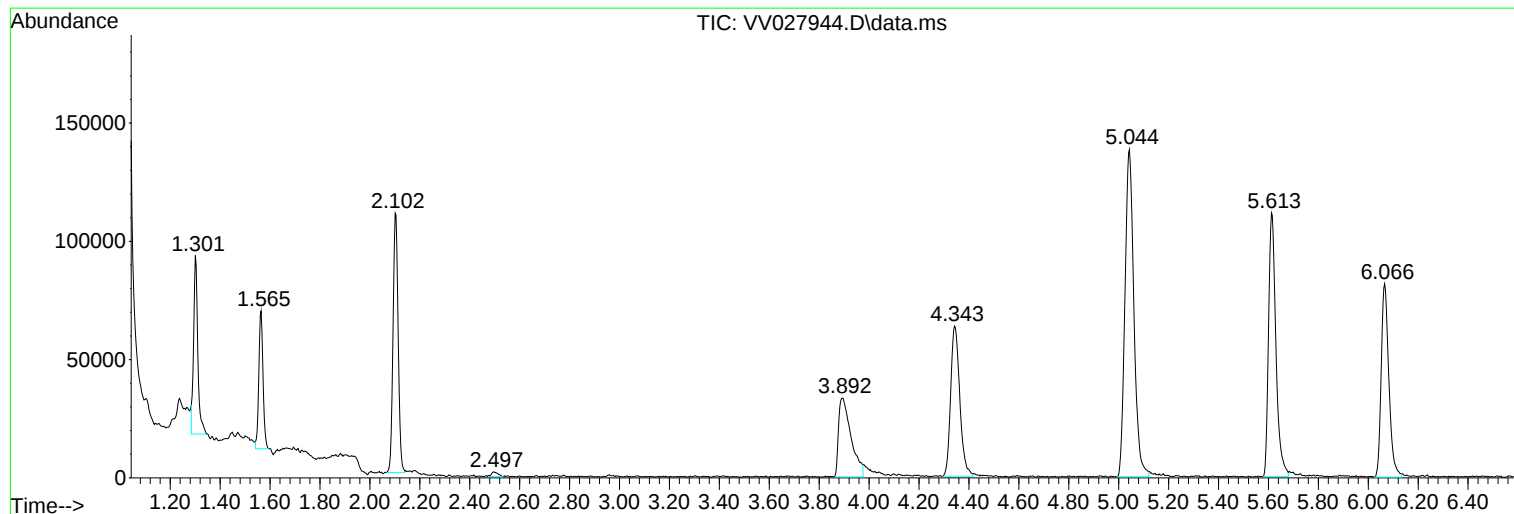

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027944.D
Acq On : 19 Sep 2022 23:07
Operator : SY/MD
Sample : N4658-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027944.D
Acq On : 19 Sep 2022 23:07
Operator : SY/MD
Sample : N4658-10
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E99

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc