

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027948.D
 Acq On : 20 Sep 2022 00:46
 Operator : SY/MD
 Sample : N4658-14
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED8

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027948.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	98	rVB	75702	85188	24.97%	2.799%
2	1.564	156	163	172	rBV	60723	65244	19.12%	2.143%
3	2.105	320	331	346	rBV	106244	155875	45.69%	5.121%
4	2.507	446	456	466	rVB3	3651	5985	1.75%	0.197%
5	3.892	877	887	915	rBV2	34309	119537	35.04%	3.927%
6	4.346	1012	1028	1053	rBV3	66109	175749	51.51%	5.774%
7	5.043	1228	1245	1276	rBV3	136851	341178	100.00%	11.209%
8	5.613	1411	1422	1446	rBV2	105671	223480	65.50%	7.342%
9	5.915	1503	1516	1531	rBV3	41886	86202	25.27%	2.832%
10	6.066	1551	1563	1586	rBV2	81789	168252	49.32%	5.527%
11	6.985	1839	1849	1871	rBV2	35742	68646	20.12%	2.255%
12	7.313	1939	1951	1970	rBV	150450	268574	78.72%	8.823%
13	7.625	2037	2048	2061	rBV2	20304	38316	11.23%	1.259%
14	7.940	2138	2146	2157	rVB3	2688	3875	1.14%	0.127%
15	8.088	2180	2192	2218	rBV2	170027	332790	97.54%	10.933%
16	8.850	2419	2429	2448	rBV	179135	290898	85.26%	9.557%
17	10.214	2840	2853	2866	rBV2	66817	105213	30.84%	3.457%
18	10.384	2897	2906	2915	rBV3	4479	7591	2.22%	0.249%
19	11.246	3163	3174	3194	rBV	166367	262766	77.02%	8.633%
20	11.532	3255	3263	3264	rBV3	4122	4083	1.20%	0.134%
21	11.622	3280	3291	3310	rBV	148964	234472	68.72%	7.703%




Sum of corrected areas: 3043914

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027948.D
Acq On : 20 Sep 2022 00:46
Operator : SY/MD
Sample : N4658-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

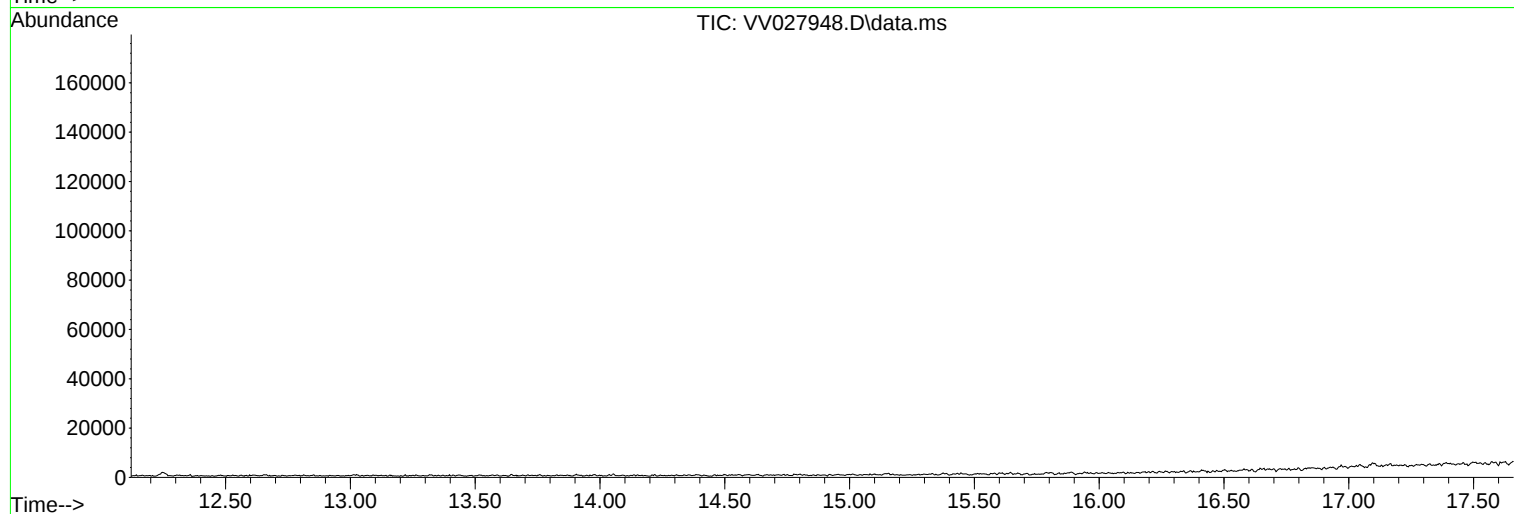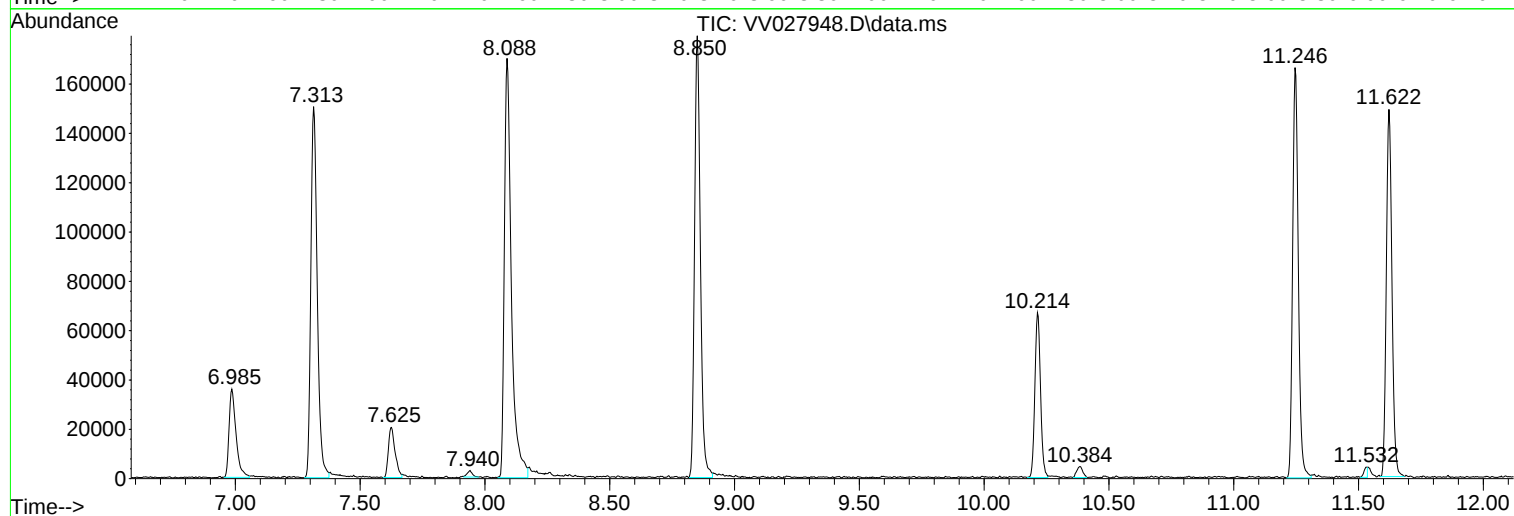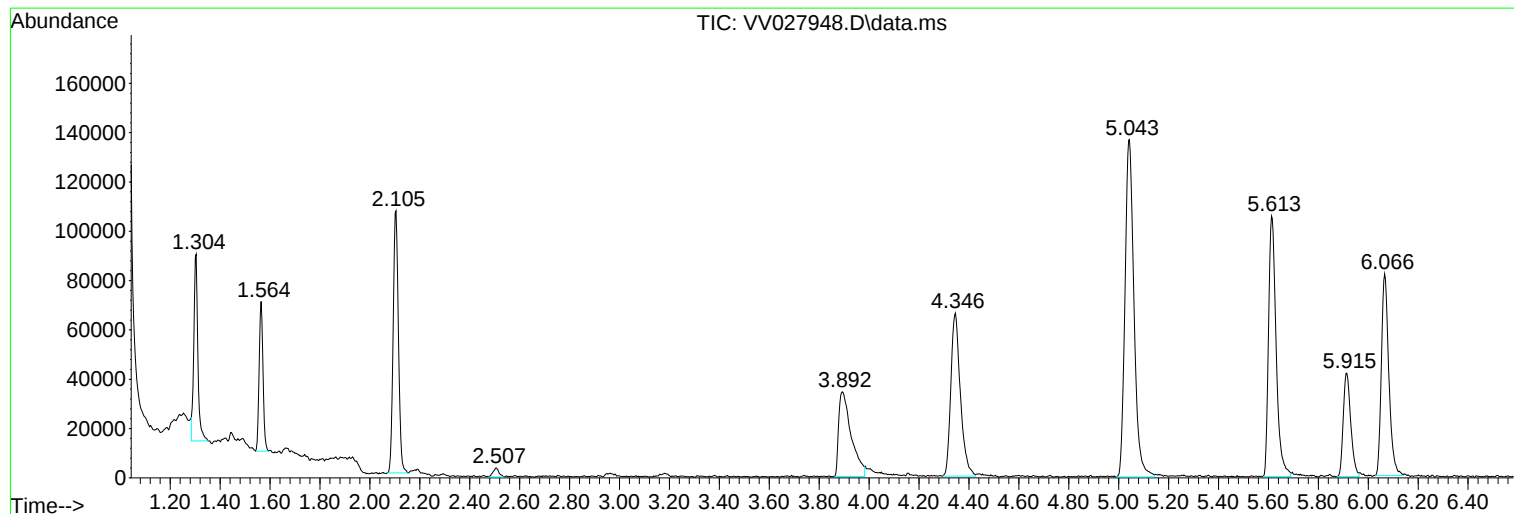

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027948.D
Acq On : 20 Sep 2022 00:46
Operator : SY/MD
Sample : N4658-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027948.D
Acq On : 20 Sep 2022 00:46
Operator : SY/MD
Sample : N4658-14
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED8

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc