

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027949.D
 Acq On : 20 Sep 2022 01:10
 Operator : SY/MD
 Sample : N4658-15
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0ED9

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027949.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	94	rVB	75016	84905	22.17%	2.718%
2	1.565	156	163	173	rVB	59388	66277	17.31%	2.122%
3	2.105	319	331	345	rVB	113832	161855	42.27%	5.181%
4	3.892	878	887	924	rBV	37613	136265	35.59%	4.362%
5	4.343	1012	1027	1052	rBV	74374	189651	49.53%	6.071%
6	5.044	1228	1245	1268	rBV4	154042	382909	100.00%	12.257%
7	5.613	1410	1422	1442	rBV	123000	251004	65.55%	8.035%
8	6.066	1550	1563	1589	rBV	91995	193296	50.48%	6.188%
9	6.986	1840	1849	1875	rBV2	35507	69091	18.04%	2.212%
10	7.314	1936	1951	1977	rBV	144650	260449	68.02%	8.337%
11	7.622	2038	2047	2063	rBV2	21924	39945	10.43%	1.279%
12	7.937	2138	2145	2156	rVB2	4218	6169	1.61%	0.197%
13	8.088	2181	2192	2220	rBV	168100	328769	85.86%	10.524%
14	8.850	2415	2429	2445	rBV	182311	299591	78.24%	9.590%
15	10.214	2842	2853	2865	rBV	70815	111467	29.11%	3.568%
16	10.384	2897	2906	2916	rVB2	6345	10448	2.73%	0.334%
17	11.246	3164	3174	3195	rBV	172463	268437	70.10%	8.593%
18	11.529	3252	3262	3276	rBV3	6789	13470	3.52%	0.431%
19	11.622	3281	3291	3310	rBV	157341	249915	65.27%	8.000%




Sum of corrected areas: 3123913

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027949.D
Acq On : 20 Sep 2022 01:10
Operator : SY/MD
Sample : N4658-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

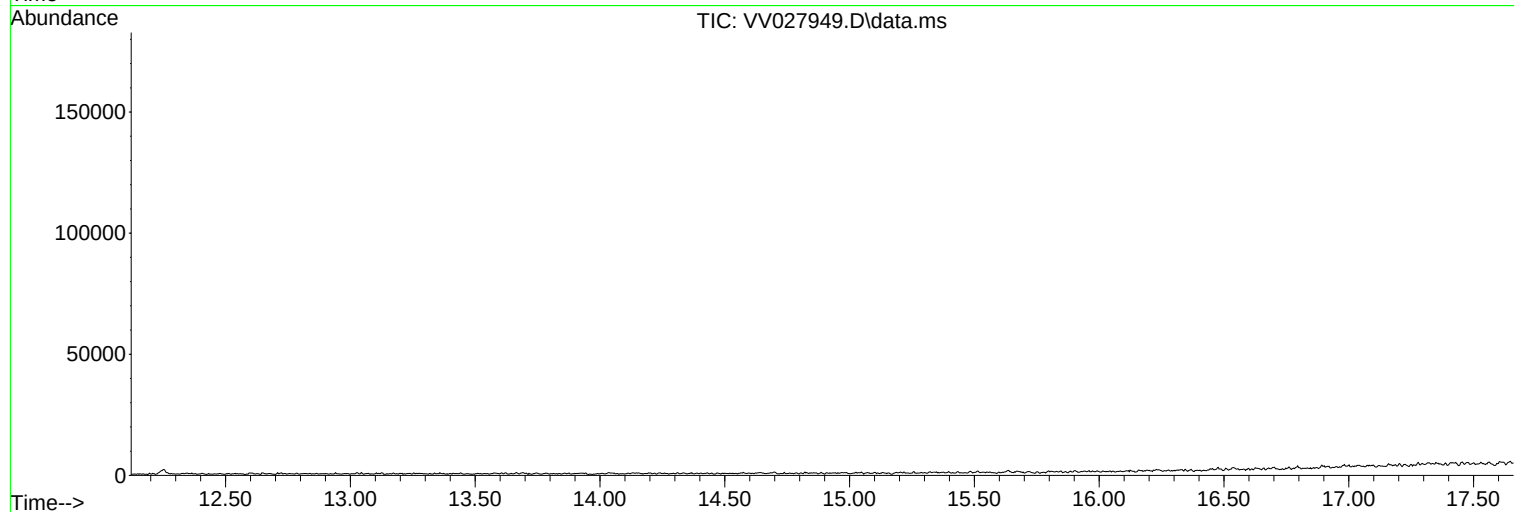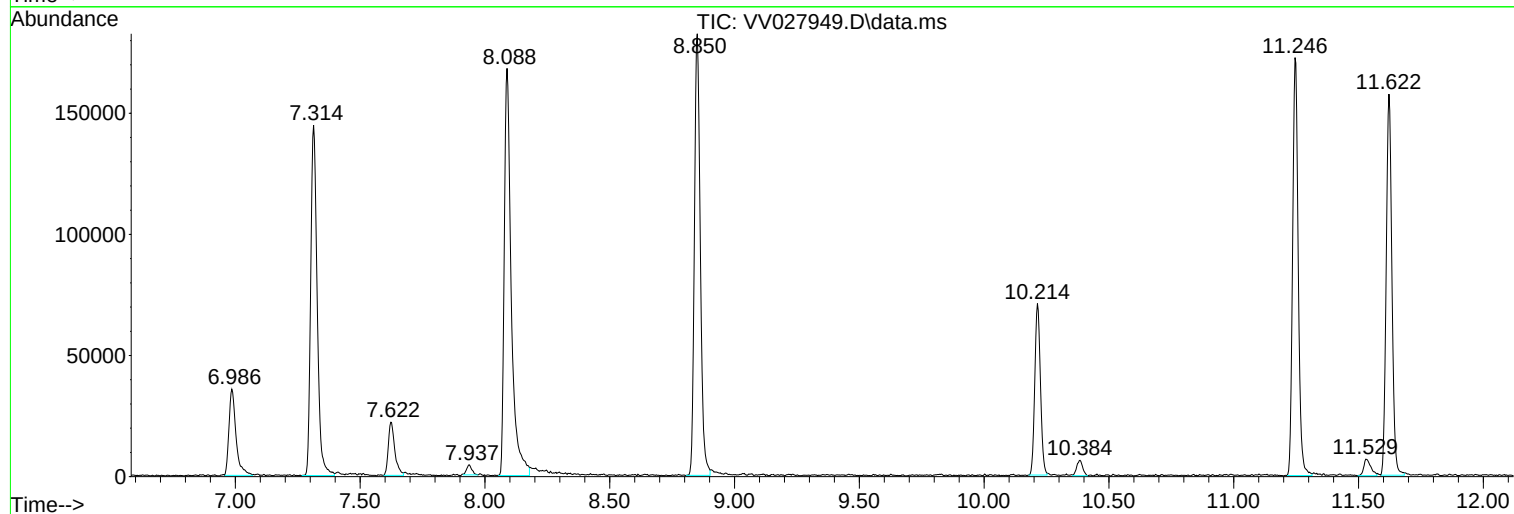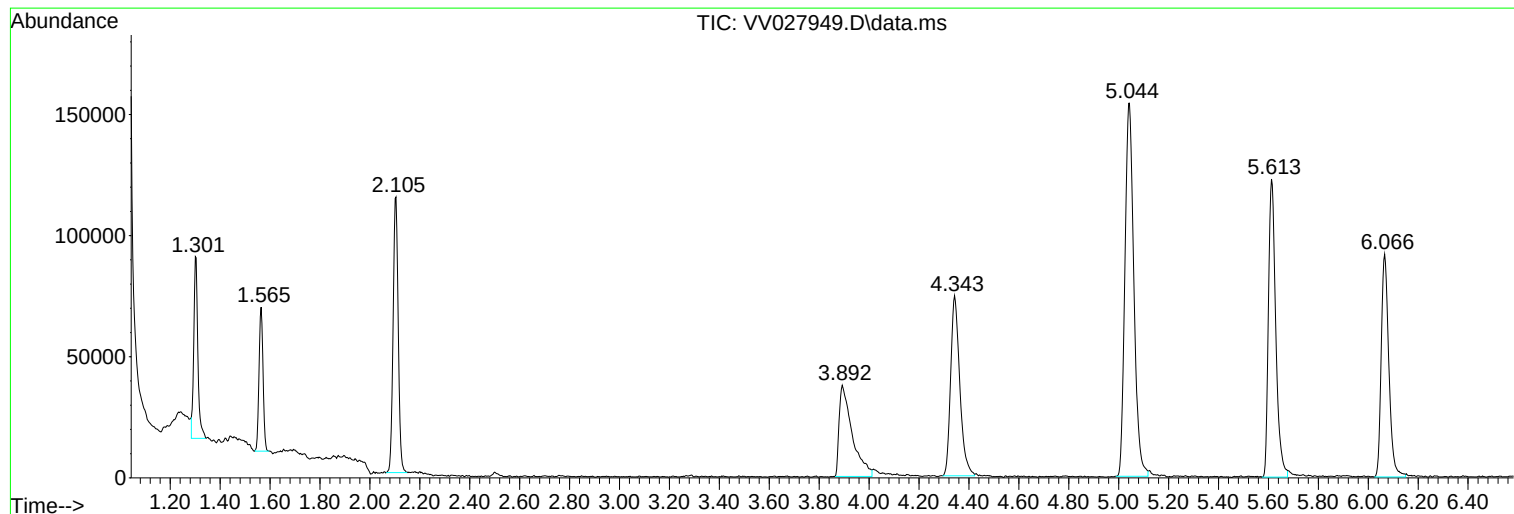

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027949.D
Acq On : 20 Sep 2022 01:10
Operator : SY/MD
Sample : N4658-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027949.D
Acq On : 20 Sep 2022 01:10
Operator : SY/MD
Sample : N4658-15
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0ED9

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
