

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027950.D
 Acq On : 20 Sep 2022 01:35
 Operator : SY/MD
 Sample : N4658-16
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE0

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027950.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	99	rVB	70870	82352	25.05%	2.839%
2	1.564	156	163	175	rVB	56128	63558	19.34%	2.191%
3	2.101	317	330	343	rBV	105236	151300	46.03%	5.216%
4	2.500	443	454	465	rVB5	4640	8683	2.64%	0.299%
5	3.895	878	888	923	rBV	32863	125708	38.24%	4.334%
6	4.342	1012	1027	1054	rBV	63721	163354	49.70%	5.631%
7	5.043	1229	1245	1265	rBV2	131296	328704	100.00%	11.332%
8	5.612	1409	1422	1439	rBV	107052	219315	66.72%	7.561%
9	6.066	1550	1563	1580	rBV	79923	164510	50.05%	5.671%
10	6.985	1836	1849	1864	rBV2	32538	62406	18.99%	2.151%
11	7.313	1940	1951	1971	rBV	132659	239512	72.87%	8.257%
12	7.622	2039	2047	2064	rBV3	19278	35992	10.95%	1.241%
13	7.937	2138	2145	2154	rBV4	3492	6159	1.87%	0.212%
14	8.088	2182	2192	2214	rBV	156407	302545	92.04%	10.430%
15	8.850	2417	2429	2454	rBV	186196	306606	93.28%	10.570%
16	10.213	2843	2853	2870	rBV	71078	113717	34.60%	3.920%
17	10.381	2896	2905	2914	rBV2	7245	12331	3.75%	0.425%
18	11.246	3164	3174	3192	rBV	176061	271643	82.64%	9.364%
19	11.529	3256	3262	3273	rBV4	5487	8638	2.63%	0.298%
20	11.622	3280	3291	3310	rVB	143012	224272	68.23%	7.731%
21	12.252	3479	3487	3496	rVB6	2244	3754	1.14%	0.129%
22	13.750	3944	3953	3960	rBV6	4279	5737	1.75%	0.198%




Sum of corrected areas: 2900796

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027950.D
Acq On : 20 Sep 2022 01:35
Operator : SY/MD
Sample : N4658-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

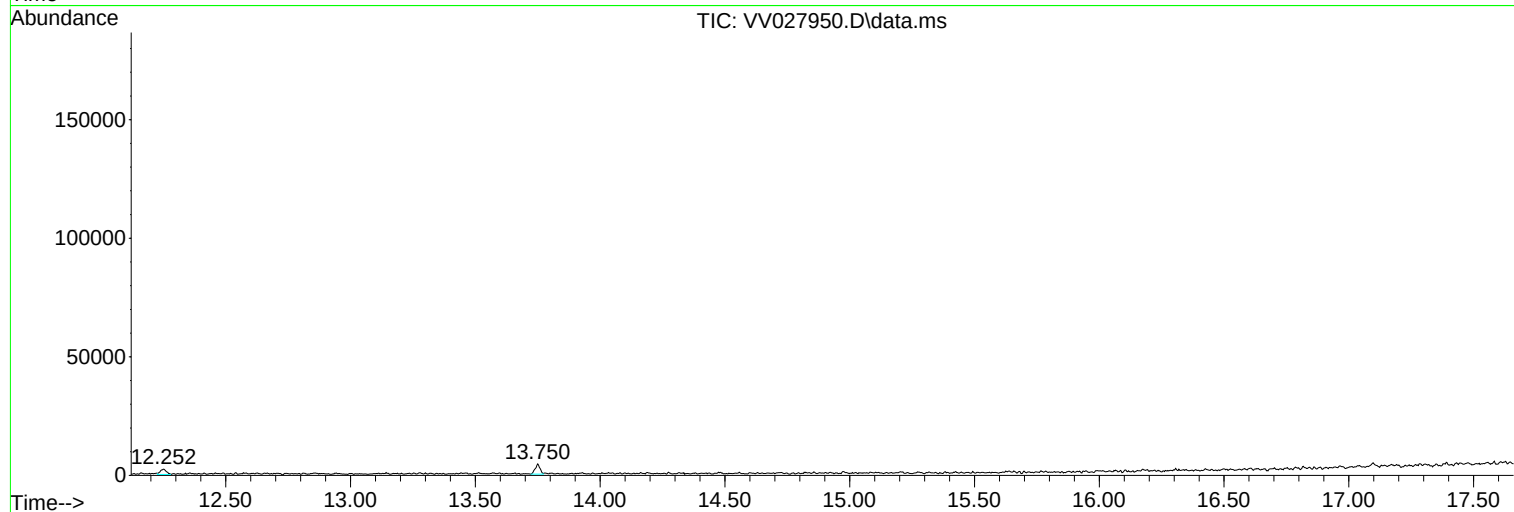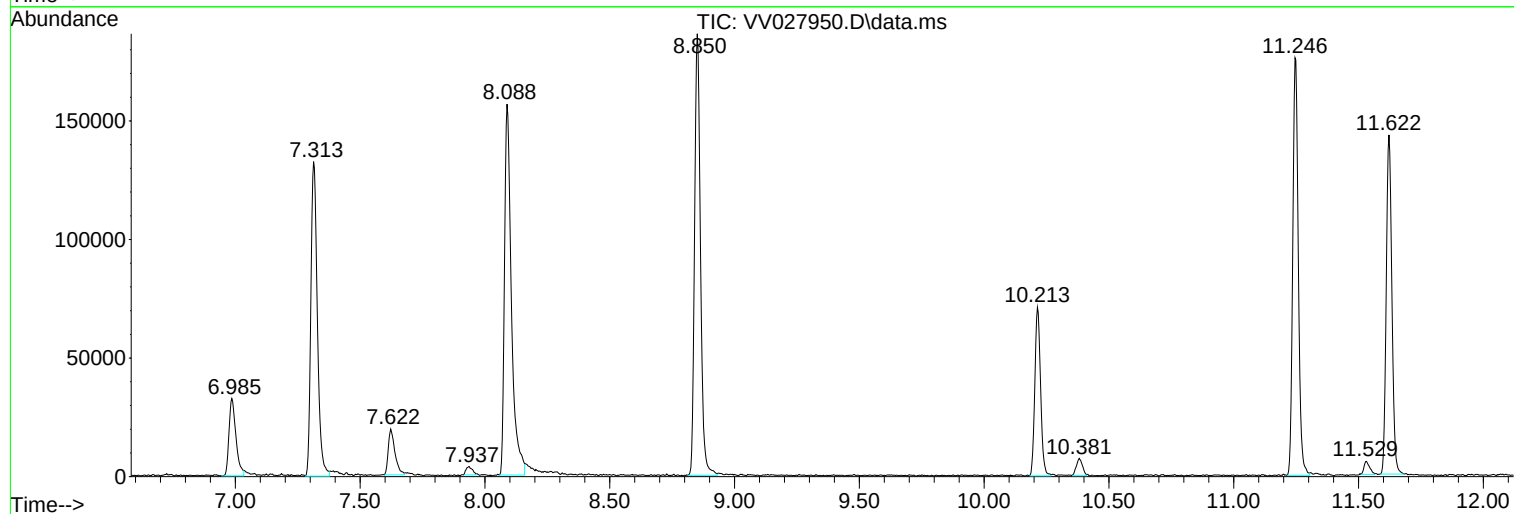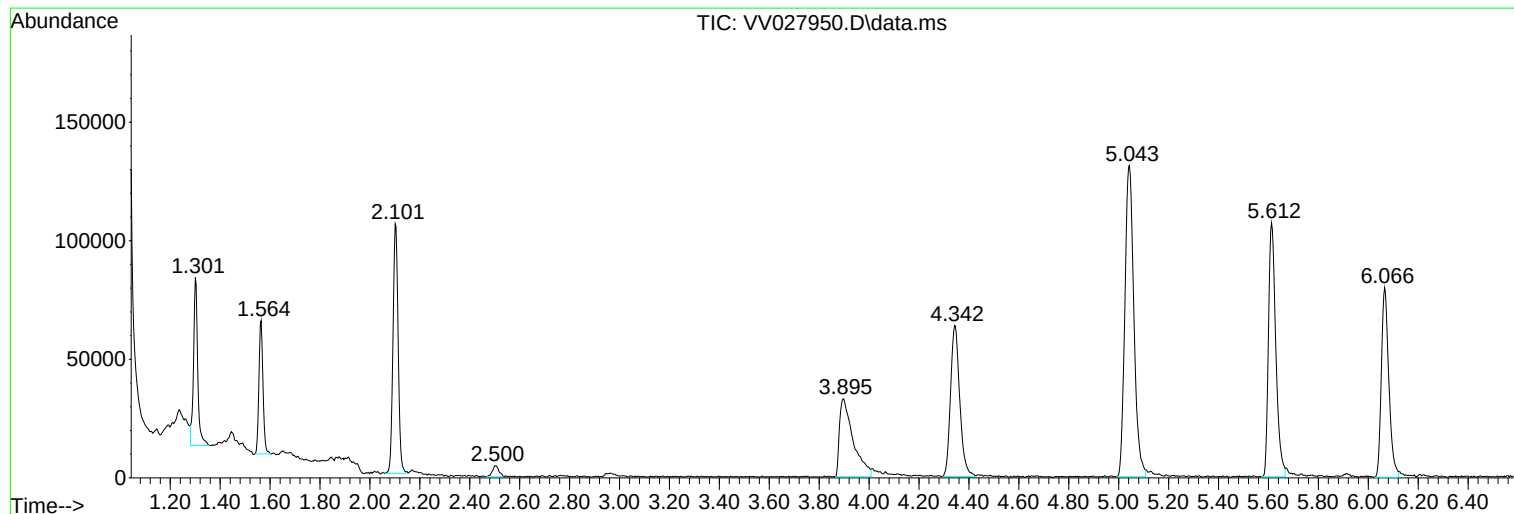

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027950.D
Acq On : 20 Sep 2022 01:35
Operator : SY/MD
Sample : N4658-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027950.D
Acq On : 20 Sep 2022 01:35
Operator : SY/MD
Sample : N4658-16
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 25 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE0

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
