

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027951.D
 Acq On : 20 Sep 2022 02:00
 Operator : SY/MD
 Sample : N4658-17
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE1

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027951.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.304	76	82	97	rVB	71506	82309	22.55%	2.777%
2	1.564	155	163	173	rVB	57778	67920	18.60%	2.291%
3	2.105	320	331	346	rBV	106338	152039	41.65%	5.129%
4	2.503	448	455	465	rVB5	2316	3789	1.04%	0.128%
5	3.899	878	889	919	rBV	34970	127565	34.94%	4.304%
6	4.342	1009	1027	1055	rBV2	68641	180111	49.34%	6.076%
7	5.043	1227	1245	1270	rBV2	146182	365064	100.00%	12.316%
8	5.612	1406	1422	1444	rBV	113554	237538	65.07%	8.014%
9	6.066	1551	1563	1581	rBV	82993	170813	46.79%	5.763%
10	6.985	1839	1849	1864	rBV2	32785	61934	16.97%	2.089%
11	7.313	1937	1951	1975	rBV	138547	244130	66.87%	8.236%
12	7.625	2038	2048	2066	rBV2	20102	37074	10.16%	1.251%
13	8.088	2182	2192	2224	rBV	163121	322365	88.30%	10.875%
14	8.850	2418	2429	2447	rBV	175397	290226	79.50%	9.791%
15	10.214	2841	2853	2870	rBV3	66512	107440	29.43%	3.625%
16	10.381	2896	2905	2918	rBV2	5704	9454	2.59%	0.319%
17	11.246	3164	3174	3196	rBV	164909	262915	72.02%	8.870%
18	11.535	3253	3264	3271	rBV3	6243	11039	3.02%	0.372%
19	11.622	3281	3291	3307	rVB	146224	230472	63.13%	7.775%




Sum of corrected areas: 2964197

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027951.D
Acq On : 20 Sep 2022 02:00
Operator : SY/MD
Sample : N4658-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

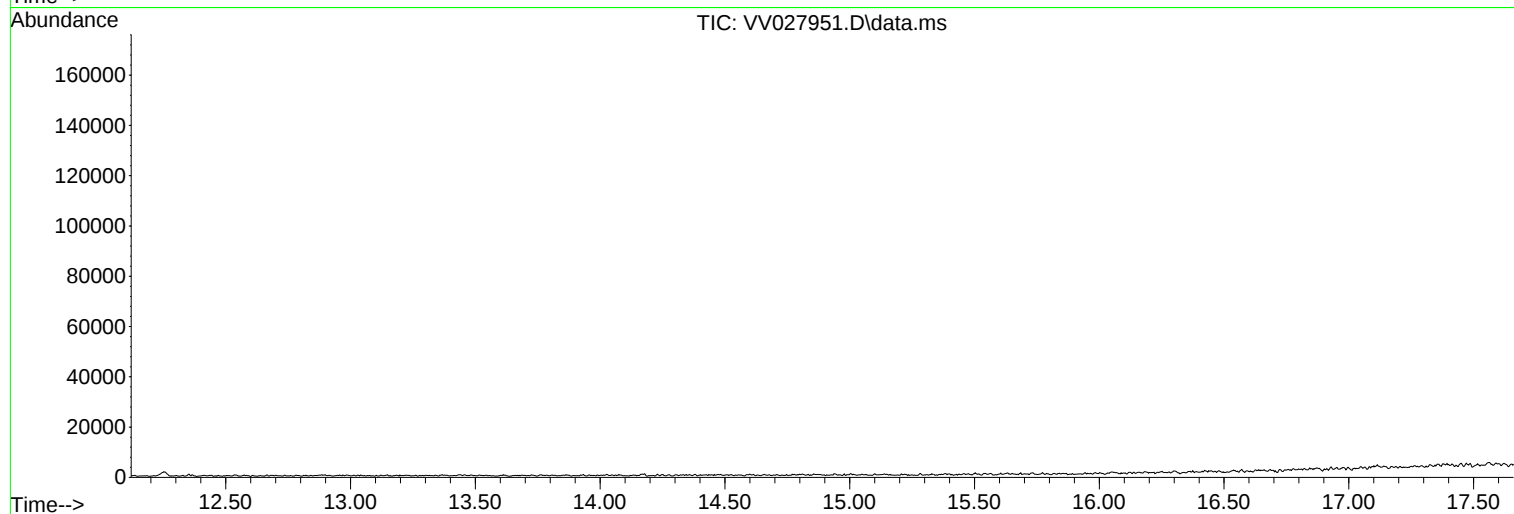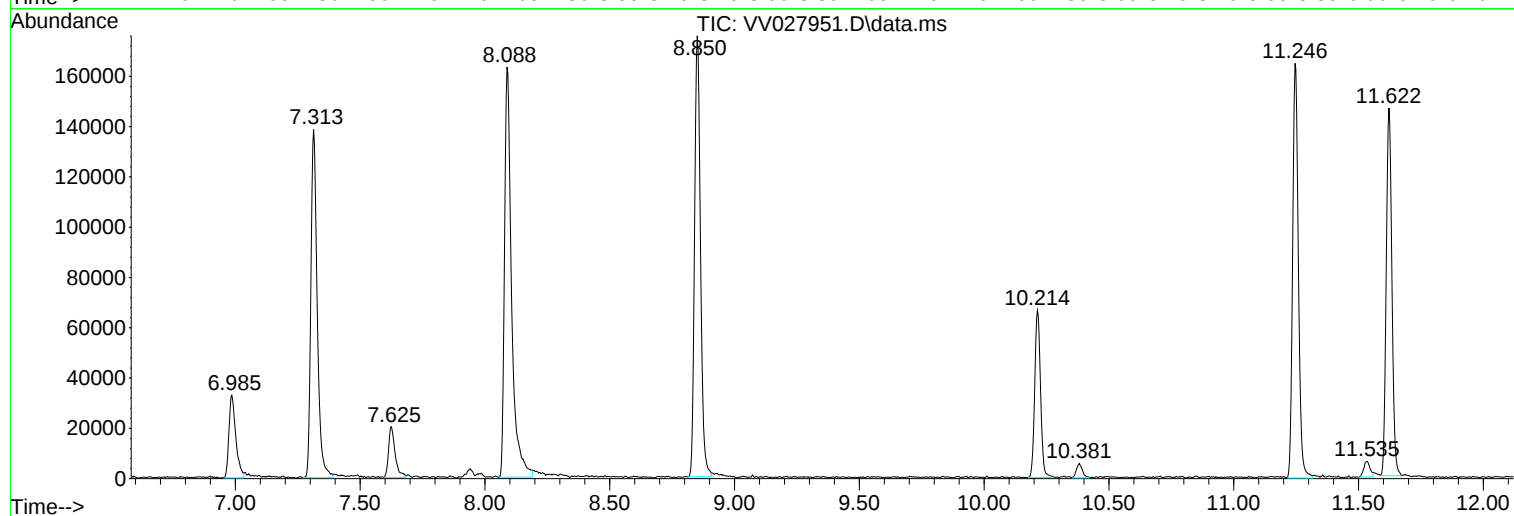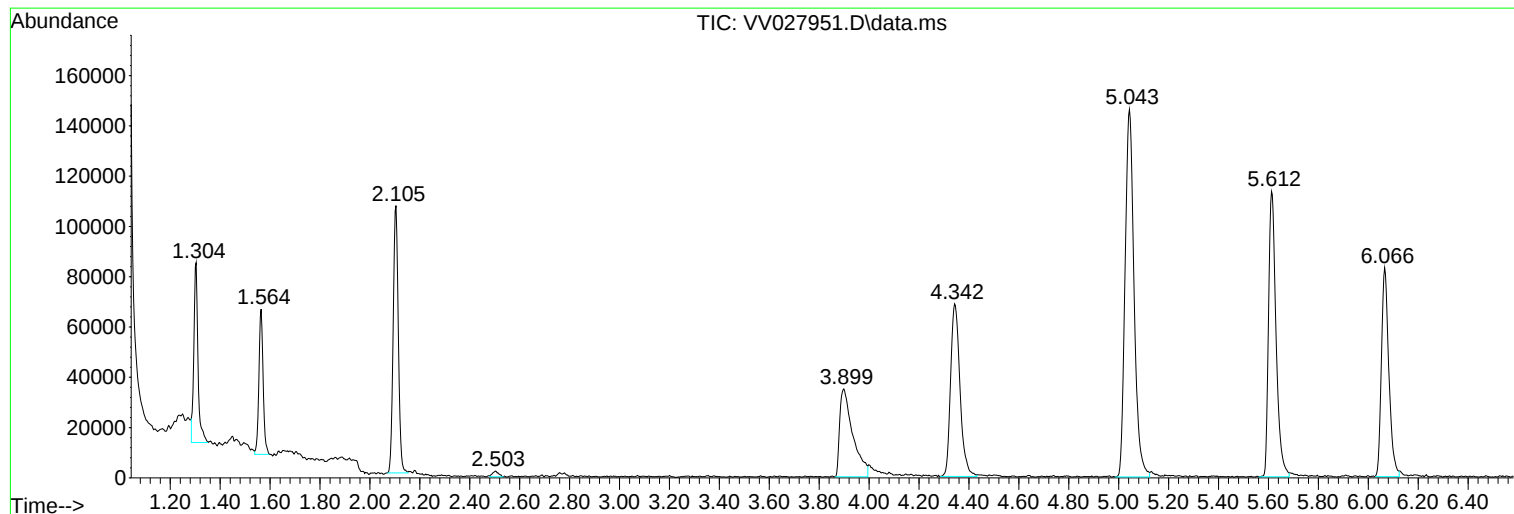

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027951.D
Acq On : 20 Sep 2022 02:00
Operator : SY/MD
Sample : N4658-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027951.D
Acq On : 20 Sep 2022 02:00
Operator : SY/MD
Sample : N4658-17
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
