

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027952.D
 Acq On : 20 Sep 2022 02:25
 Operator : SY/MD
 Sample : N4658-18
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE3

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027952.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.198	45	49	54	rBV2	13287	12360	3.67%	0.426%
2	1.304	76	82	93	rVB	72286	78036	23.17%	2.687%
3	1.564	156	163	174	rVB	57657	63763	18.94%	2.195%
4	2.105	319	331	345	rBV	105049	150716	44.76%	5.189%
5	3.895	878	888	915	rBV	33106	122840	36.48%	4.229%
6	4.342	1011	1027	1049	rBV2	68948	172410	51.20%	5.936%
7	5.043	1229	1245	1269	rBV2	133715	336733	100.00%	11.594%
8	5.612	1411	1422	1448	rBV	108167	222999	66.22%	7.678%
9	6.066	1551	1563	1585	rBV2	80792	167886	49.86%	5.780%
10	6.985	1840	1849	1865	rBV2	31310	61082	18.14%	2.103%
11	7.313	1939	1951	1974	rBV	138394	245523	72.91%	8.454%
12	7.625	2039	2048	2063	rBV2	19513	36674	10.89%	1.263%
13	7.934	2136	2144	2153	rBV2	2401	3952	1.17%	0.136%
14	8.088	2180	2192	2215	rBV	154164	305492	90.72%	10.518%
15	8.850	2416	2429	2445	rBV	190999	309431	91.89%	10.654%
16	10.214	2841	2853	2870	rBV	70527	112375	33.37%	3.869%
17	10.384	2896	2906	2918	rBV2	5372	9154	2.72%	0.315%
18	11.246	3163	3174	3191	rBV	166911	263550	78.27%	9.074%
19	11.622	3279	3291	3304	rBV2	145050	229413	68.13%	7.899%




Sum of corrected areas: 2904389

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027952.D
Acq On : 20 Sep 2022 02:25
Operator : SY/MD
Sample : N4658-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

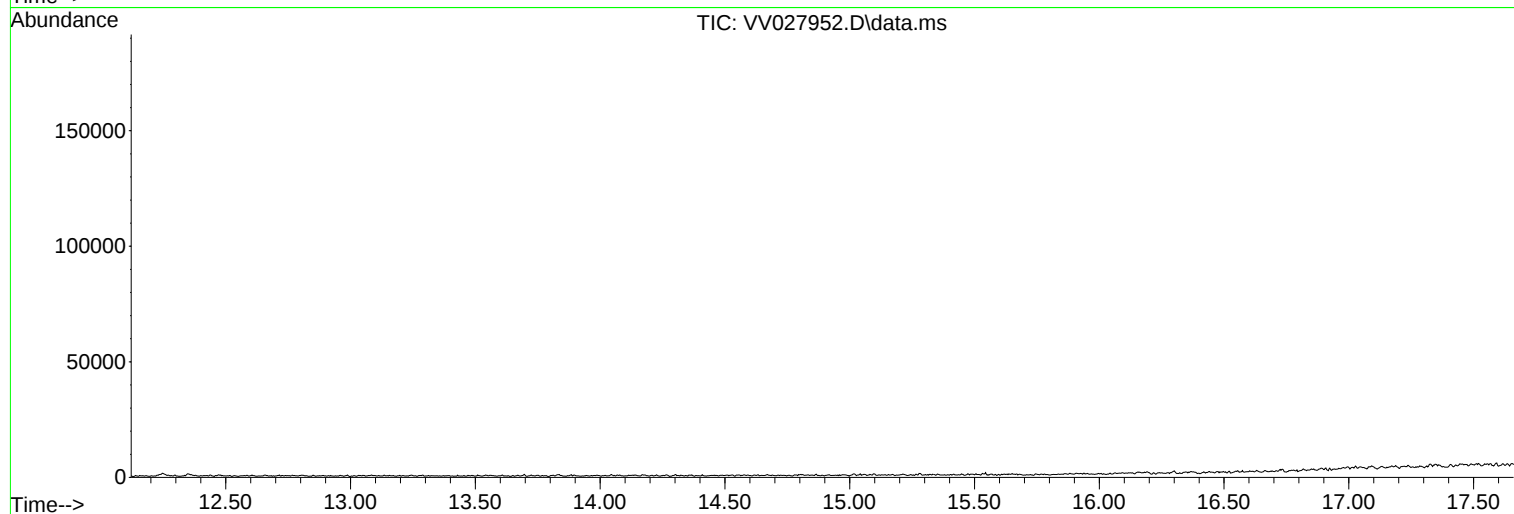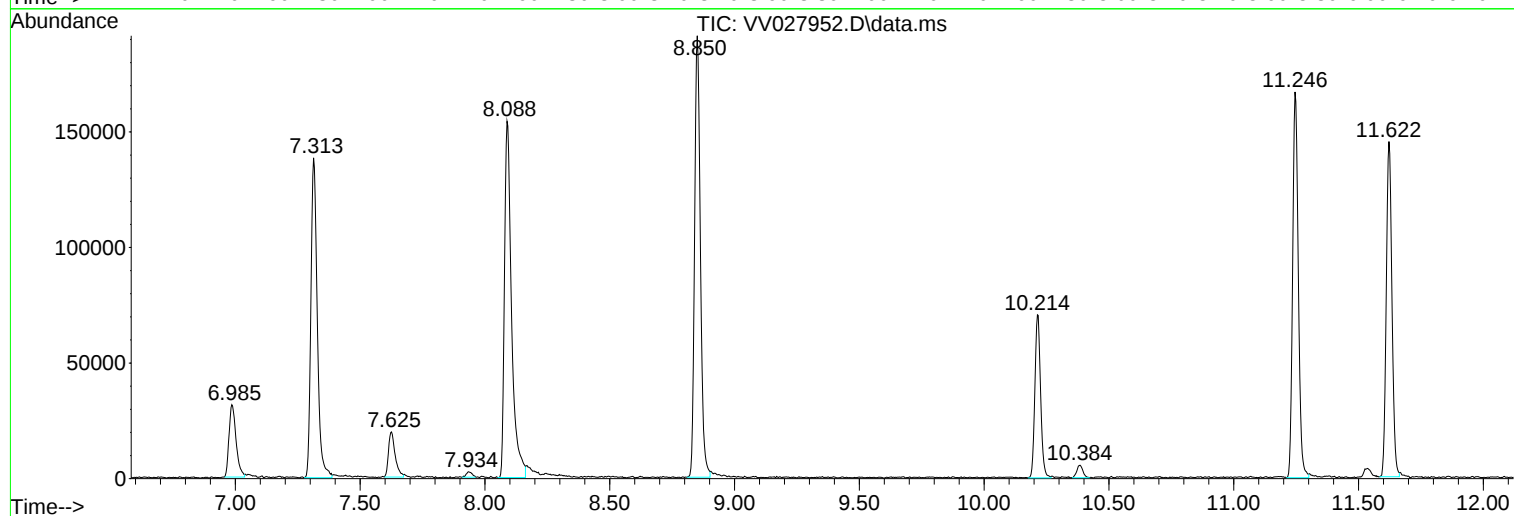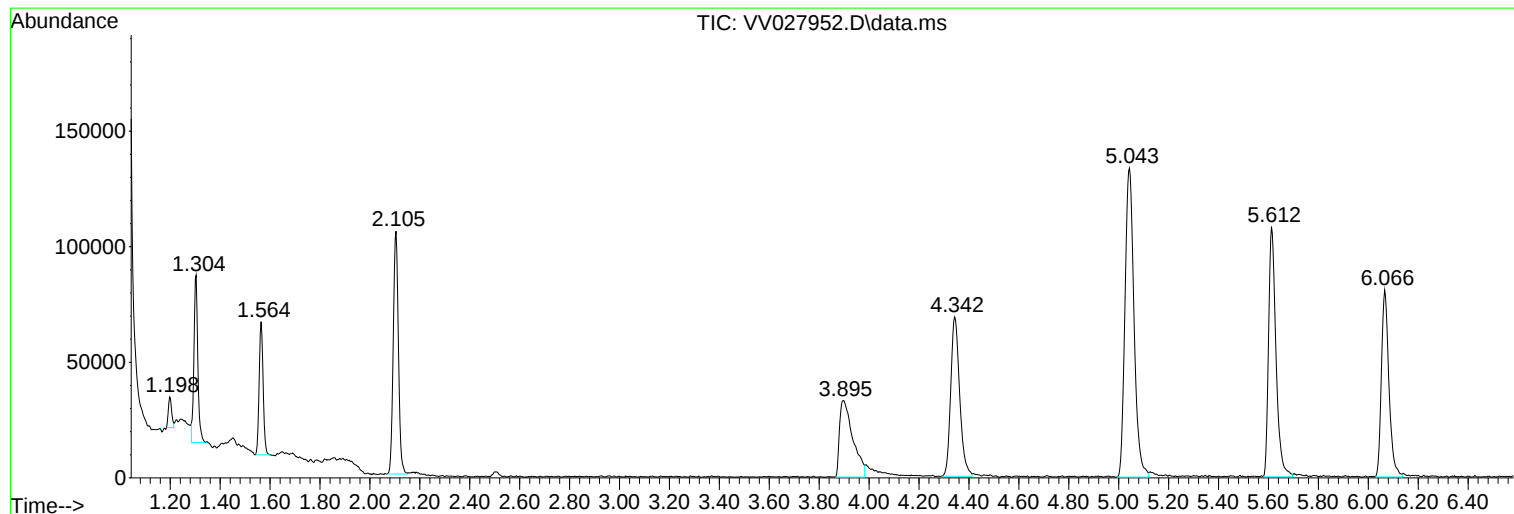

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027952.D
Acq On : 20 Sep 2022 02:25
Operator : SY/MD
Sample : N4658-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027952.D
Acq On : 20 Sep 2022 02:25
Operator : SY/MD
Sample : N4658-18
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc