

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027953.D
 Acq On : 20 Sep 2022 02:50
 Operator : SY/MD
 Sample : N4658-19
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 28 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EE4

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M

Title : TRACE VOA SFAM1.0

Signal : TIC: VV027953.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.198	45	49	56	rBV2	14113	13954	3.82%	0.456%
2	1.301	75	81	100	rVB	72341	84290	23.09%	2.753%
3	1.564	156	163	172	rVB	55970	63484	17.39%	2.073%
4	2.101	320	330	348	rVB	107807	153864	42.14%	5.025%
5	3.895	877	888	922	rBV	33902	130389	35.71%	4.259%
6	4.342	1012	1027	1051	rBV	68931	173848	47.62%	5.678%
7	5.043	1229	1245	1270	rBV2	146438	365106	100.00%	11.924%
8	5.612	1410	1422	1449	rBV	122224	250980	68.74%	8.197%
9	6.066	1549	1563	1582	rBV2	84990	179588	49.19%	5.865%
10	6.985	1836	1849	1870	rBV	34788	69356	19.00%	2.265%
11	7.313	1938	1951	1979	rBV	148585	269047	73.69%	8.787%
12	7.622	2039	2047	2063	rBV	21493	39360	10.78%	1.286%
13	7.937	2134	2145	2154	rBV3	3101	5412	1.48%	0.177%
14	8.088	2181	2192	2217	rBV	167656	329598	90.27%	10.765%
15	8.850	2418	2429	2453	rBV	185294	302294	82.80%	9.873%
16	10.214	2841	2853	2866	rBV	68767	107371	29.41%	3.507%
17	10.381	2898	2905	2917	rVB2	5025	7777	2.13%	0.254%
18	11.246	3162	3174	3190	rBV	173203	269695	73.87%	8.808%
19	11.532	3253	3263	3275	rBV6	5779	10716	2.94%	0.350%
20	11.622	3280	3291	3308	rBV	149085	235703	64.56%	7.698%




Sum of corrected areas: 3061832

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027953.D
Acq On : 20 Sep 2022 02:50
Operator : SY/MD
Sample : N4658-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

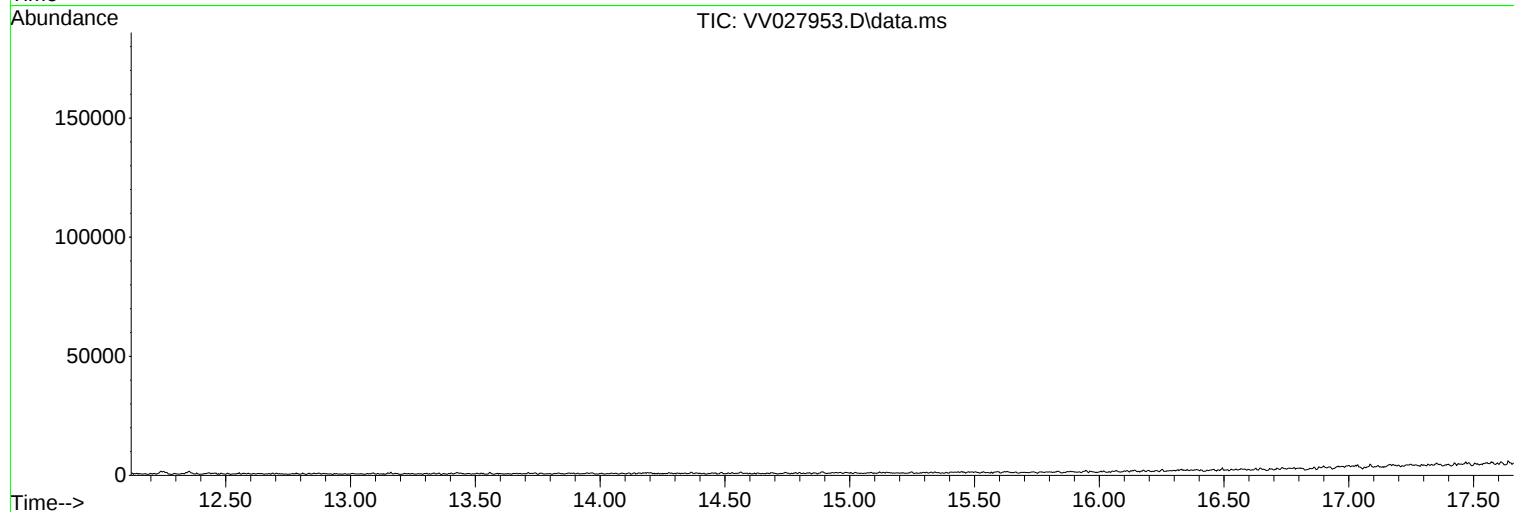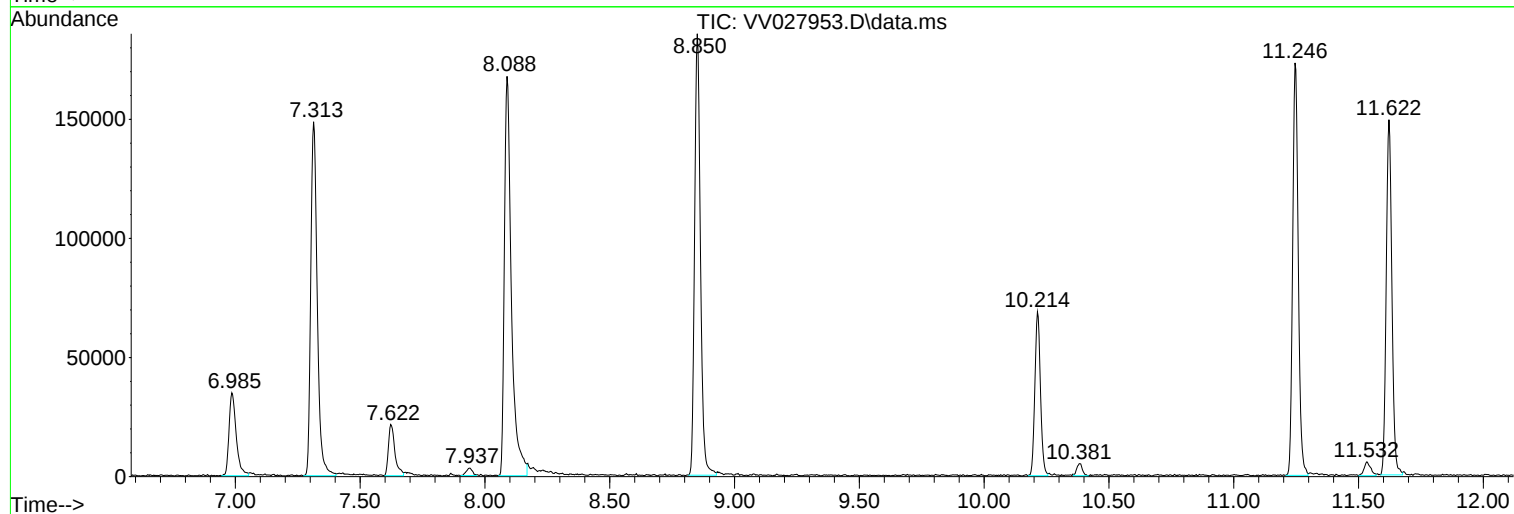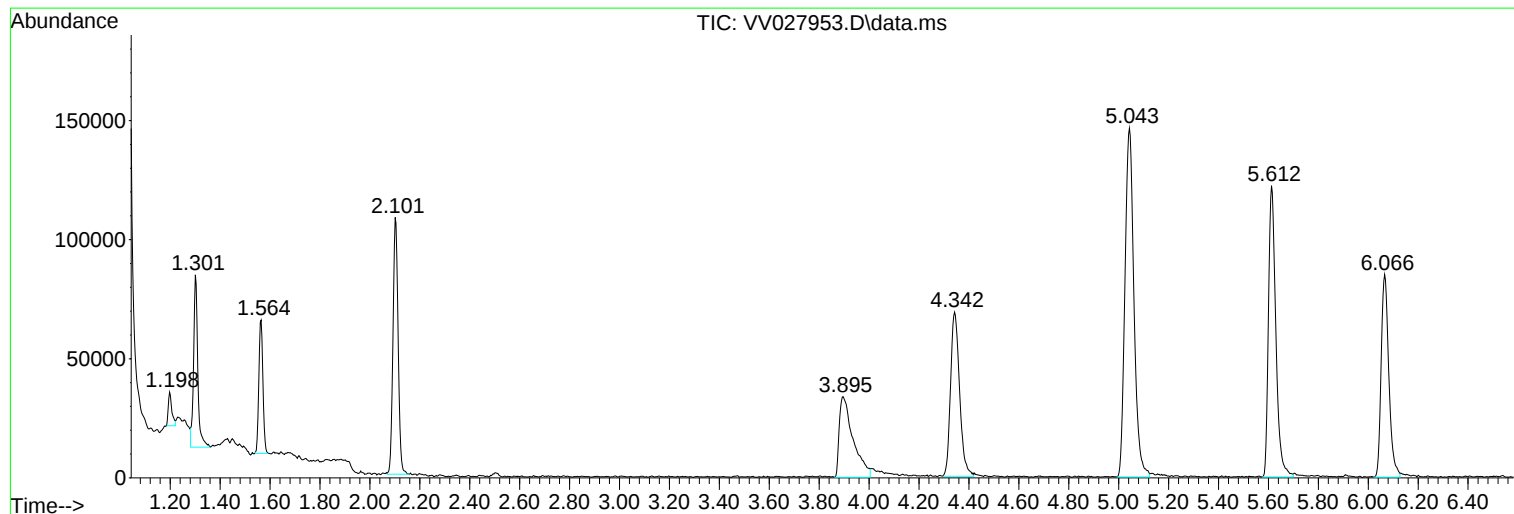

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027953.D
Acq On : 20 Sep 2022 02:50
Operator : SY/MD
Sample : N4658-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027953.D
Acq On : 20 Sep 2022 02:50
Operator : SY/MD
Sample : N4658-19
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 28 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EE4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc