

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027954.D
 Acq On : 20 Sep 2022 03:14
 Operator : SY/MD
 Sample : N4658-04
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VHBLK001

Integration Parameters: rteint.p

Integrator: RTE

Smoothing : ON

Filtering: 5

Sampling : 1

Min Area: 3 % of largest Peak

Start Thrs: 0.1

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Title : TRACE VOA SFAM1.0

Signal : TIC: VV027954.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.198	46	49	53	rBV2	5997	4445	1.29%	0.148%
2	1.301	75	81	101	rVB	74815	91195	26.52%	3.040%
3	1.564	156	163	174	rVB	57497	65715	19.11%	2.190%
4	2.105	318	331	344	rBV	112953	161208	46.88%	5.373%
5	2.503	446	455	467	rVB8	3451	5583	1.62%	0.186%
6	3.892	875	887	916	rBV	34593	123180	35.82%	4.106%
7	4.343	1012	1027	1052	rBV	69002	173373	50.42%	5.779%
8	5.043	1226	1245	1271	rBV3	136030	343843	100.00%	11.461%
9	5.613	1409	1422	1442	rBV2	108135	224969	65.43%	7.499%
10	6.066	1550	1563	1588	rBV2	80751	171631	49.92%	5.721%
11	6.985	1838	1849	1868	rBV2	33502	63912	18.59%	2.130%
12	7.313	1941	1951	1974	rBV	144131	257683	74.94%	8.589%
13	7.622	2038	2047	2066	rBV2	21407	40666	11.83%	1.355%
14	7.937	2139	2145	2154	rBV5	2456	3912	1.14%	0.130%
15	8.088	2181	2192	2218	rBV	165538	331278	96.35%	11.042%
16	8.850	2414	2429	2444	rBV	195457	321193	93.41%	10.706%
17	10.214	2841	2853	2867	rBV	66677	106690	31.03%	3.556%
18	10.384	2896	2906	2916	rBV4	3547	6166	1.79%	0.206%
19	11.246	3164	3174	3189	rBV	172285	265955	77.35%	8.865%
20	11.542	3256	3266	3273	rBV6	2038	3652	1.06%	0.122%
21	11.622	3279	3291	3306	rBV2	148059	233864	68.01%	7.795%




Sum of corrected areas: 3000113

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027954.D
Acq On : 20 Sep 2022 03:14
Operator : SY/MD
Sample : N4658-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

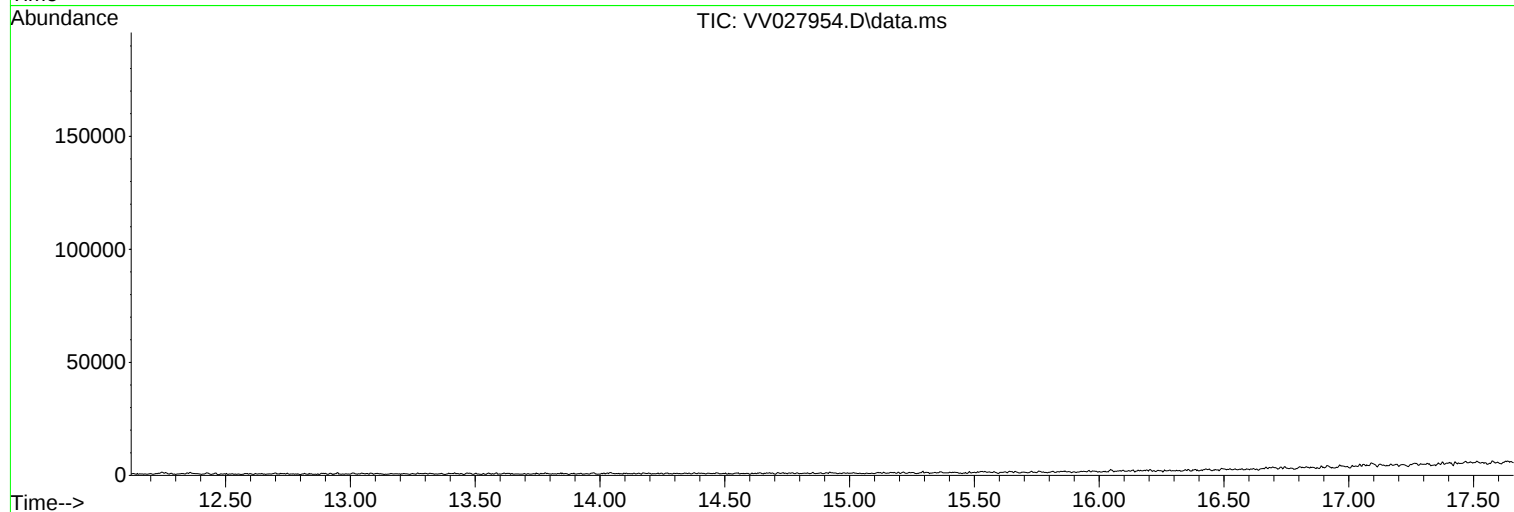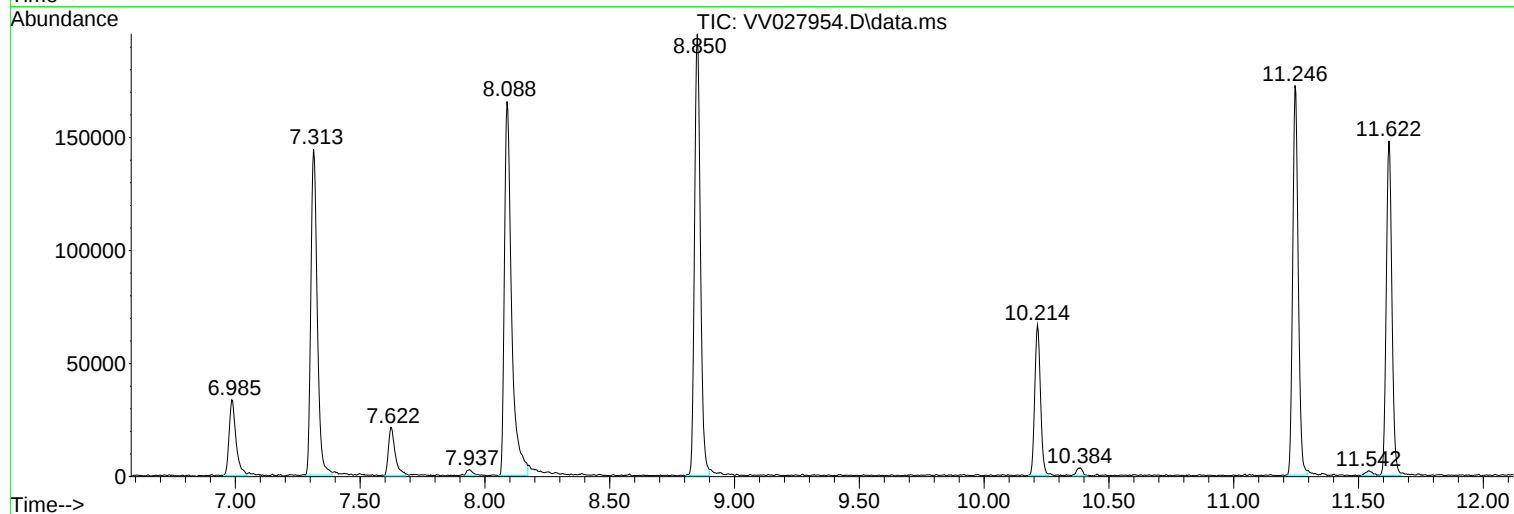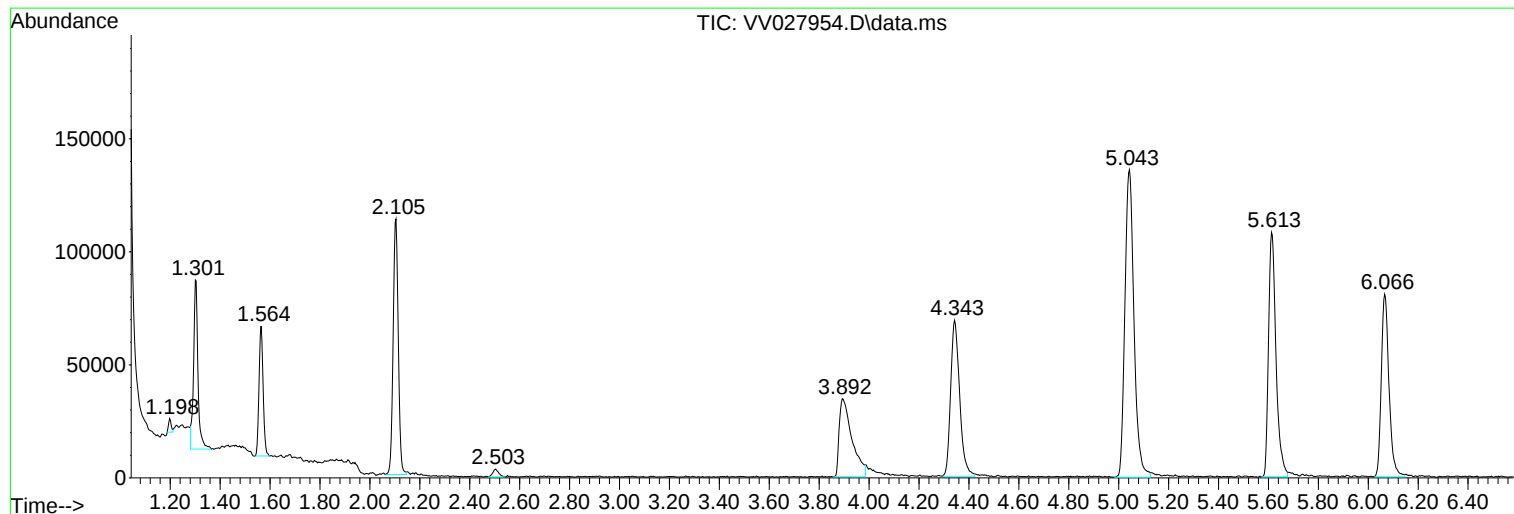

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027954.D
Acq On : 20 Sep 2022 03:14
Operator : SY/MD
Sample : N4658-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
Data File : VV027954.D
Acq On : 20 Sep 2022 03:14
Operator : SY/MD
Sample : N4658-04
Misc : 25.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VHBLK001

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
Quant Title : TRACE VOA SFAM1.0

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
