
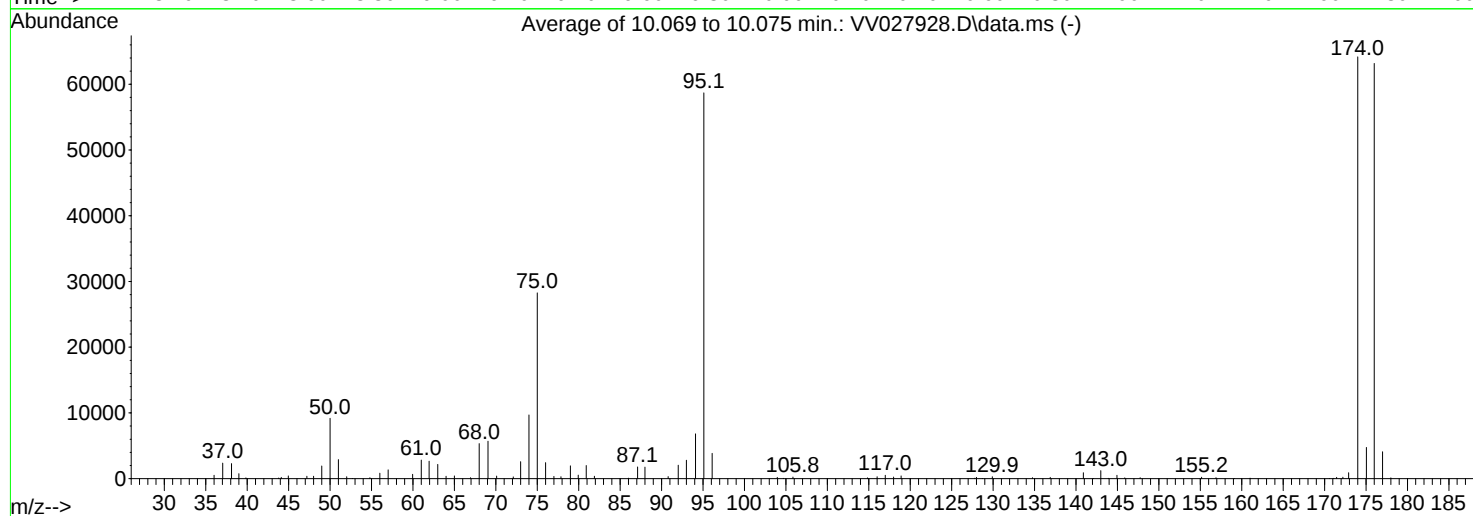


Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV091922\
 Data File : VV027928.D
 Acq On : 19 Sep 2022 10:20
 Operator : SY/MD
 Sample : BFB373
 Misc : 25.0mL/MSVOA_V/WATER
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 BFB373

Integration File: rteint.p

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVTR091922WMA.M
 Title : TRACE VOA SFAM1.0
 Last Update : Tue Sep 20 01:54:53 2022

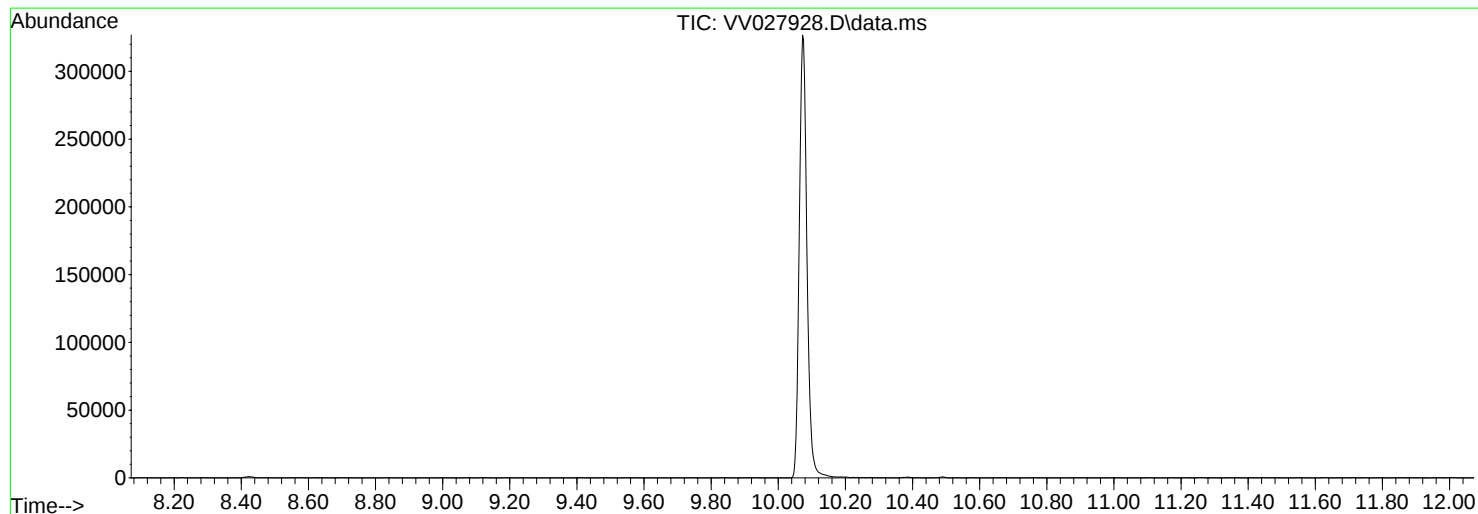

AutoFind: Scans 2808, 2809, 2810; Background Corrected with Scan 2797

Target Mass	Rel. to Mass	Lower Limit%	Upper Limit%	Rel. Abn%	Raw Abn	Result Pass/Fail
50	95	15	40	15.6	9171	PASS
75	95	30	80	48.2	28261	PASS
95	95	100	100	100.0	58688	PASS
96	95	5	9	6.5	3836	PASS
173	174	0.00	2	1.4	894	PASS
174	95	50	120	109.3	64173	PASS
175	174	5	9	7.4	4740	PASS
176	174	95	105	98.4	63163	PASS
177	176	5	10	6.5	4092	PASS

m/z Abundance

Instrument :
MSVOA_V
ClientSampleId :
BFB373

m/z	Abundance
36.00	466.0
37.10	2334.0
38.10	2151.0
39.00	730.0
39.90	109.0
43.80	311.0
45.00	367.0
47.20	343.0
47.90	392.0
49.00	1889.0
50.00	8826.0
51.00	2763.0
52.00	268.0
54.80	193.0
56.00	823.0
57.00	1214.0
60.00	627.0
61.00	2698.0
62.00	2677.0
63.00	1979.0
64.00	364.0
65.00	453.0
67.10	140.0
68.00	5098.0
69.00	5277.0
70.10	393.0
72.10	215.0
73.00	2266.0
74.00	8930.0
75.00	27200.0
76.00	2494.0
77.00	316.0
78.00	214.0
79.00	1771.0
80.00	515.0
80.90	1915.0
81.90	367.0
87.10	1669.0
88.00	1666.0
90.80	341.0
92.00	2030.0
93.00	2628.0
94.10	6613.0
95.10	55352.0
96.10	3738.0
104.00	200.0
104.70	120.0
105.90	267.0
114.80	126.0
116.00	227.0
117.10	512.0
117.90	230.0
119.00	413.0
127.80	226.0
128.70	112.0
129.90	269.0
134.80	154.0
136.90	177.0
140.90	789.0
142.10	104.0
143.00	1120.0
144.90	544.0
145.90	122.0
147.80	162.0
155.20	184.0
156.90	117.0
171.10	131.0
171.50	150.0
172.20	331.0
172.90	805.0
174.00	60048.0
175.00	4562.0
176.00	58208.0
177.00	3827.0
178.00	131.0

Instrument :
MSVOA_V
ClientSampleId :
BFB373

m/z	Abundance
36.00	519.0
37.10	2419.0
38.10	2382.0
39.00	766.0
39.90	139.0
44.10	303.0
45.00	430.0
47.20	379.0
48.00	403.0
49.00	1932.0
50.00	9530.0
51.00	3015.0
52.00	311.0
54.80	167.0
56.00	883.0
57.00	1405.0
59.90	697.0
61.00	2938.0
61.90	2750.0
63.00	2226.0
64.00	392.0
65.00	457.0
66.90	152.0
68.00	5577.0
69.10	5864.0
70.10	391.0
72.10	287.0
73.00	2667.0
74.00	10011.0
75.00	29216.0
76.00	2551.0
77.00	343.0
77.80	293.0
79.00	1951.0
79.90	566.0
80.90	2015.0
81.90	364.0
86.00	119.0
87.10	1867.0
88.00	1857.0
90.80	342.0
92.00	2118.0
93.00	2900.0
94.10	7131.0
95.10	60824.0
96.10	3940.0
103.90	210.0
105.90	249.0
114.80	126.0
116.00	330.0
117.00	532.0
118.00	240.0
118.90	427.0
128.00	288.0
129.90	306.0
134.80	147.0
136.90	198.0
140.90	940.0
143.00	1234.0
145.00	562.0
145.90	125.0
147.70	151.0
155.20	217.0
156.90	150.0
161.00	110.0
171.40	198.0
172.20	371.0
172.90	925.0
174.00	66312.0
175.00	4926.0
176.00	65328.0
177.00	4269.0
178.00	134.0

Instrument :
MSVOA_V
ClientSampleId :
BFB373

m/z	Abundance
36.00	540.0
37.00	2325.0
38.10	2306.0
39.00	741.0
39.80	153.0
44.10	265.0
44.90	432.0
47.20	411.0
48.10	324.0
49.00	1937.0
50.00	9158.0
51.00	2893.0
52.00	291.0
52.70	100.0
54.80	113.0
56.00	796.0
57.00	1418.0
60.00	682.0
61.00	2834.0
61.90	2538.0
63.00	2299.0
64.00	359.0
65.00	371.0
66.80	157.0
68.00	5348.0
69.10	5950.0
70.10	366.0
72.10	347.0
73.00	2790.0
74.00	10133.0
75.00	28368.0
76.00	2277.0
77.00	354.0
77.80	348.0
79.00	2151.0
79.90	539.0
80.90	2073.0
81.90	400.0
86.00	127.0
87.10	1804.0
88.00	1736.0
90.80	279.0
92.00	1961.0
93.00	2862.0
94.10	6745.0
95.10	59888.0
96.10	3829.0
104.00	202.0
105.80	234.0
114.90	119.0
116.00	327.0
116.90	525.0
118.10	243.0
118.80	440.0
128.00	333.0
129.90	292.0
134.70	118.0
136.90	190.0
140.90	947.0
143.00	1269.0
143.90	121.0
145.00	475.0
145.90	117.0
147.70	142.0
155.10	237.0
156.90	158.0
159.10	101.0
161.00	110.0
170.60	113.0
171.50	204.0
172.90	951.0
174.00	66160.0
175.10	4733.0
176.00	65952.0
177.00	4179.0
178.00	113.0

Instrument :
MSVOA_V
ClientSampleId :
BFB373