

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027989.D
 Acq On : 21 Sep 2022 02:39
 Operator : SY/MD
 Sample : N4674-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E97

Quant Time: Sep 21 08:05:11 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 21 06:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	357098	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	345448	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	153353	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	139635	44.542	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	89.080%		
7) Chloroethane-d5	1.558	69	117695	46.997	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	94.000%		
11) 1,1-Dichloroethene-d2	2.101	63	193630	34.865	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	69.740%		
21) 2-Butanone-d5	3.873	46	193079	103.575	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	103.570%		
24) Chloroform-d	4.342	84	244971	46.543	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	93.080%		
26) 1,2-Dichloroethane-d4	5.024	65	161676	47.400	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.800%		
32) Benzene-d6	5.043	84	475982	47.805	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.600%		
36) 1,2-Dichloropropane-d6	6.063	67	164839	53.613	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	107.220%		
41) Toluene-d8	7.310	98	417994	45.843	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	91.680%		
43) trans-1,3-Dichloroprop...	7.619	79	70070	45.574	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	91.140%		
47) 2-Hexanone-d5	8.085	63	162005	107.558	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	107.560%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	232397	51.354	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	102.700%		
66) 1,2-Dichlorobenzene-d4	11.622	152	160843	54.030	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	108.060%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.101	101	2134	0.823	ug/L	# 22


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027989.D
Acq On : 21 Sep 2022 02:39
Operator : SY/MD
Sample : N4674-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E97

Quant Time: Sep 21 08:05:11 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 21 06:45:13 2022
Response via : Initial Calibration

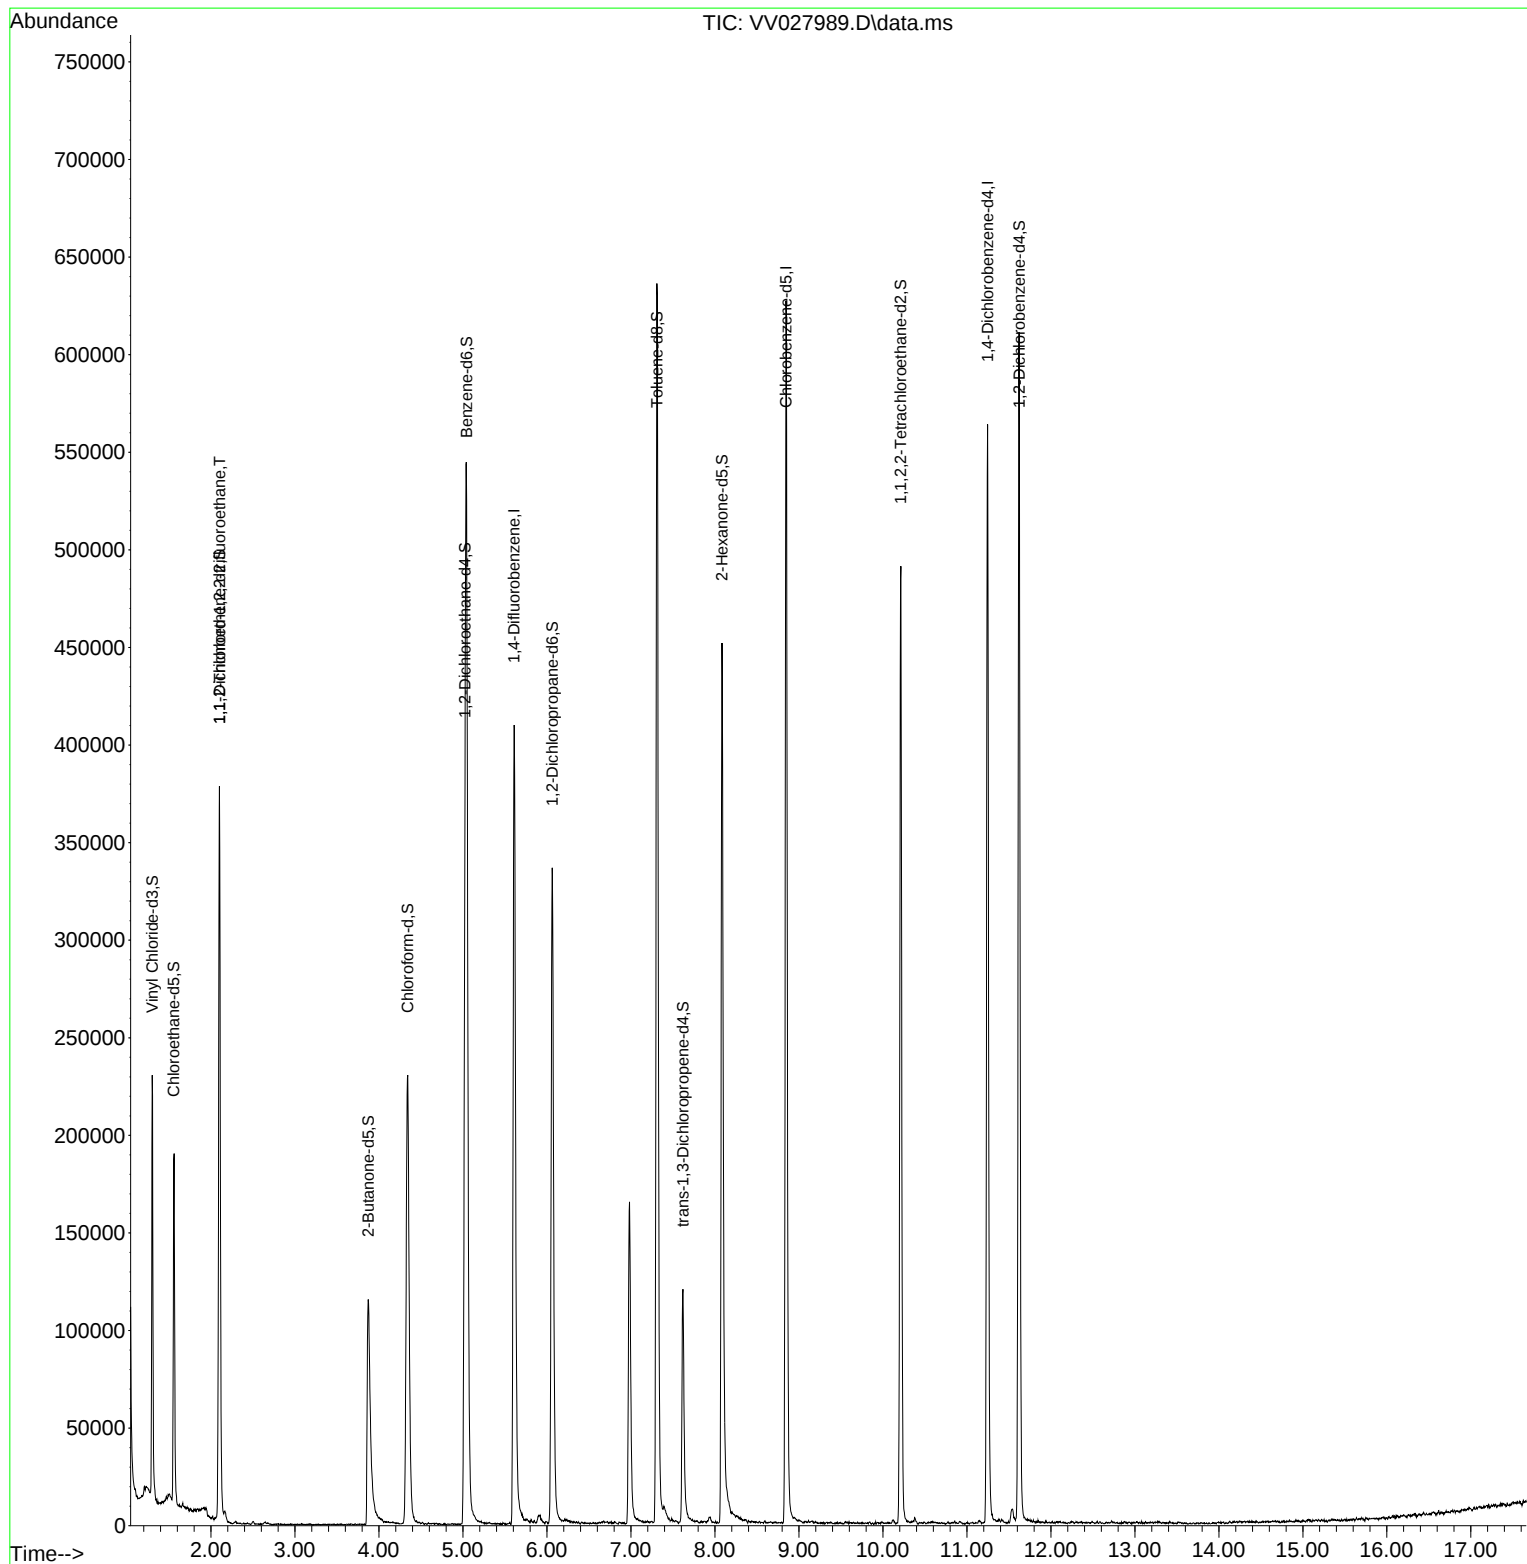

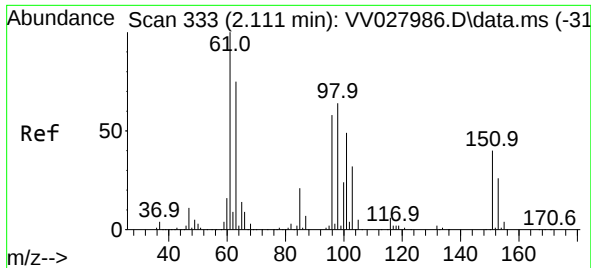

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.823 ug/L
 RT: 2.101 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV027989.D
 Acq: 21 Sep 2022 02:39

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E97

Tgt Ion:101 Resp: 2134
 Ion Ratio Lower Upper
 101 100
 85 1.9 35.6 53.4#
 151 3.6 62.2 93.4#

