

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027994.D
 Acq On : 21 Sep 2022 04:43
 Operator : SY/MD
 Sample : N4674-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA4

Quant Time: Sep 21 08:06:05 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 21 06:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.613	114	357109	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	344653	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	152454	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	134394	42.869	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.740%		
7) Chloroethane-d5	1.558	69	115108	45.963	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	91.920%		
11) 1,1-Dichloroethene-d2	2.101	63	186728	33.621	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	67.240%		
21) 2-Butanone-d5	3.873	46	216339	116.049	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	116.050%		
24) Chloroform-d	4.339	84	252055	47.888	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	95.780%		
26) 1,2-Dichloroethane-d4	5.024	65	168503	49.400	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.800%		
32) Benzene-d6	5.043	84	487408	49.065	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	98.140%		
36) 1,2-Dichloropropane-d6	6.063	67	159885	52.122	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	104.240%		
41) Toluene-d8	7.310	98	397143	43.657	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.320%		
43) trans-1,3-Dichloroprop...	7.619	79	63734	41.549	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	83.100%		
47) 2-Hexanone-d5	8.085	63	155932	103.765	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	103.760%		
56) 1,1,2,2-Tetrachloroeth...	10.210	84	230415	51.033	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	102.060%		
66) 1,2-Dichlorobenzene-d4	11.622	152	155715	52.616	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.240%		
Target Compounds						Qvalue
10) 1,1,2-Trichloro-1,2,2-...	2.101	101	1863	0.719	ug/L	# 18


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027994.D
Acq On : 21 Sep 2022 04:43
Operator : SY/MD
Sample : N4674-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA4

Quant Time: Sep 21 08:06:05 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 21 06:45:13 2022
Response via : Initial Calibration

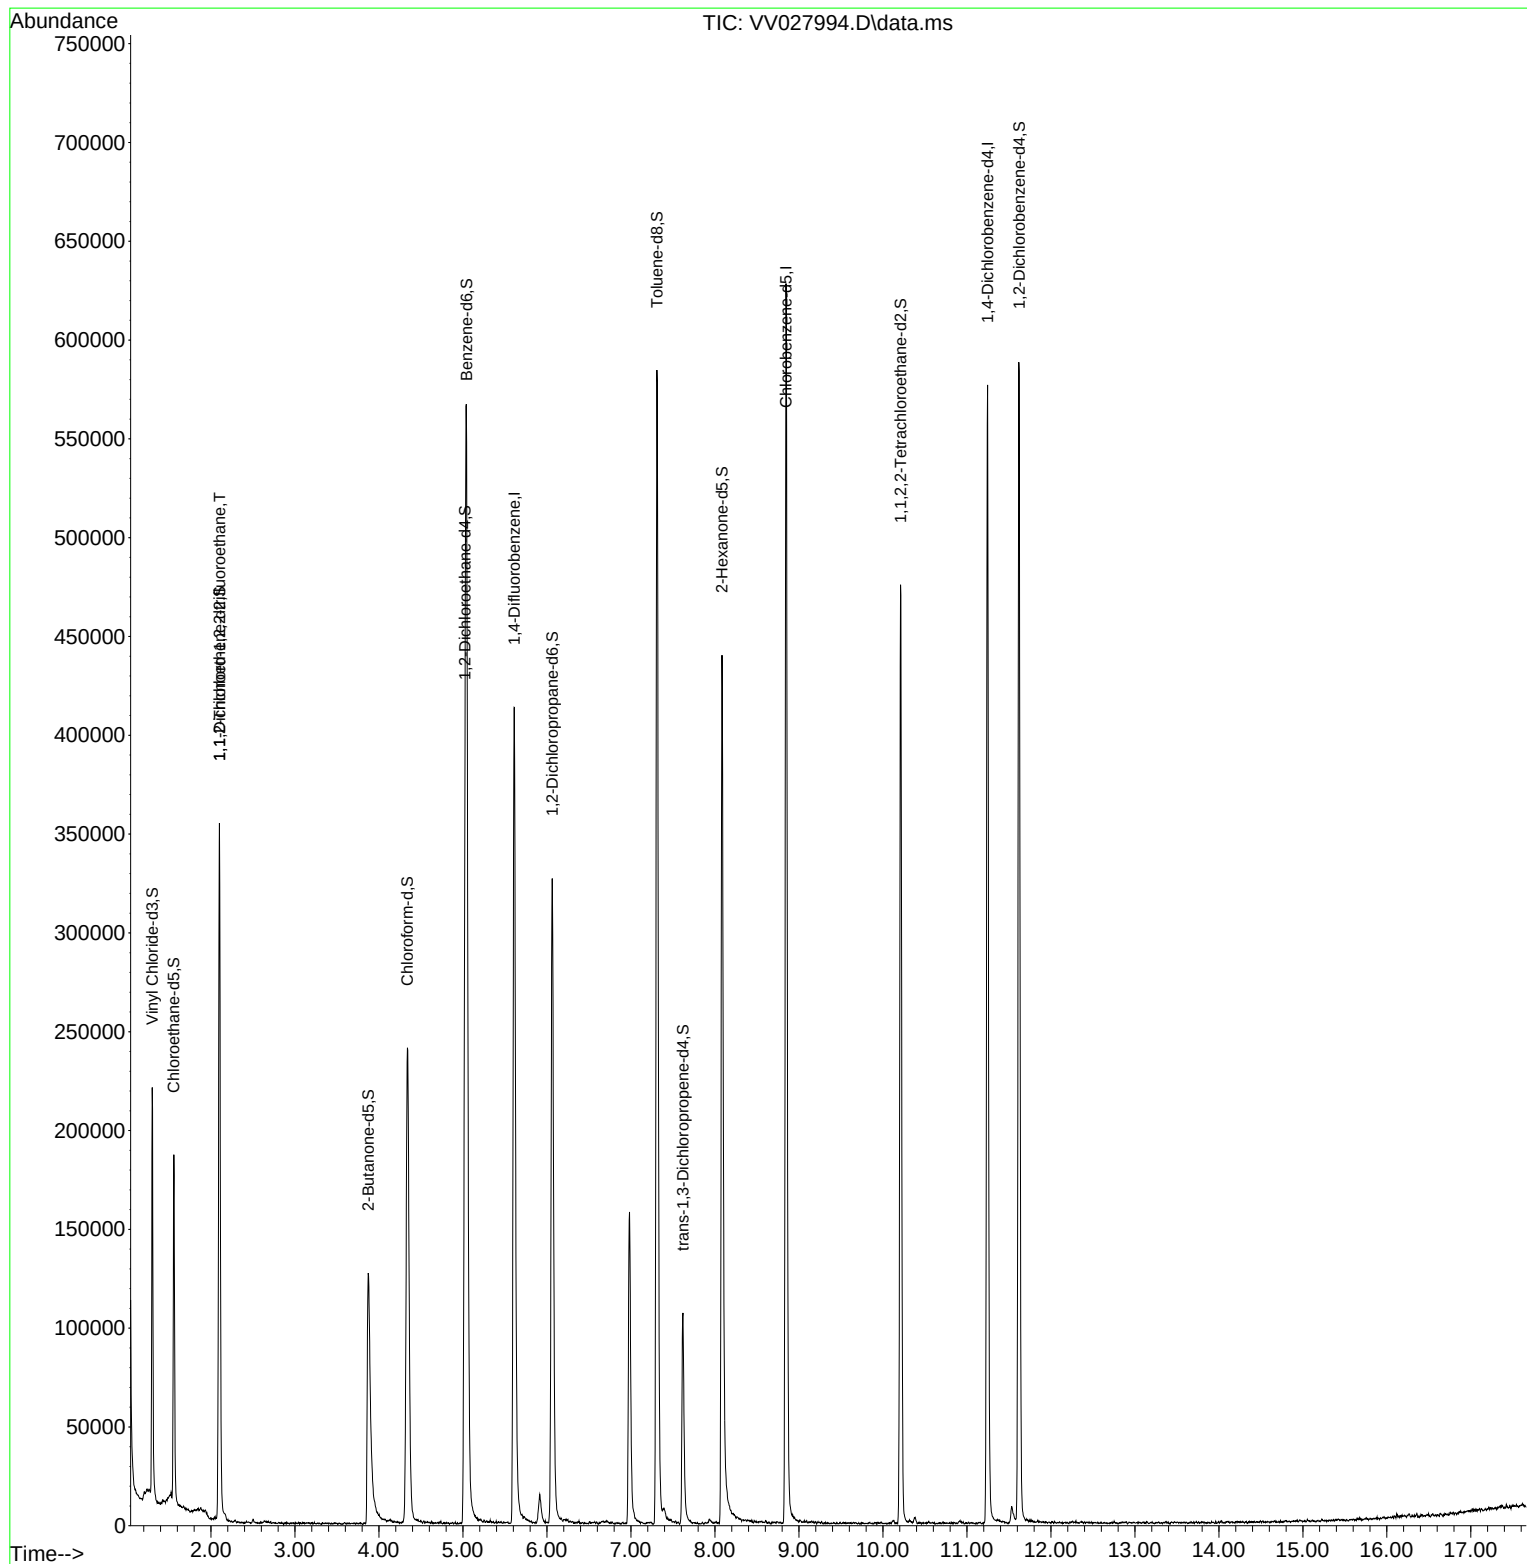

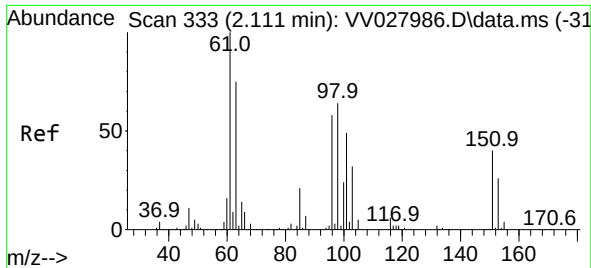

#10
 1,1,2-Trichloro-1,2,2-trifluoroethane
 Concen: 0.719 ug/L
 RT: 2.101 min Scan# 31
 Delta R.T. -0.010 min
 Lab File: VV027994.D
 Acq: 21 Sep 2022 04:43

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA4

Tgt Ion:101 Resp: 1863
 Ion Ratio Lower Upper
 101 100
 85 0.0 35.6 53.4#
 151 0.0 62.2 93.4#

