

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV028004.D
 Acq On : 21 Sep 2022 08:49
 Operator : SY/MD
 Sample : N4674-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 51 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EC3

Quant Time: Sep 21 17:41:41 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 21 06:45:13 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.612	114	328529	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.850	117	312883	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	141168	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	123003	42.648	ug/L	0.00
Spiked Amount 50.000	Range 60 - 135		Recovery =	85.300%		
7) Chloroethane-d5	1.561	69	107956	46.857	ug/L	0.00
Spiked Amount 50.000	Range 70 - 130		Recovery =	93.720%		
11) 1,1-Dichloroethene-d2	2.101	63	170810	33.431	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	66.860%		
21) 2-Butanone-d5	3.876	46	166590	97.136	ug/L	0.00
Spiked Amount 100.000	Range 40 - 130		Recovery =	97.140%		
24) Chloroform-d	4.339	84	222781	46.008	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	92.020%		
26) 1,2-Dichloroethane-d4	5.024	65	143488	45.726	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	91.460%		
32) Benzene-d6	5.043	84	425454	47.177	ug/L	0.00
Spiked Amount 50.000	Range 70 - 125		Recovery =	94.360%		
36) 1,2-Dichloropropane-d6	6.063	67	130714	46.939	ug/L	0.00
Spiked Amount 50.000	Range 70 - 120		Recovery =	93.880%		
41) Toluene-d8	7.310	98	360215	43.618	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	87.240%		
43) trans-1,3-Dichloroprop...	7.619	79	57387	41.210	ug/L	0.00
Spiked Amount 50.000	Range 60 - 125		Recovery =	82.420%		
47) 2-Hexanone-d5	8.085	63	134775	98.793	ug/L	0.00
Spiked Amount 100.000	Range 45 - 130		Recovery =	98.790%		
56) 1,1,2,2-Tetrachloroeth...	10.210	84	190496	46.476	ug/L	0.00
Spiked Amount 50.000	Range 65 - 120		Recovery =	92.960%		
66) 1,2-Dichlorobenzene-d4	11.622	152	145154	52.968	ug/L	0.00
Spiked Amount 50.000	Range 80 - 120		Recovery =	105.940%		
Target Compounds						Qvalue
61) 1,2,3-Trichloropropane	11.246	75	13842	5.224	ug/L	# 67


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV028004.D
Acq On : 21 Sep 2022 08:49
Operator : SY/MD
Sample : N4674-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 51 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EC3

Quant Time: Sep 21 17:41:41 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 21 06:45:13 2022
Response via : Initial Calibration

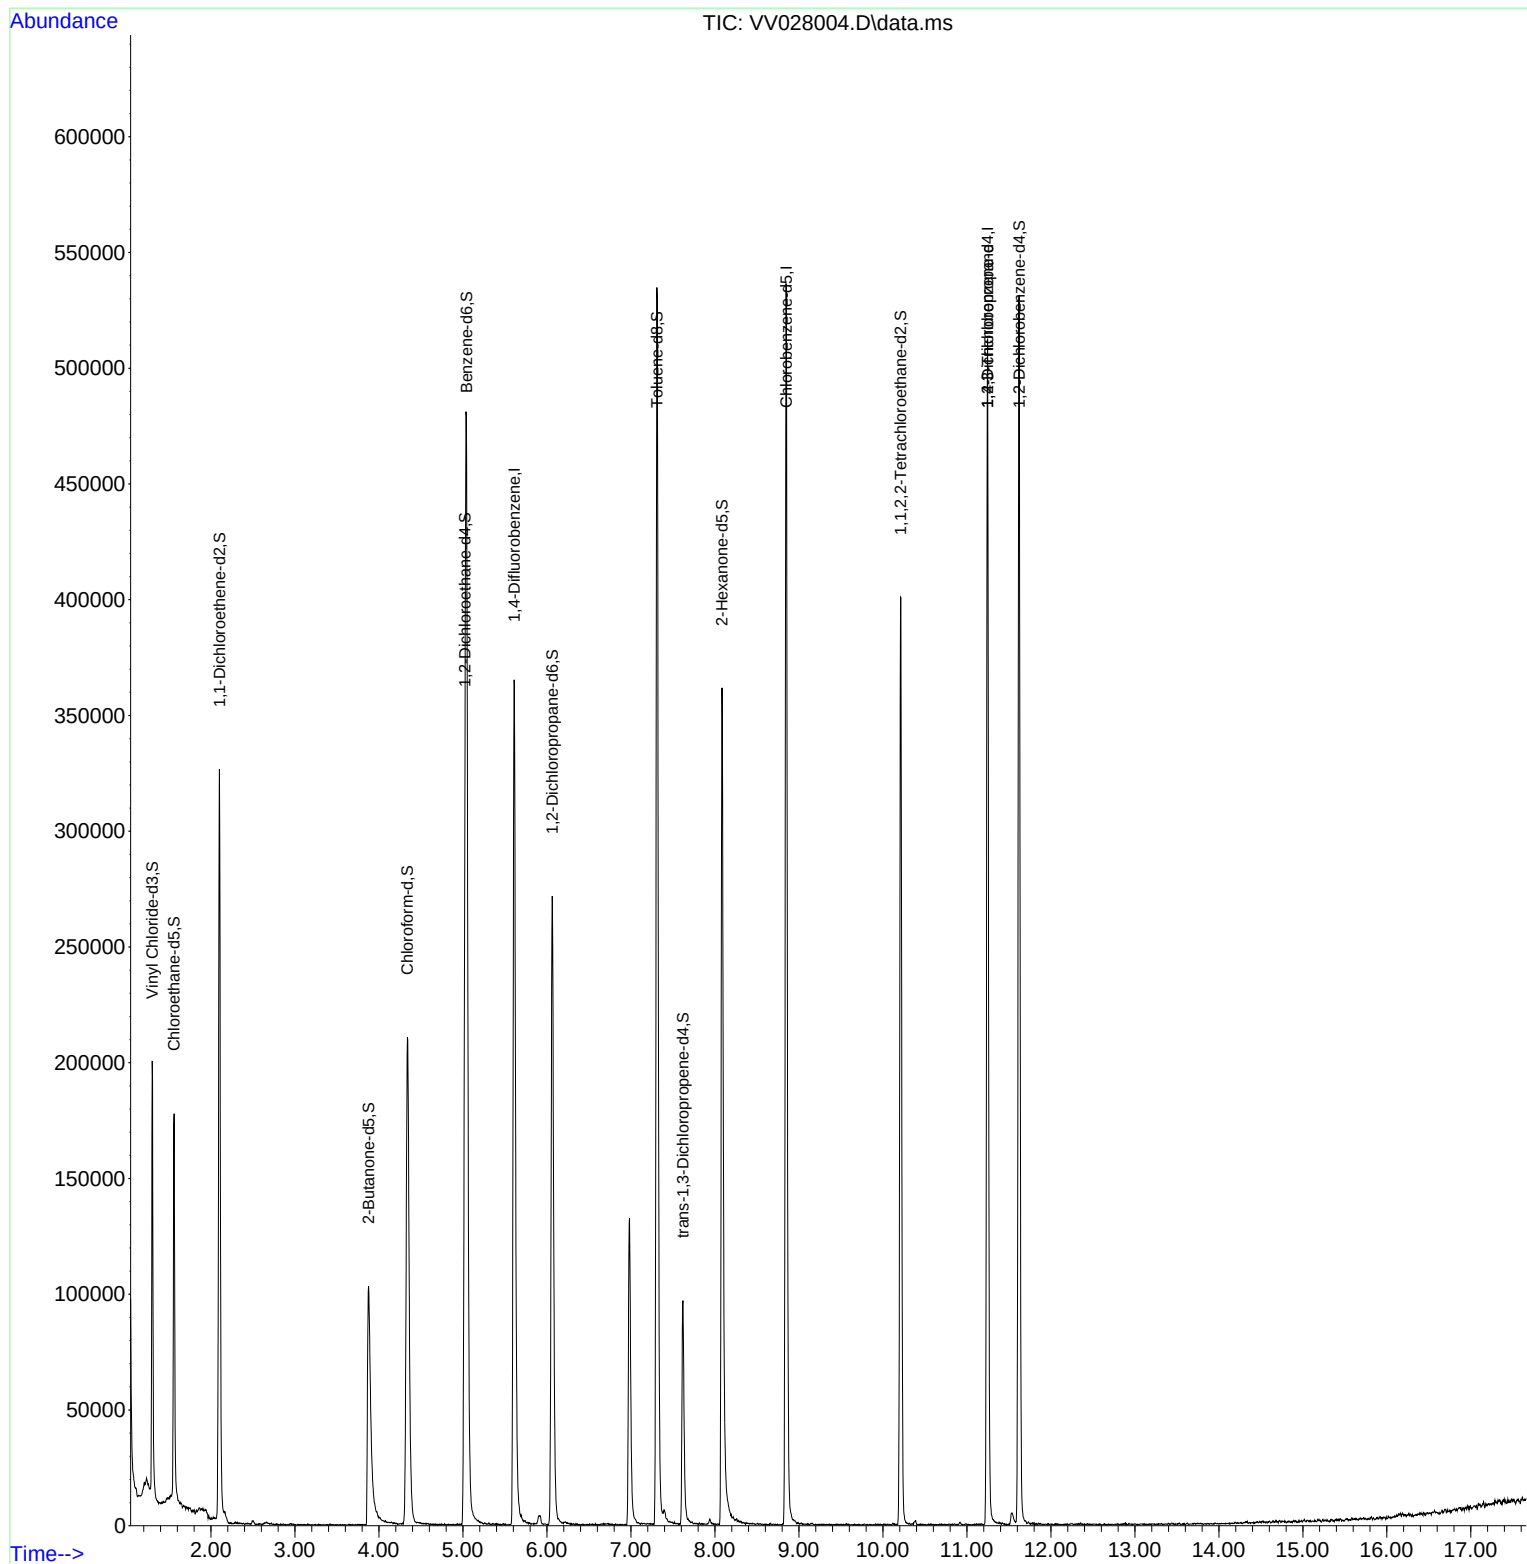

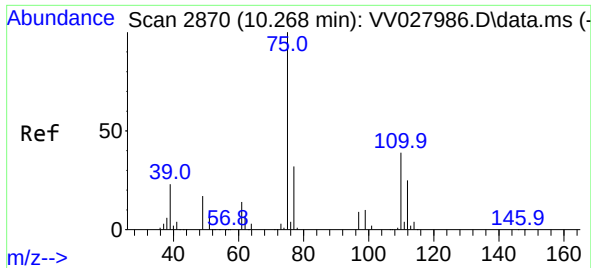

#61
1,2,3-Trichloropropane
Concen: 5.224 ug/L
RT: 11.246 min Scan# 31
Delta R.T. 0.977 min
Lab File: VV028004.D
Acq: 21 Sep 2022 08:49

Instrument :
MSVOA_V
ClientSampleId :
C0EC3

Tgt Ion: 75 Resp: 13842
Ion Ratio Lower Upper
75 100
77 30.4 25.9 38.9
110 3.9 31.1 46.7#

