

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027965.D
 Acq On : 20 Sep 2022 16:20
 Operator : SY/MD
 Sample : N4619-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E13

Quant Time: Sep 21 05:15:35 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 21 01:52:39 2022
 Response via : Initial Calibration

Compound	R.T. QIon		Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	328306	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	326664	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	150798	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	160790	55.788	ug/L	0.00
Spiked Amount	50.000	Range 60 - 135	Recovery	= 111.580%		
7) Chloroethane-d5	1.552	69	128476	55.801	ug/L	0.00
Spiked Amount	50.000	Range 70 - 130	Recovery	= 111.600%		
11) 1,1-Dichloroethene-d2	2.098	63	221720	43.424	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 86.840%		
21) 2-Butanone-d5	3.867	46	189631	110.646	ug/L	0.00
Spiked Amount	100.000	Range 40 - 130	Recovery	= 110.650%		
24) Chloroform-d	4.336	84	258577	53.437	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 106.880%		
26) 1,2-Dichloroethane-d4	5.021	65	174982	55.800	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 111.600%		
32) Benzene-d6	5.040	84	519075	55.130	ug/L	0.00
Spiked Amount	50.000	Range 70 - 125	Recovery	= 110.260%		
36) 1,2-Dichloropropane-d6	6.063	67	164771	56.673	ug/L	0.00
Spiked Amount	50.000	Range 70 - 120	Recovery	= 113.340%		
41) Toluene-d8	7.310	98	483490	56.076	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	= 112.160%		
43) trans-1,3-Dichloroprop...	7.616	79	83747	57.602	ug/L	0.00
Spiked Amount	50.000	Range 60 - 125	Recovery	= 115.200%		
47) 2-Hexanone-d5	8.082	63	164662	115.608	ug/L	0.00
Spiked Amount	100.000	Range 45 - 130	Recovery	= 115.610%		
56) 1,1,2,2-Tetrachloroeth...	10.214	84	248352	58.035	ug/L	0.00
Spiked Amount	50.000	Range 65 - 120	Recovery	= 116.060%		
66) 1,2-Dichlorobenzene-d4	11.622	152	185804	63.472	ug/L	0.00
Spiked Amount	50.000	Range 80 - 120	Recovery	#126.940%		
Target Compounds						Qvalue
13) Acetone	2.156	43	4390	2.874	ug/L	91


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027965.D
Acq On : 20 Sep 2022 16:20
Operator : SY/MD
Sample : N4619-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E13

Quant Time: Sep 21 05:15:35 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 21 01:52:39 2022
Response via : Initial Calibration

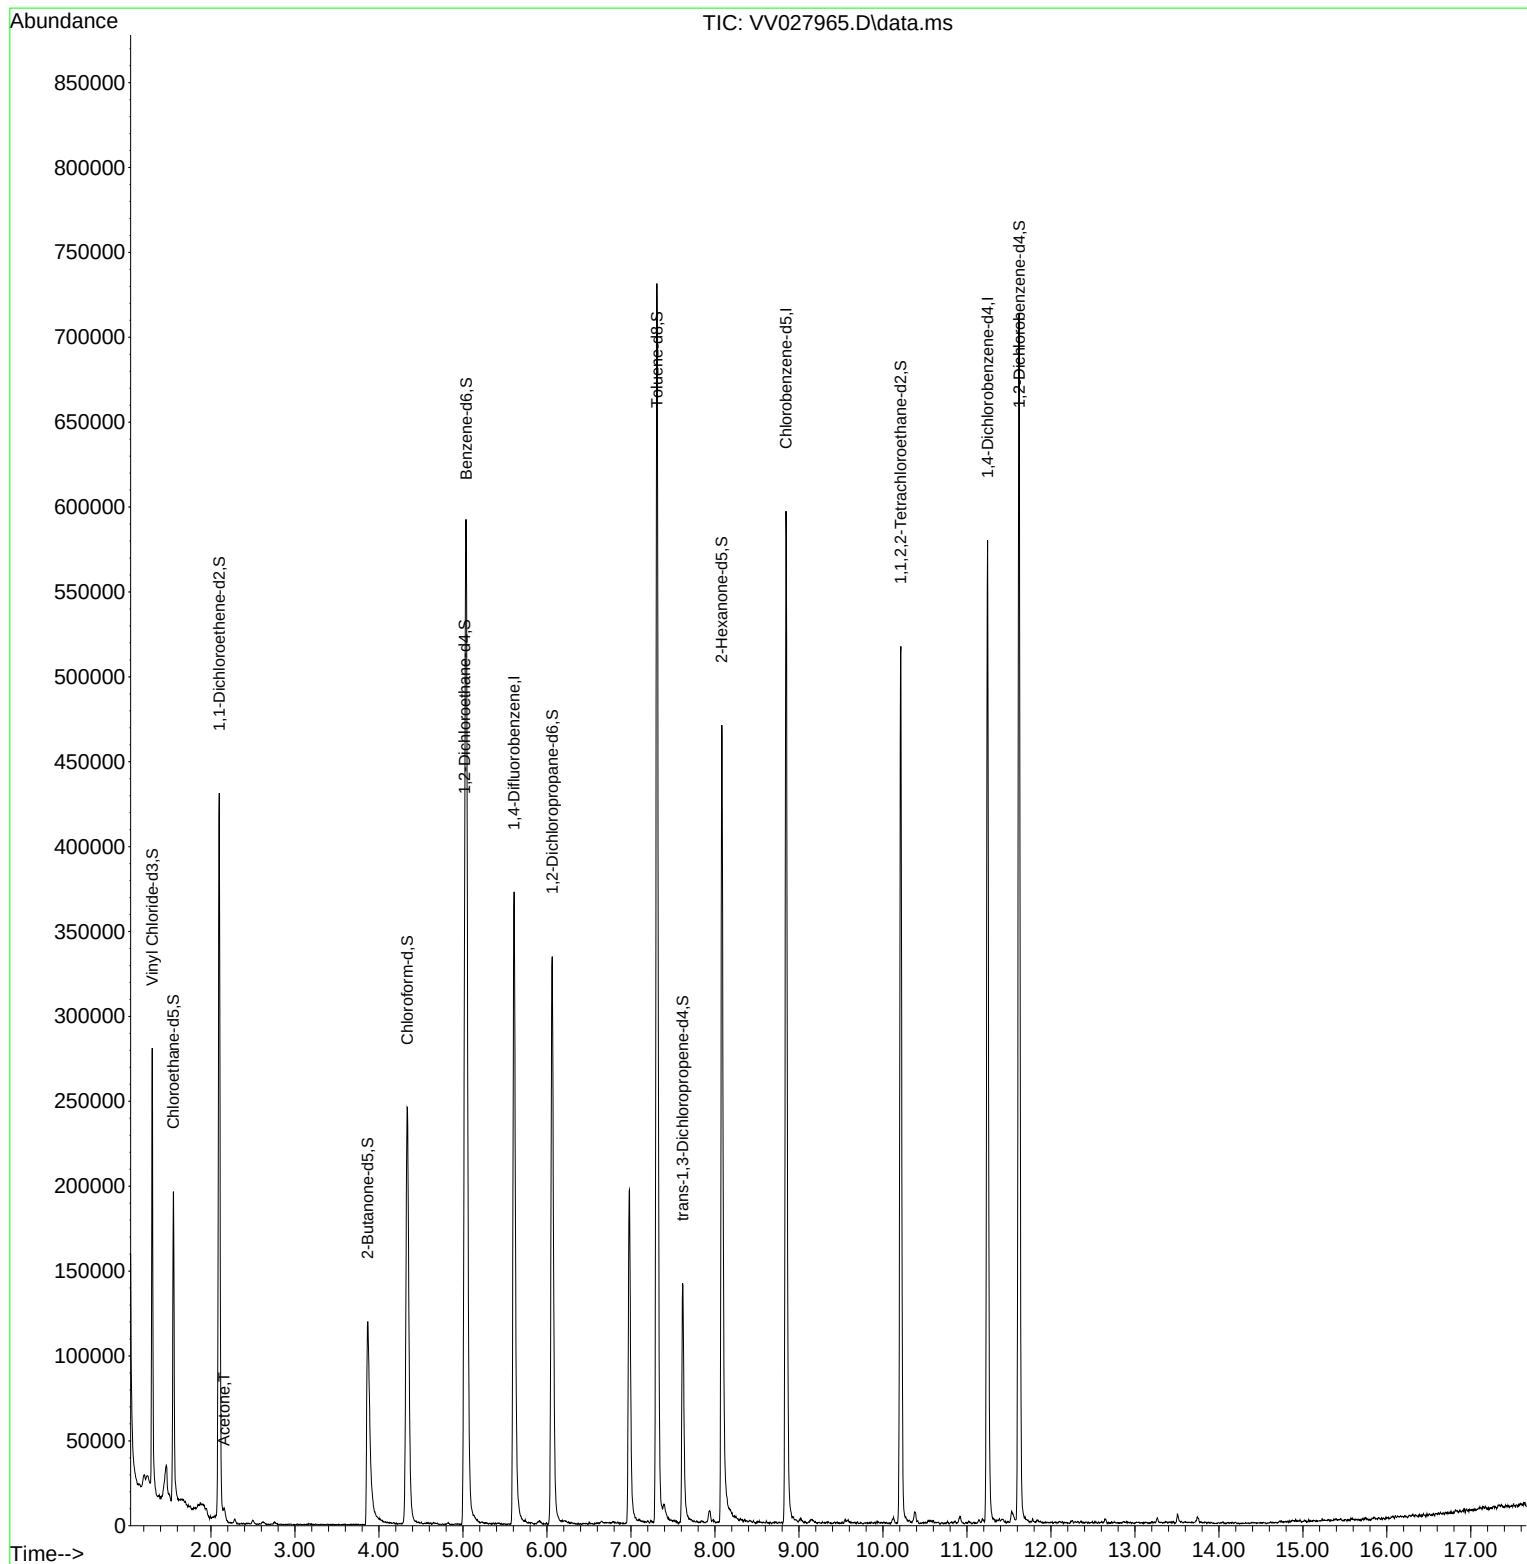

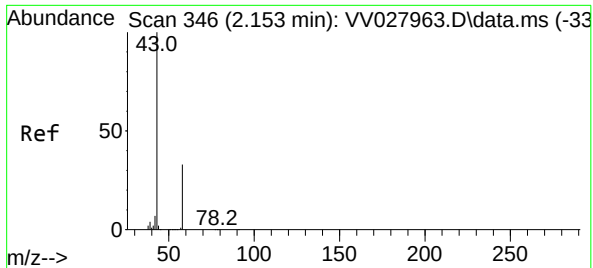

#13
 Acetone
 Concen: 2.874 ug/L
 RT: 2.156 min Scan# 34
 Delta R.T. 0.003 min
 Lab File: VV027965.D
 Acq: 20 Sep 2022 16:20

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E13

Tgt Ion: 43 Resp: 4390
 Ion Ratio Lower Upper
 43 100
 58 27.8 0.0 66.2

