

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027981.D
 Acq On : 20 Sep 2022 22:57
 Operator : SY/MD
 Sample : N4619-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E37

Quant Time: Sep 21 05:18:36 2022
 Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Quant Title : VOC Analysis
 QLast Update : Wed Sep 21 01:52:39 2022
 Response via : Initial Calibration

Compound	R.T.	QIon	Response	Conc	Units	Dev(Min)


Internal Standards						
1) 1,4-Difluorobenzene	5.609	114	355402	50.000	ug/L	0.00
28) Chlorobenzene-d5	8.847	117	342947	50.000	ug/L	0.00
58) 1,4-Dichlorobenzene-d4	11.246	152	154009	50.000	ug/L	0.00
System Monitoring Compounds						
4) Vinyl Chloride-d3	1.301	65	142694	45.735	ug/L	0.00
Spiked Amount	50.000	Range	60 - 135	Recovery	=	91.460%
7) Chloroethane-d5	1.555	69	116977	46.933	ug/L	0.00
Spiked Amount	50.000	Range	70 - 130	Recovery	=	93.860%
11) 1,1-Dichloroethene-d2	2.098	63	198693	35.947	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	71.900%
21) 2-Butanone-d5	3.867	46	184631	99.515	ug/L	0.00
Spiked Amount	100.000	Range	40 - 130	Recovery	=	99.520%
24) Chloroform-d	4.339	84	239852	45.788	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	91.580%
26) 1,2-Dichloroethane-d4	5.024	65	172700	50.873	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.740%
32) Benzene-d6	5.040	84	502529	50.839	ug/L	0.00
Spiked Amount	50.000	Range	70 - 125	Recovery	=	101.680%
36) 1,2-Dichloropropane-d6	6.063	67	166220	54.457	ug/L	0.00
Spiked Amount	50.000	Range	70 - 120	Recovery	=	108.920%
41) Toluene-d8	7.310	98	424765	46.926	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	93.860%
43) trans-1,3-Dichloroprop...	7.616	79	71838	47.065	ug/L	0.00
Spiked Amount	50.000	Range	60 - 125	Recovery	=	94.120%
47) 2-Hexanone-d5	8.085	63	156895	104.925	ug/L	0.00
Spiked Amount	100.000	Range	45 - 130	Recovery	=	104.920%
56) 1,1,2,2-Tetrachloroeth...	10.210	84	222157	49.449	ug/L	0.00
Spiked Amount	50.000	Range	65 - 120	Recovery	=	98.900%
66) 1,2-Dichlorobenzene-d4	11.622	152	165830	55.468	ug/L	0.00
Spiked Amount	50.000	Range	80 - 120	Recovery	=	110.940%
Target Compounds						
13) Acetone	2.156	43	9703	5.868	ug/L	Qvalue 99


(#) = qualifier out of range (m) = manual integration (+) = signals summed

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027981.D
Acq On : 20 Sep 2022 22:57
Operator : SY/MD
Sample : N4619-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E37

Quant Time: Sep 21 05:18:36 2022
Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis
QLast Update : Wed Sep 21 01:52:39 2022
Response via : Initial Calibration

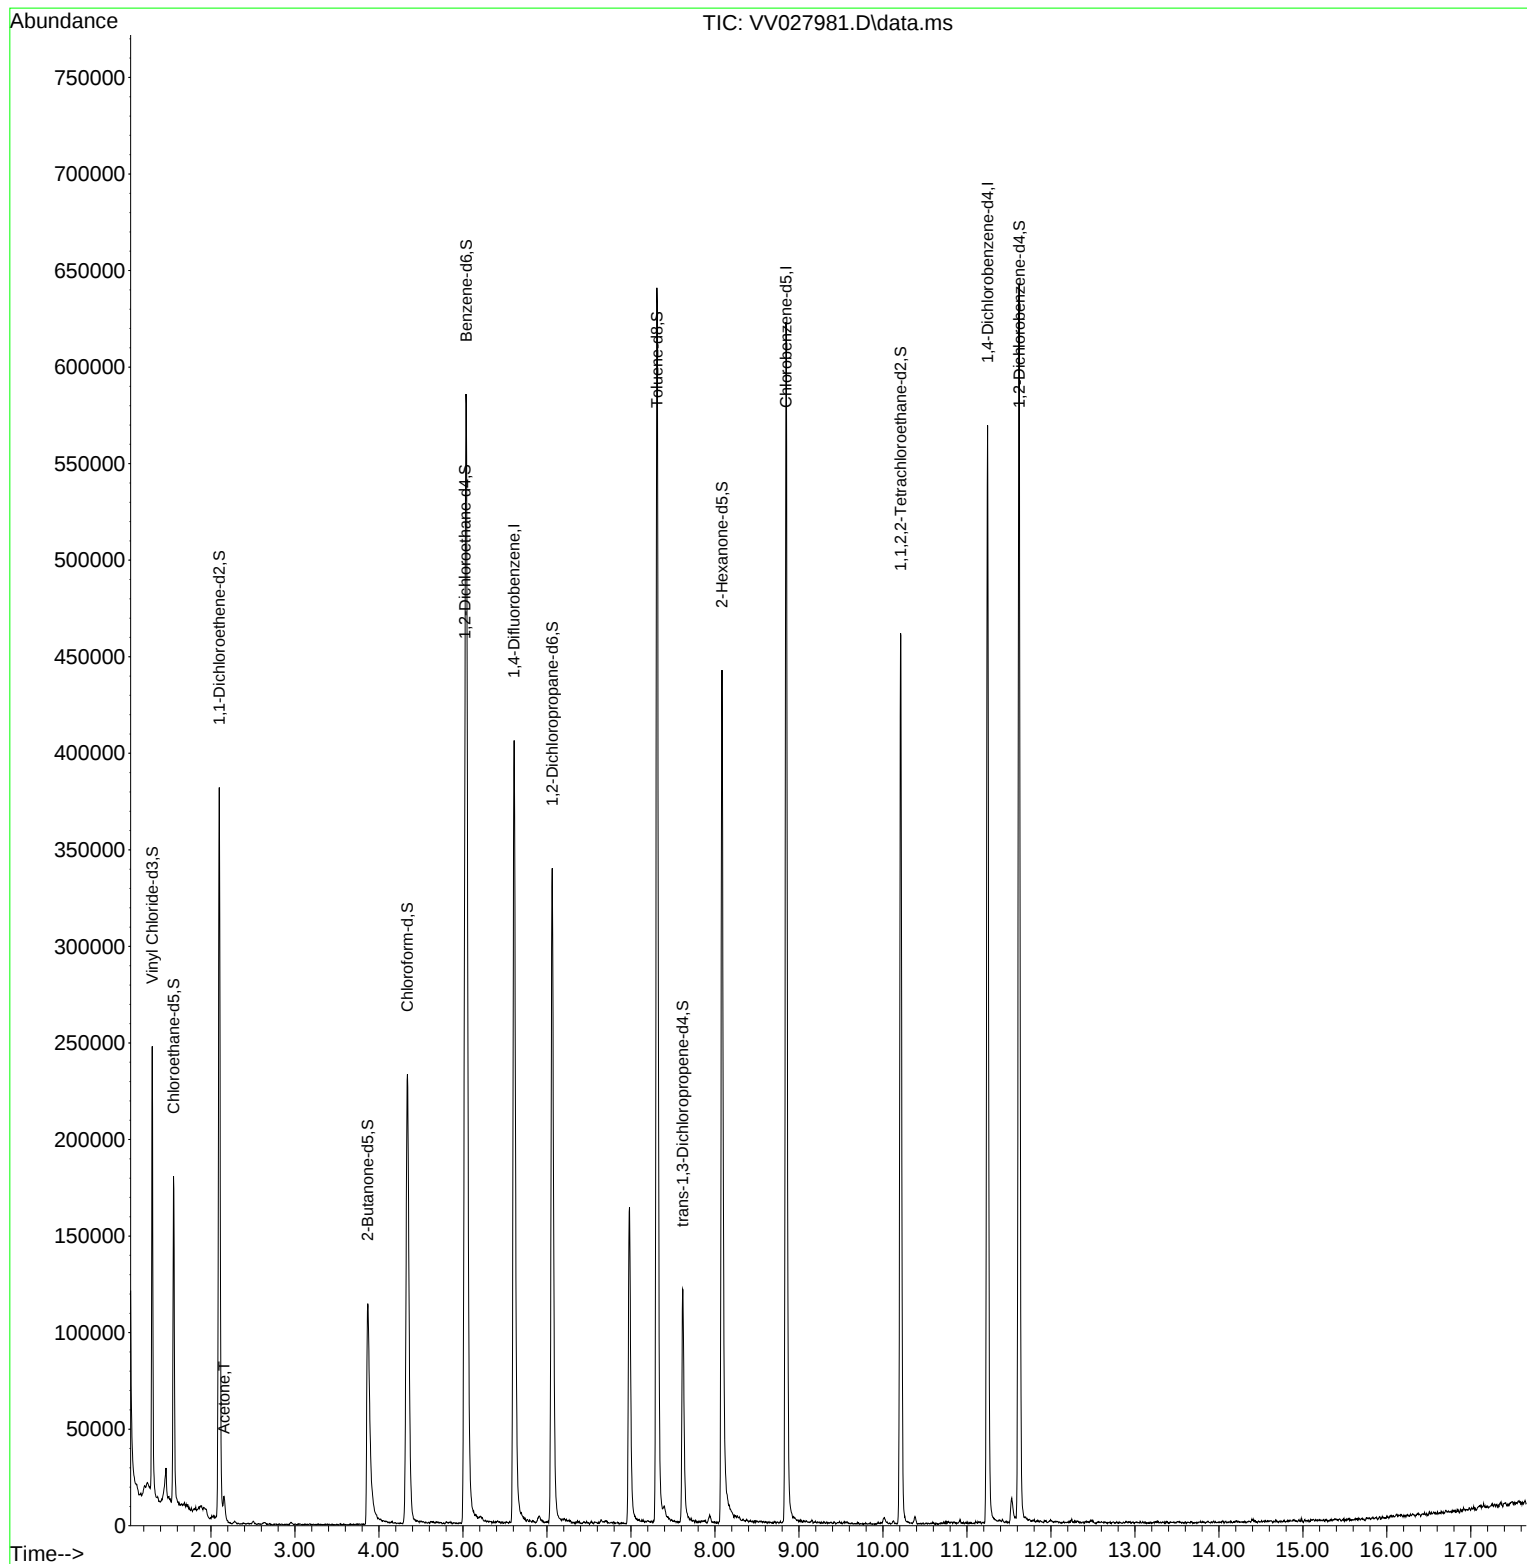

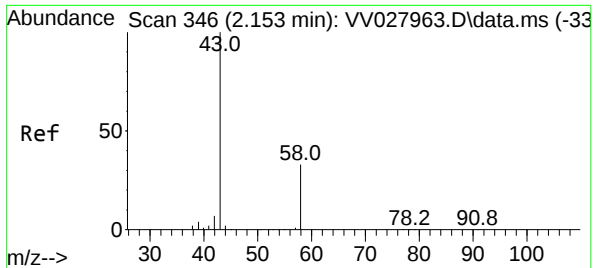

#13

Acetone

Concen: 5.868 ug/L

RT: 2.156 min Scan# 34

Delta R.T. 0.003 min

Lab File: VV027981.D


Acq: 20 Sep 2022 22:57

Instrument :

MSVOA_V

ClientSampleId :

C0E37

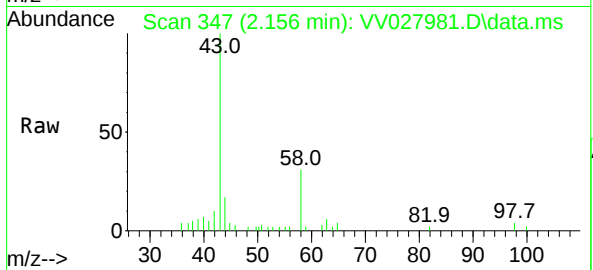

Tgt Ion: 43 Resp: 9703

Ion Ratio Lower Upper

43 100

58 32.4 0.0 66.2

