

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027964.D
 Acq On : 20 Sep 2022 15:52
 Operator : SY/MD
 Sample : VV0920WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027964.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	250647	258205	16.31%	2.202%
2	1.555	154	160	185	rVB	179202	216538	13.68%	1.846%
3	2.098	320	329	345	rBV	408893	585113	36.97%	4.989%
4	2.281	380	386	392	rBV3	2548	3863	0.24%	0.033%
5	2.426	429	431	435	rBV3	613	467	0.03%	0.004%
6	2.500	446	454	466	rVV4	5991	11217	0.71%	0.096%
7	2.548	466	469	470	rVB	394	187	0.01%	0.002%
8	2.632	493	495	496	rBV	306	116	0.01%	0.001%
9	2.706	514	518	521	rBV3	610	502	0.03%	0.004%
10	2.738	526	528	530	rVV3	520	260	0.02%	0.002%
11	2.757	530	534	543	rVB7	1223	1703	0.11%	0.015%
12	2.793	543	545	547	rBV	406	167	0.01%	0.001%
13	2.831	552	557	562	rBV2	766	609	0.04%	0.005%
14	2.867	566	568	569	rBV	357	144	0.01%	0.001%
15	2.905	578	580	582	rBV2	550	222	0.01%	0.002%
16	2.918	582	584	585	rVV	336	108	0.01%	0.001%
17	2.928	585	587	590	rVV2	358	211	0.01%	0.002%
18	2.992	605	607	609	rBV	354	194	0.01%	0.002%
19	3.040	621	622	624	rVB2	359	115	0.01%	0.001%
20	3.162	658	660	662	rBV	167	106	0.01%	0.001%
21	3.207	671	674	678	rVB	665	448	0.03%	0.004%
22	3.240	681	684	686	rBV	294	176	0.01%	0.002%
23	3.265	690	692	693	rBV	134	73	0.00%	0.001%
24	3.275	693	695	697	rVV	203	104	0.01%	0.001%
25	3.288	697	699	707	rVB3	442	423	0.03%	0.004%
26	3.368	722	724	726	rBV2	284	114	0.01%	0.001%
27	3.387	728	730	734	rVB	385	259	0.02%	0.002%
28	3.416	737	739	740	rBV	524	238	0.02%	0.002%
29	3.461	750	753	757	rVV2	439	305	0.02%	0.003%
30	3.494	761	763	765	rVB	190	84	0.01%	0.001%
31	3.513	765	769	772	rVB	499	315	0.02%	0.003%
32	3.529	772	774	775	rBV	192	101	0.01%	0.001%
33	3.535	775	776	779	rVV2	236	84	0.01%	0.001%
34	3.551	779	781	782	rVB2	509	184	0.01%	0.002%
35	3.567	782	786	789	rBV2	425	257	0.02%	0.002%
36	3.587	789	792	796	rVB3	441	260	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027964.D
 Acq On : 20 Sep 2022 15:52
 Operator : SY/MD
 Sample : VV0920WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.603	796	797	800	rBV2	382	140	0.01%	0.001%
38	3.622	800	803	805	rBV	193	130	0.01%	0.001%
39	3.632	805	806	807	rVB	213	41	0.00%	0.000%
40	3.645	808	810	813	rBV2	252	86	0.01%	0.001%
41	3.696	824	826	827	rBV	317	116	0.01%	0.001%
42	3.715	830	832	834	rBB2	249	85	0.01%	0.001%
43	3.738	838	839	842	rBV	218	99	0.01%	0.001%
44	3.754	842	844	847	rBV3	260	137	0.01%	0.001%
45	3.802	858	859	860	rVB	229	44	0.00%	0.000%
46	3.815	860	863	865	rBV	445	199	0.01%	0.002%
47	3.867	869	879	919	rBV	127857	343219	21.68%	2.927%
48	4.259	999	1001	1004	rBV3	598	227	0.01%	0.002%
49	4.339	1010	1026	1051	rBV2	243152	603315	38.12%	5.144%
50	5.037	1227	1243	1269	rBV2	622616	1582798	100.00%	13.496%
51	5.609	1409	1421	1445	rBV	426863	869883	54.96%	7.417%
52	6.063	1549	1562	1583	rBV	354260	722371	45.64%	6.159%
53	6.519	1702	1704	1705	rVB	613	234	0.01%	0.002%
54	6.538	1705	1710	1711	rBV3	951	790	0.05%	0.007%
55	6.850	1806	1807	1811	rVB3	767	273	0.02%	0.002%
56	6.911	1823	1826	1828	rBV2	740	286	0.02%	0.002%
57	6.982	1838	1848	1873	rBV	190657	349126	22.06%	2.977%
58	7.310	1939	1950	1971	rBV	679258	1196520	75.60%	10.202%
59	7.619	2034	2046	2065	rBV	129977	232471	14.69%	1.982%
60	8.085	2181	2191	2222	rBV	485229	861260	54.41%	7.344%
61	8.850	2418	2429	2456	rBV	640723	1066012	67.35%	9.090%
62	9.288	2562	2565	2570	rVB6	1292	1281	0.08%	0.011%
63	9.448	2612	2615	2618	rBV4	1238	924	0.06%	0.008%
64	9.516	2633	2636	2638	rBV2	843	618	0.04%	0.005%
65	9.908	2756	2758	2760	rBV2	980	680	0.04%	0.006%
66	9.995	2783	2785	2787	rBV	597	322	0.02%	0.003%
67	10.214	2841	2853	2870	rBV	510469	801235	50.62%	6.832%
68	10.490	2933	2939	2942	rBV4	565	572	0.04%	0.005%
69	10.516	2946	2947	2949	rBV2	623	182	0.01%	0.002%
70	10.532	2949	2952	2954	rBV3	1432	1014	0.06%	0.009%
71	10.667	2989	2994	2998	rBV3	731	776	0.05%	0.007%
72	10.696	3001	3003	3005	rVB	655	218	0.01%	0.002%
73	10.738	3013	3016	3019	rBV4	506	329	0.02%	0.003%
74	10.754	3019	3021	3023	rBV2	513	196	0.01%	0.002%
75	10.824	3041	3043	3046	rBV3	612	285	0.02%	0.002%
76	10.847	3048	3050	3058	rVB4	1039	1032	0.07%	0.009%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027964.D
 Acq On : 20 Sep 2022 15:52
 Operator : SY/MD
 Sample : VV0920WBL01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 VBLK264

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.918	3062	3072	3078	rBV9	4447	6251	0.39%	0.053%
78	10.966	3085	3087	3089	rVB2	396	102	0.01%	0.001%
79	10.976	3089	3090	3094	rVB3	494	277	0.02%	0.002%
80	11.004	3096	3099	3103	rVB	830	551	0.03%	0.005%
81	11.033	3103	3108	3110	rBV3	1133	1008	0.06%	0.009%
82	11.069	3117	3119	3123	rBV3	616	418	0.03%	0.004%
83	11.088	3123	3125	3127	rVB2	663	245	0.02%	0.002%
84	11.098	3127	3128	3130	rBV	603	271	0.02%	0.002%
85	11.185	3151	3155	3163	rVB7	2893	2949	0.19%	0.025%
86	11.246	3163	3174	3192	rBV	600124	924247	58.39%	7.881%
87	11.622	3278	3291	3309	rBV	676563	1055631	66.69%	9.001%
88	12.133	3448	3450	3452	rBV2	950	614	0.04%	0.005%
89	12.197	3468	3470	3472	rVB2	652	196	0.01%	0.002%
90	12.320	3506	3508	3511	rBV2	927	636	0.04%	0.005%
91	12.754	3641	3643	3646	rVB2	937	417	0.03%	0.004%
92	13.329	3818	3822	3825	rVB2	1044	760	0.05%	0.006%
93	13.374	3833	3836	3839	rBV3	1125	718	0.05%	0.006%
94	13.509	3872	3878	3888	rVB4	5851	9167	0.58%	0.078%
95	13.657	3922	3924	3928	rVB2	1036	444	0.03%	0.004%




Sum of corrected areas: 11727900

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027964.D
Acq On : 20 Sep 2022 15:52
Operator : SY/MD
Sample : VV0920WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

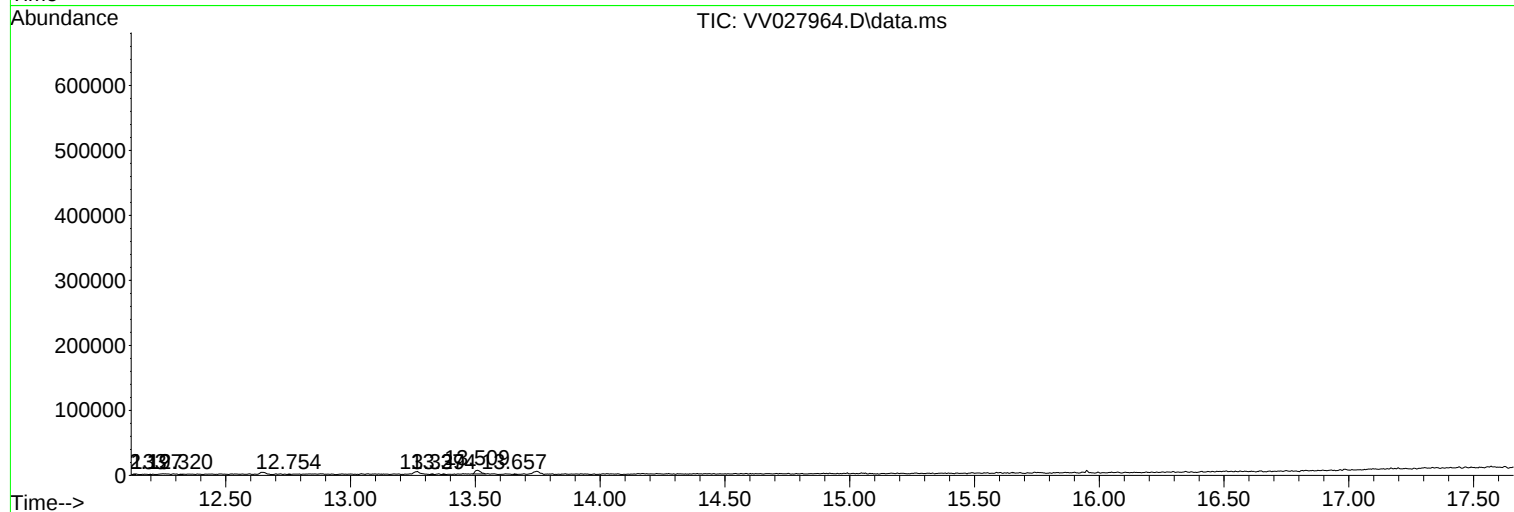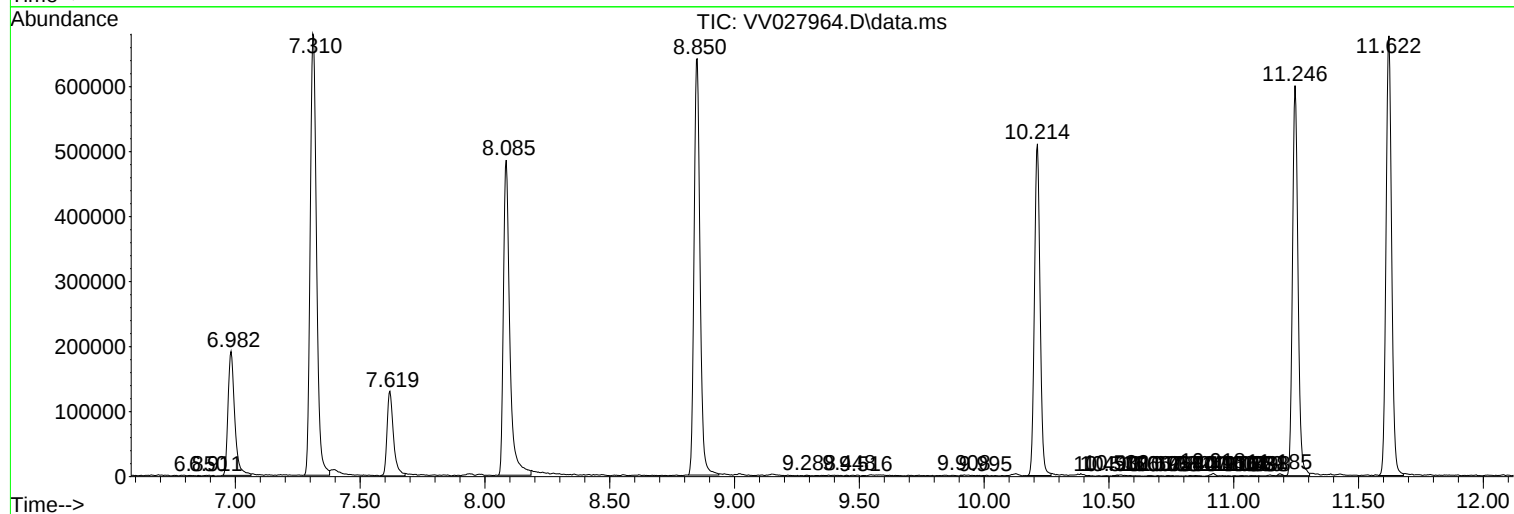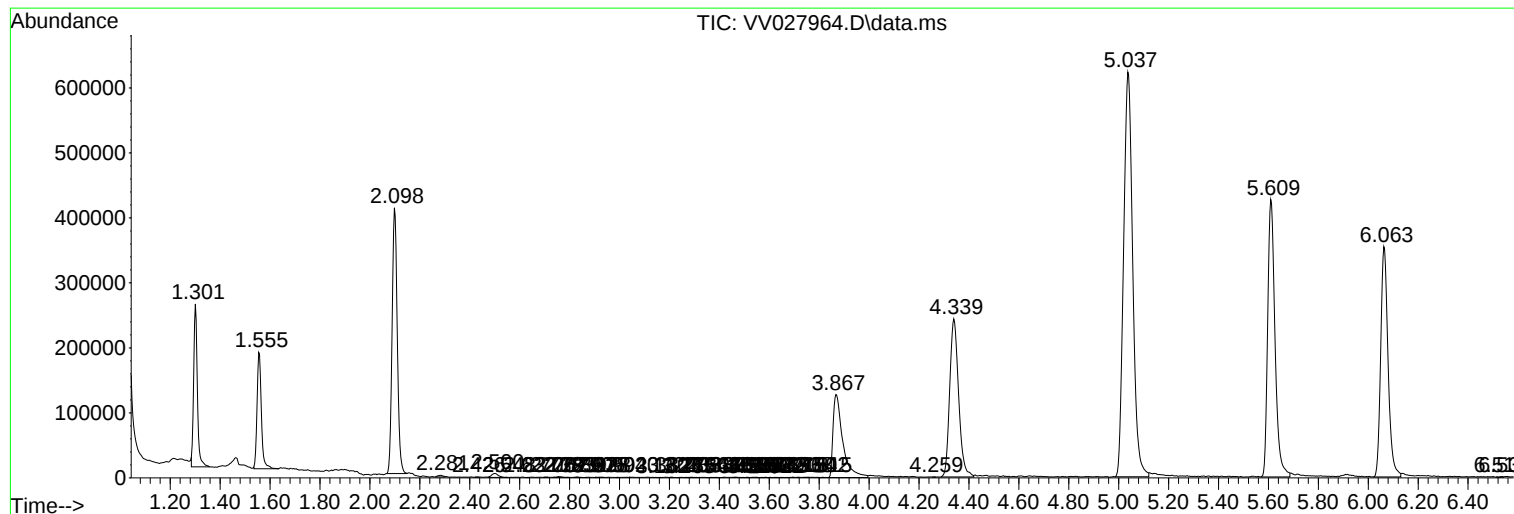

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027964.D
Acq On : 20 Sep 2022 15:52
Operator : SY/MD
Sample : VV0920WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027964.D
Acq On : 20 Sep 2022 15:52
Operator : SY/MD
Sample : VV0920WBL01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
VBLK264

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST20.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------