

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027965.D
 Acq On : 20 Sep 2022 16:20
 Operator : SY/MD
 Sample : N4619-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027965.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	100	rVB	264147	270850	17.76%	2.347%
2	1.552	153	159	178	rVB	181757	219646	14.41%	1.903%
3	2.098	320	329	343	rBV	422843	594235	38.97%	5.149%
4	2.497	447	453	467	rVB5	2508	4302	0.28%	0.037%
5	2.574	475	477	482	rBV	526	427	0.03%	0.004%
6	2.606	483	487	488	rBV2	908	553	0.04%	0.005%
7	2.658	502	503	505	rVB2	424	145	0.01%	0.001%
8	2.670	505	507	510	rVB3	341	173	0.01%	0.001%
9	2.687	510	512	515	rBV2	326	160	0.01%	0.001%
10	2.754	528	533	536	rBV5	1238	1171	0.08%	0.010%
11	2.889	573	575	576	rBV2	180	75	0.00%	0.001%
12	2.915	581	583	585	rBV2	257	137	0.01%	0.001%
13	2.989	604	606	608	rVB	324	144	0.01%	0.001%
14	3.015	610	614	615	rBV	240	156	0.01%	0.001%
15	3.027	615	618	622	rVB4	496	315	0.02%	0.003%
16	3.047	622	624	626	rBV	222	117	0.01%	0.001%
17	3.159	657	659	660	rBV	518	164	0.01%	0.001%
18	3.188	666	668	678	rVB4	548	568	0.04%	0.005%
19	3.224	678	679	681	rVB	272	86	0.01%	0.001%
20	3.246	681	686	689	rBV2	512	429	0.03%	0.004%
21	3.307	700	705	706	rBV	301	245	0.02%	0.002%
22	3.413	737	738	741	rVB2	277	114	0.01%	0.001%
23	3.429	741	743	746	rVB2	419	173	0.01%	0.001%
24	3.452	746	750	751	rBV	491	243	0.02%	0.002%
25	3.465	751	754	756	rVB2	349	216	0.01%	0.002%
26	3.474	756	757	760	rBV	364	238	0.02%	0.002%
27	3.500	763	765	768	rVB	200	94	0.01%	0.001%
28	3.519	769	771	774	rBV	339	174	0.01%	0.002%
29	3.555	779	782	784	rVB	217	84	0.01%	0.001%
30	3.574	784	788	791	rBV2	438	279	0.02%	0.002%
31	3.590	791	793	795	rBV2	259	148	0.01%	0.001%
32	3.619	801	802	803	rBV	215	53	0.00%	0.000%
33	3.645	808	810	814	rVB2	242	137	0.01%	0.001%
34	3.667	814	817	820	rVB2	556	302	0.02%	0.003%
35	3.693	824	825	830	rVB2	506	269	0.02%	0.002%
36	3.715	830	832	834	rBV	412	191	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027965.D
 Acq On : 20 Sep 2022 16:20
 Operator : SY/MD
 Sample : N4619-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.732	834	837	839	rBV	302	143	0.01%	0.001%
38	3.780	849	852	854	rBV2	276	186	0.01%	0.002%
39	3.825	862	866	868	rVB2	291	174	0.01%	0.002%
40	3.867	870	879	912	rBV	119623	330435	21.67%	2.863%
41	4.207	983	985	988	rVB4	744	340	0.02%	0.003%
42	4.336	1011	1025	1055	rBV	244305	597848	39.21%	5.180%
43	4.648	1116	1122	1124	rBV6	1294	1174	0.08%	0.010%
44	4.783	1160	1164	1166	rBV3	411	299	0.02%	0.003%
45	4.793	1166	1167	1169	rBV	255	66	0.00%	0.001%
46	4.809	1169	1172	1173	rBV2	417	258	0.02%	0.002%
47	4.899	1197	1200	1202	rBV2	475	322	0.02%	0.003%
48	4.915	1203	1205	1209	rVB	496	360	0.02%	0.003%
49	4.941	1210	1213	1214	rBV	429	215	0.01%	0.002%
50	4.966	1219	1221	1223	rBV2	547	189	0.01%	0.002%
51	5.037	1225	1243	1270	rBV2	592089	1524729	100.00%	13.210%
52	5.358	1341	1343	1349	rVB5	826	607	0.04%	0.005%
53	5.387	1349	1352	1354	rBV3	855	514	0.03%	0.004%
54	5.471	1376	1378	1380	rVB2	292	108	0.01%	0.001%
55	5.490	1380	1384	1388	rBV3	570	506	0.03%	0.004%
56	5.609	1409	1421	1446	rBV	372353	752995	49.39%	6.524%
57	5.809	1481	1483	1486	rBV4	808	631	0.04%	0.005%
58	5.854	1495	1497	1498	rBV2	575	247	0.02%	0.002%
59	5.960	1528	1530	1531	rBV	507	160	0.01%	0.001%
60	6.063	1546	1562	1593	rBV	334682	701063	45.98%	6.074%
61	6.288	1629	1632	1634	rBV4	775	434	0.03%	0.004%
62	6.397	1664	1666	1670	rVB3	602	393	0.03%	0.003%
63	6.420	1670	1673	1675	rBV2	690	410	0.03%	0.004%
64	6.490	1693	1695	1696	rBV	285	99	0.01%	0.001%
65	6.503	1696	1699	1702	rVV5	1362	956	0.06%	0.008%
66	6.567	1716	1719	1720	rBV3	774	296	0.02%	0.003%
67	6.873	1811	1814	1820	rBV6	819	1028	0.07%	0.009%
68	6.982	1837	1848	1869	rBV	196206	364441	23.90%	3.158%
69	7.310	1938	1950	1971	rBV	729863	1271269	83.38%	11.014%
70	7.616	2036	2045	2064	rBV	140652	249120	16.34%	2.158%
71	8.082	2181	2190	2218	rBV	468829	820530	53.81%	7.109%
72	8.500	2316	2320	2321	rBV2	942	687	0.05%	0.006%
73	8.715	2385	2387	2389	rBV	735	339	0.02%	0.003%
74	8.847	2417	2428	2450	rBV	595567	977471	64.11%	8.469%
75	9.551	2642	2647	2650	rBV4	2126	1922	0.13%	0.017%
76	9.860	2741	2743	2745	rBV3	909	466	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027965.D
 Acq On : 20 Sep 2022 16:20
 Operator : SY/MD
 Sample : N4619-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E13

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

77	9.931	2760	2765	2768	rBV4	1779	1652	0.11%	0.014%
78	10.214	2840	2853	2869	rBV	516511	818202	53.66%	7.089%
79	10.757	3020	3022	3023	rBV	747	296	0.02%	0.003%
80	11.246	3163	3174	3193	rBV	578115	893692	58.61%	7.743%
81	11.622	3280	3291	3310	rBV	709900	1119861	73.45%	9.703%
82	12.641	3606	3608	3611	rBV4	1755	1292	0.08%	0.011%
83	13.506	3872	3877	3885	rBV3	4926	6303	0.41%	0.055%
84	14.258	4108	4111	4112	rBV3	591	363	0.02%	0.003%


Sum of corrected areas: 11541904

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027965.D
Acq On : 20 Sep 2022 16:20
Operator : SY/MD
Sample : N4619-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

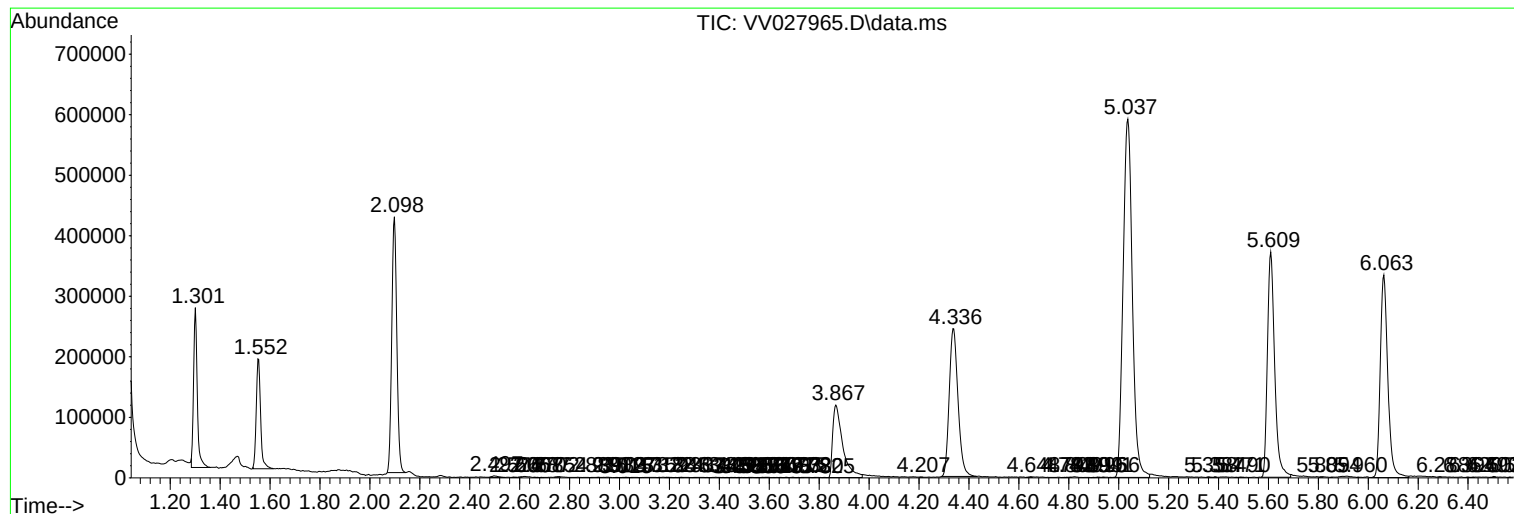

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027965.D
Acq On : 20 Sep 2022 16:20
Operator : SY/MD
Sample : N4619-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027965.D
Acq On : 20 Sep 2022 16:20
Operator : SY/MD
Sample : N4619-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 11 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E13

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc