

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027966.D
 Acq On : 20 Sep 2022 16:44
 Operator : SY/MD
 Sample : N4619-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027966.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	249466	258001	4.64%	1.472%
2	1.555	153	160	175	rVB	172327	204885	3.69%	1.169%
3	2.102	320	330	360	rVB2	524044	890661	16.03%	5.083%
4	2.253	374	377	379	rBV3	1035	701	0.01%	0.004%
5	2.577	477	478	479	rBV	347	84	0.00%	0.000%
6	2.703	515	517	522	rBV4	503	432	0.01%	0.002%
7	2.754	525	533	546	rBV10	3122	5900	0.11%	0.034%
8	2.844	559	561	563	rBV2	259	92	0.00%	0.001%
9	2.925	583	586	587	rBV	293	186	0.00%	0.001%
10	2.966	596	599	602	rBV2	368	303	0.01%	0.002%
11	2.982	602	604	607	rVB2	463	215	0.00%	0.001%
12	2.999	607	609	611	rBV2	335	182	0.00%	0.001%
13	3.024	615	617	620	rBV2	433	328	0.01%	0.002%
14	3.063	627	629	630	rBV	504	201	0.00%	0.001%
15	3.098	638	640	643	rVB2	384	135	0.00%	0.001%
16	3.134	645	651	652	rBV2	599	377	0.01%	0.002%
17	3.185	658	667	681	rVB3	5565	10557	0.19%	0.060%
18	3.253	687	688	690	rBV3	231	93	0.00%	0.001%
19	3.265	690	692	695	rVB2	407	188	0.00%	0.001%
20	3.298	701	702	706	rVB2	446	144	0.00%	0.001%
21	3.320	707	709	711	rVB	303	99	0.00%	0.001%
22	3.336	711	714	716	rBV2	561	331	0.01%	0.002%
23	3.349	716	718	723	rVB2	422	234	0.00%	0.001%
24	3.381	723	728	731	rVB3	508	459	0.01%	0.003%
25	3.397	731	733	737	rBV	198	154	0.00%	0.001%
26	3.420	738	740	748	rVB2	289	270	0.00%	0.002%
27	3.452	748	750	753	rBV	244	158	0.00%	0.001%
28	3.513	766	769	770	rVB2	326	127	0.00%	0.001%
29	3.523	770	772	774	rVB2	158	62	0.00%	0.000%
30	3.539	774	777	779	rBV3	483	290	0.01%	0.002%
31	3.555	781	782	784	rBV	272	107	0.00%	0.001%
32	3.603	794	797	799	rBV2	148	104	0.00%	0.001%
33	3.619	799	802	804	rBV3	360	192	0.00%	0.001%
34	3.655	811	813	814	rBV3	162	36	0.00%	0.000%
35	3.664	814	816	817	rVB	418	157	0.00%	0.001%
36	3.674	817	819	824	rBV2	283	198	0.00%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027966.D
 Acq On : 20 Sep 2022 16:44
 Operator : SY/MD
 Sample : N4619-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.700	825	827	829	rVB2	269	87	0.00%	0.000%
38	3.719	830	833	836	rBV2	291	159	0.00%	0.001%
39	3.732	836	837	840	rBV2	396	172	0.00%	0.001%
40	3.745	840	841	842	rVB	249	48	0.00%	0.000%
41	3.754	842	844	845	rBV	208	78	0.00%	0.000%
42	3.818	862	864	865	rBV	290	146	0.00%	0.001%
43	3.899	870	889	922	rBV2	197952	717656	12.92%	4.096%
44	4.182	975	977	982	rBV3	625	451	0.01%	0.003%
45	4.339	1011	1026	1056	rBV	226973	563489	10.14%	3.216%
46	4.600	1091	1107	1126	rBV3	103731	260472	4.69%	1.487%
47	4.719	1142	1144	1146	rBV3	665	287	0.01%	0.002%
48	4.754	1154	1155	1156	rBV	372	137	0.00%	0.001%
49	4.777	1160	1162	1163	rBV2	368	164	0.00%	0.001%
50	4.851	1183	1185	1188	rBV2	285	93	0.00%	0.001%
51	4.902	1199	1201	1202	rBV	366	163	0.00%	0.001%
52	5.037	1224	1243	1277	rBV2	554559	1423136	25.62%	8.122%
53	5.400	1352	1356	1358	rBV3	838	579	0.01%	0.003%
54	5.452	1370	1372	1374	rVB3	677	258	0.00%	0.001%
55	5.471	1374	1378	1380	rBV5	638	474	0.01%	0.003%
56	5.516	1390	1392	1398	rVB4	734	629	0.01%	0.004%
57	5.542	1398	1400	1403	rVB2	389	229	0.00%	0.001%
58	5.564	1403	1407	1409	rBV3	707	612	0.01%	0.003%
59	5.609	1409	1421	1449	rBV	383577	773586	13.92%	4.415%
60	5.838	1490	1492	1494	rBV3	684	299	0.01%	0.002%
61	5.905	1499	1513	1539	rBV	2919432	5555459	100.00%	31.706%
62	6.063	1551	1562	1588	rVB	312276	632709	11.39%	3.611%
63	6.362	1653	1655	1657	rBV2	864	493	0.01%	0.003%
64	6.625	1733	1737	1740	rBV2	577	462	0.01%	0.003%
65	6.735	1769	1771	1772	rBV	595	198	0.00%	0.001%
66	6.764	1776	1780	1785	rBV5	850	753	0.01%	0.004%
67	6.796	1787	1790	1792	rVB2	416	190	0.00%	0.001%
68	6.822	1797	1798	1799	rBV	308	89	0.00%	0.001%
69	6.918	1825	1828	1830	rBV	483	301	0.01%	0.002%
70	6.982	1837	1848	1876	rBV	172916	323028	5.81%	1.844%
71	7.310	1939	1950	1972	rBV	661222	1144576	20.60%	6.532%
72	7.619	2037	2046	2072	rVB	129147	222651	4.01%	1.271%
73	7.937	2138	2145	2154	rVB2	19457	31636	0.57%	0.181%
74	8.085	2181	2191	2219	rBV	453602	801528	14.43%	4.575%
75	8.847	2418	2428	2455	rBV	597918	993342	17.88%	5.669%
76	9.140	2515	2519	2522	rBV5	1374	1395	0.03%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027966.D
 Acq On : 20 Sep 2022 16:44
 Operator : SY/MD
 Sample : N4619-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E14

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.506	2631	2633	2635	rBV2	633	374	0.01%	0.002%
78	9.744	2705	2707	2709	rBV2	618	211	0.00%	0.001%
79	10.018	2790	2792	2795	rBV3	984	811	0.01%	0.005%
80	10.101	2816	2818	2819	rBV	1000	456	0.01%	0.003%
81	10.214	2841	2853	2874	rBV	485956	772406	13.90%	4.408%
82	10.474	2931	2934	2936	rBV3	1109	567	0.01%	0.003%
83	10.969	3086	3088	3092	rVB4	1232	613	0.01%	0.003%
84	11.246	3163	3174	3195	rBV	574566	894165	16.10%	5.103%
85	11.622	3280	3291	3311	rVB	652506	1021887	18.39%	5.832%
86	12.304	3501	3503	3504	rBV2	880	319	0.01%	0.002%
87	13.059	3736	3738	3741	rBV4	899	391	0.01%	0.002%
88	14.561	4203	4205	4207	rBV2	1242	463	0.01%	0.003%




Sum of corrected areas: 17521520

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027966.D
Acq On : 20 Sep 2022 16:44
Operator : SY/MD
Sample : N4619-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

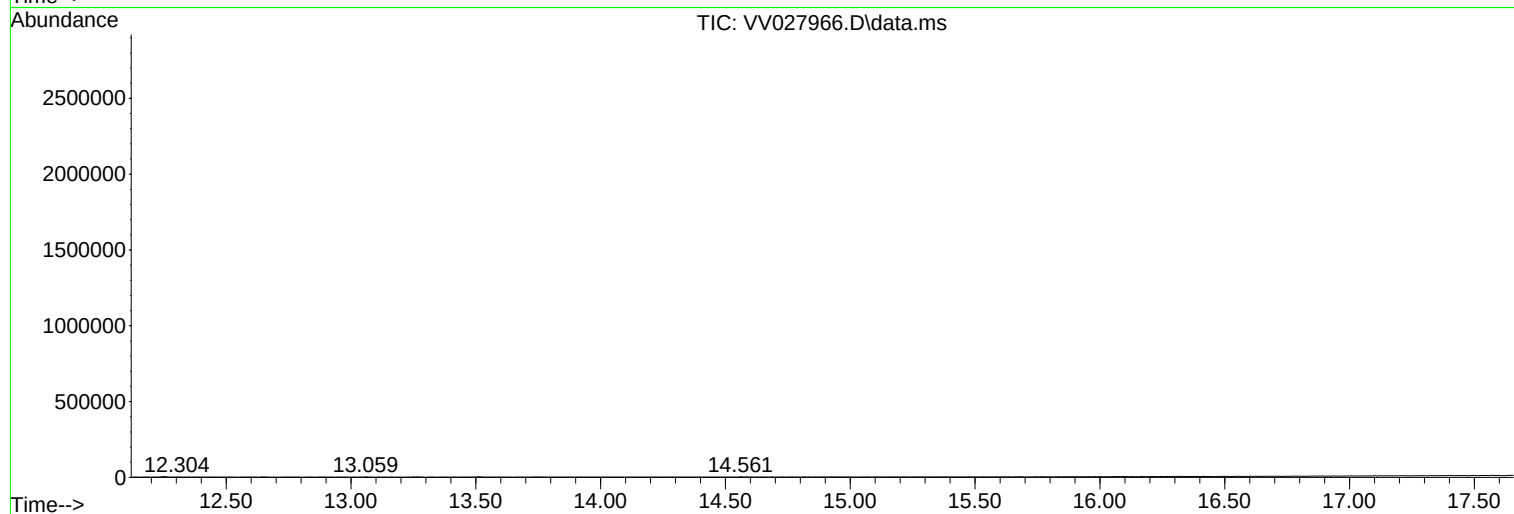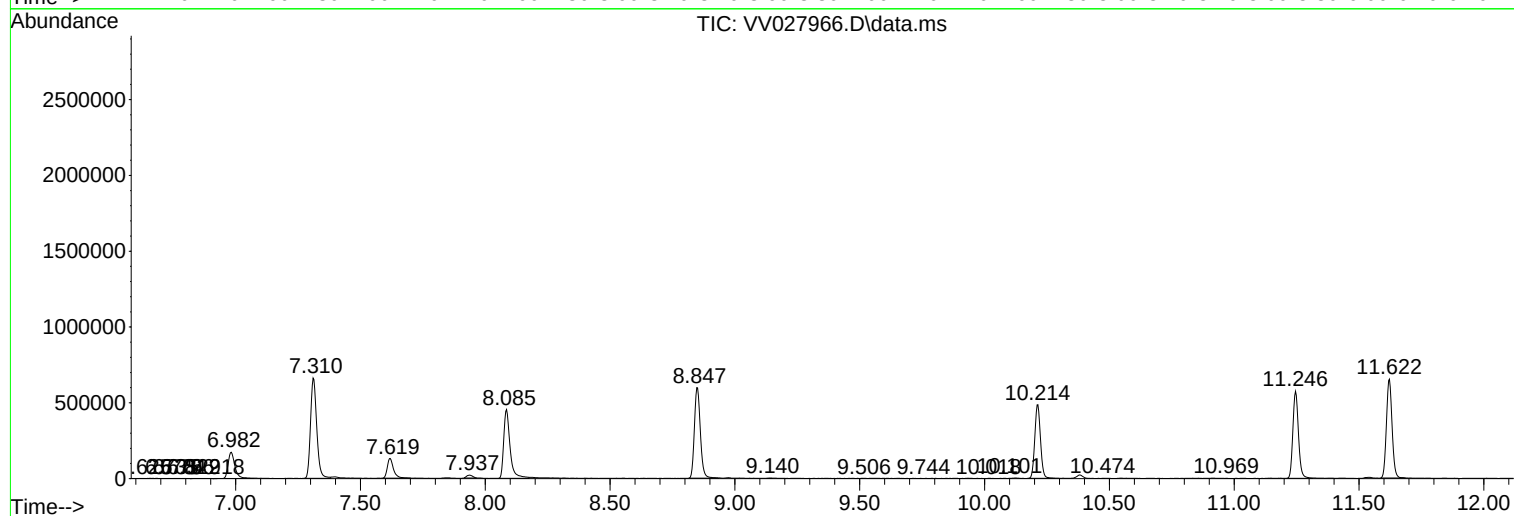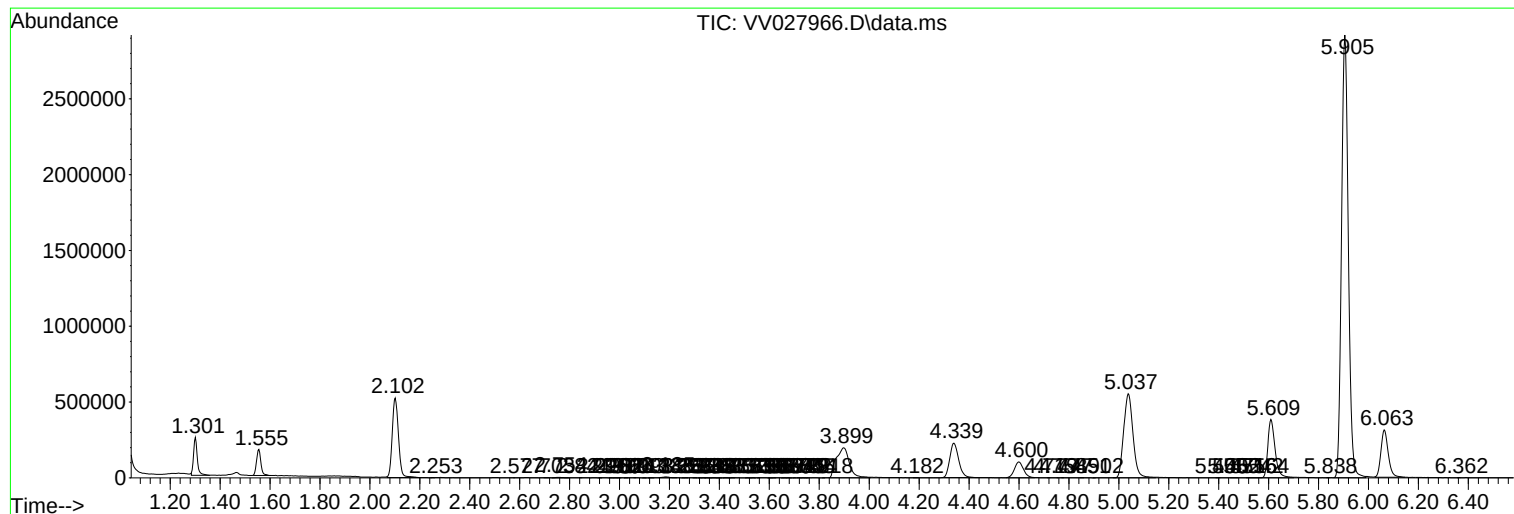

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027966.D
Acq On : 20 Sep 2022 16:44
Operator : SY/MD
Sample : N4619-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027966.D
Acq On : 20 Sep 2022 16:44
Operator : SY/MD
Sample : N4619-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 12 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E14

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------