

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027968.D
 Acq On : 20 Sep 2022 17:34
 Operator : SY/MD
 Sample : N4619-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027968.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	98	rVB	237052	241193	16.33%	2.210%
2	1.558	155	161	178	rVB	177136	201063	13.61%	1.843%
3	2.098	320	329	345	rBV	373156	533519	36.13%	4.889%
4	2.355	407	409	411	rBV2	632	345	0.02%	0.003%
5	2.407	421	425	429	rBV3	667	597	0.04%	0.005%
6	2.429	430	432	436	rVV	527	259	0.02%	0.002%
7	2.490	445	451	453	rBV5	1654	1425	0.10%	0.013%
8	2.590	480	482	486	rVB3	584	331	0.02%	0.003%
9	2.609	486	488	491	rBV3	525	351	0.02%	0.003%
10	2.629	491	494	495	rBV2	917	565	0.04%	0.005%
11	2.757	531	534	536	rBV3	753	480	0.03%	0.004%
12	2.796	543	546	550	rVB2	581	450	0.03%	0.004%
13	2.818	550	553	554	rBV2	402	218	0.01%	0.002%
14	2.867	564	568	571	rVB2	301	207	0.01%	0.002%
15	2.963	594	598	600	rBV3	598	478	0.03%	0.004%
16	3.008	608	612	614	rBV4	426	373	0.03%	0.003%
17	3.114	640	645	646	rBV	296	168	0.01%	0.002%
18	3.130	646	650	651	rVB2	396	198	0.01%	0.002%
19	3.150	653	656	658	rBV	272	137	0.01%	0.001%
20	3.169	660	662	663	rBV2	430	184	0.01%	0.002%
21	3.211	673	675	679	rBV3	410	292	0.02%	0.003%
22	3.236	681	683	685	rVB3	392	170	0.01%	0.002%
23	3.314	704	707	710	rVV3	303	240	0.02%	0.002%
24	3.326	710	711	714	rVB	450	161	0.01%	0.001%
25	3.384	727	729	731	rVB3	334	149	0.01%	0.001%
26	3.400	731	734	737	rBV2	341	283	0.02%	0.003%
27	3.481	754	759	760	rBV2	508	355	0.02%	0.003%
28	3.519	768	771	773	rBV	401	218	0.01%	0.002%
29	3.555	779	782	787	rVB3	399	385	0.03%	0.004%
30	3.619	798	802	806	rBV4	433	395	0.03%	0.004%
31	3.645	806	810	815	rBV3	356	250	0.02%	0.002%
32	3.744	838	841	842	rBV	325	215	0.01%	0.002%
33	3.780	849	852	854	rBV3	321	172	0.01%	0.002%
34	3.789	854	855	860	rVB3	456	243	0.02%	0.002%
35	3.812	860	862	866	rVB	326	186	0.01%	0.002%
36	3.873	871	881	923	rBV	118938	337013	22.82%	3.088%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027968.D
 Acq On : 20 Sep 2022 17:34
 Operator : SY/MD
 Sample : N4619-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	4.339	1010	1026	1059	rBV	241331	597669	40.47%	5.477%
38	4.767	1157	1159	1164	rVB6	748	439	0.03%	0.004%
39	4.815	1170	1174	1177	rBV3	834	711	0.05%	0.007%
40	4.879	1193	1194	1196	rBV	658	241	0.02%	0.002%
41	5.037	1228	1243	1279	rBV2	578799	1476801	100.00%	13.534%
42	5.252	1308	1310	1313	rBV3	1000	600	0.04%	0.005%
43	5.391	1351	1353	1354	rBV3	541	180	0.01%	0.002%
44	5.461	1373	1375	1376	rBV2	942	463	0.03%	0.004%
45	5.609	1408	1421	1442	rBV	409855	830845	56.26%	7.614%
46	5.912	1504	1515	1538	rBV2	55334	117817	7.98%	1.080%
47	6.063	1549	1562	1589	rBV	331389	677099	45.85%	6.205%
48	6.301	1633	1636	1640	rBV5	1127	822	0.06%	0.008%
49	6.336	1645	1647	1648	rBV	589	201	0.01%	0.002%
50	6.352	1650	1652	1655	rBV3	696	379	0.03%	0.003%
51	6.400	1665	1667	1670	rBV3	920	370	0.03%	0.003%
52	6.432	1674	1677	1679	rBV2	613	362	0.02%	0.003%
53	6.510	1697	1701	1703	rBV3	488	307	0.02%	0.003%
54	6.587	1722	1725	1728	rBV3	705	429	0.03%	0.004%
55	6.606	1728	1731	1732	rBV2	727	440	0.03%	0.004%
56	6.648	1741	1744	1745	rBV2	495	261	0.02%	0.002%
57	6.703	1759	1761	1763	rBV3	927	390	0.03%	0.004%
58	6.828	1799	1800	1802	rBV	487	143	0.01%	0.001%
59	6.879	1814	1816	1818	rBV	448	218	0.01%	0.002%
60	6.912	1822	1826	1829	rVB3	438	340	0.02%	0.003%
61	6.934	1830	1833	1835	rVB	509	239	0.02%	0.002%
62	6.982	1836	1848	1870	rBV2	163580	300860	20.37%	2.757%
63	7.310	1938	1950	1970	rBV	607666	1052451	71.27%	9.645%
64	7.619	2036	2046	2067	rBV	115418	203555	13.78%	1.865%
65	7.940	2136	2146	2156	rBV	9442	16795	1.14%	0.154%
66	7.992	2160	2162	2163	rBV	474	171	0.01%	0.002%
67	8.030	2171	2174	2177	rBV3	501	440	0.03%	0.004%
68	8.085	2181	2191	2220	rBV	400588	723883	49.02%	6.634%
69	8.564	2338	2340	2343	rVB2	751	336	0.02%	0.003%
70	8.702	2380	2383	2384	rBV2	559	221	0.01%	0.002%
71	8.722	2388	2389	2390	rBV	619	180	0.01%	0.002%
72	8.773	2403	2405	2407	rBV2	753	445	0.03%	0.004%
73	8.847	2416	2428	2453	rBV	615983	1018020	68.93%	9.329%
74	9.194	2534	2536	2538	rBV3	888	393	0.03%	0.004%
75	9.223	2541	2545	2547	rBV5	909	611	0.04%	0.006%
76	9.301	2567	2569	2571	rBV3	1008	504	0.03%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027968.D
 Acq On : 20 Sep 2022 17:34
 Operator : SY/MD
 Sample : N4619-04
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E17

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.432	2608	2610	2612	rVB3	1131	398	0.03%	0.004%
78	9.448	2612	2615	2617	rBV3	1018	669	0.05%	0.006%
79	9.526	2638	2639	2641	rBV	713	303	0.02%	0.003%
80	9.583	2655	2657	2660	rBV2	710	480	0.03%	0.004%
81	9.600	2660	2662	2667	rVB5	1310	1076	0.07%	0.010%
82	9.628	2667	2671	2672	rBV2	779	532	0.04%	0.005%
83	9.702	2693	2694	2700	rVB3	898	668	0.05%	0.006%
84	9.728	2700	2702	2704	rBV	426	181	0.01%	0.002%
85	9.744	2704	2707	2710	rBV4	919	735	0.05%	0.007%
86	10.056	2801	2804	2805	rBV2	855	518	0.04%	0.005%
87	10.085	2811	2813	2815	rBV3	804	529	0.04%	0.005%
88	10.124	2818	2825	2831	rBV7	2523	3633	0.25%	0.033%
89	10.214	2841	2853	2870	rBV	466380	741794	50.23%	6.798%
90	10.696	3001	3003	3007	rBV3	852	647	0.04%	0.006%
91	10.728	3012	3013	3016	rVB2	697	336	0.02%	0.003%
92	10.744	3016	3018	3020	rBV2	963	597	0.04%	0.005%
93	10.773	3024	3027	3030	rBV4	1002	759	0.05%	0.007%
94	10.969	3086	3088	3090	rBV2	788	320	0.02%	0.003%
95	11.246	3163	3174	3192	rBV	571158	869609	58.88%	7.969%
96	11.622	3280	3291	3309	rBV	593227	936535	63.42%	8.583%
97	12.333	3510	3512	3515	rBV2	982	460	0.03%	0.004%
98	12.416	3536	3538	3540	rBV2	968	535	0.04%	0.005%
99	12.728	3632	3635	3637	rBV2	851	622	0.04%	0.006%
100	13.593	3903	3904	3905	rBV2	775	225	0.02%	0.002%




Sum of corrected areas: 10912060

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027968.D
Acq On : 20 Sep 2022 17:34
Operator : SY/MD
Sample : N4619-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

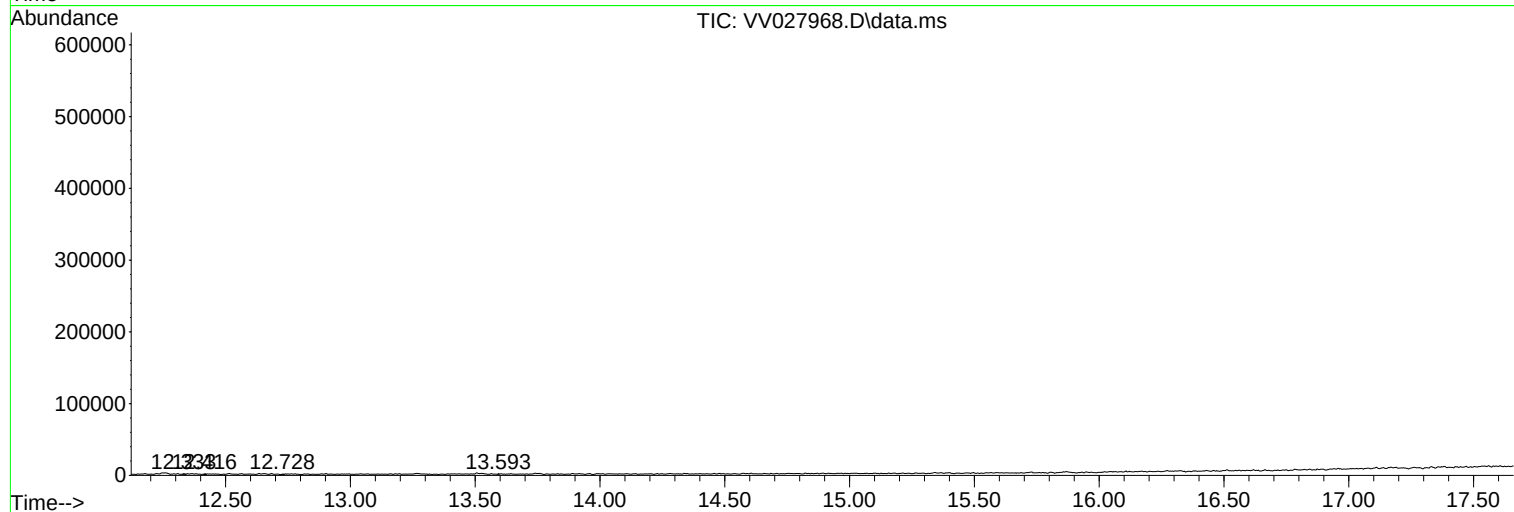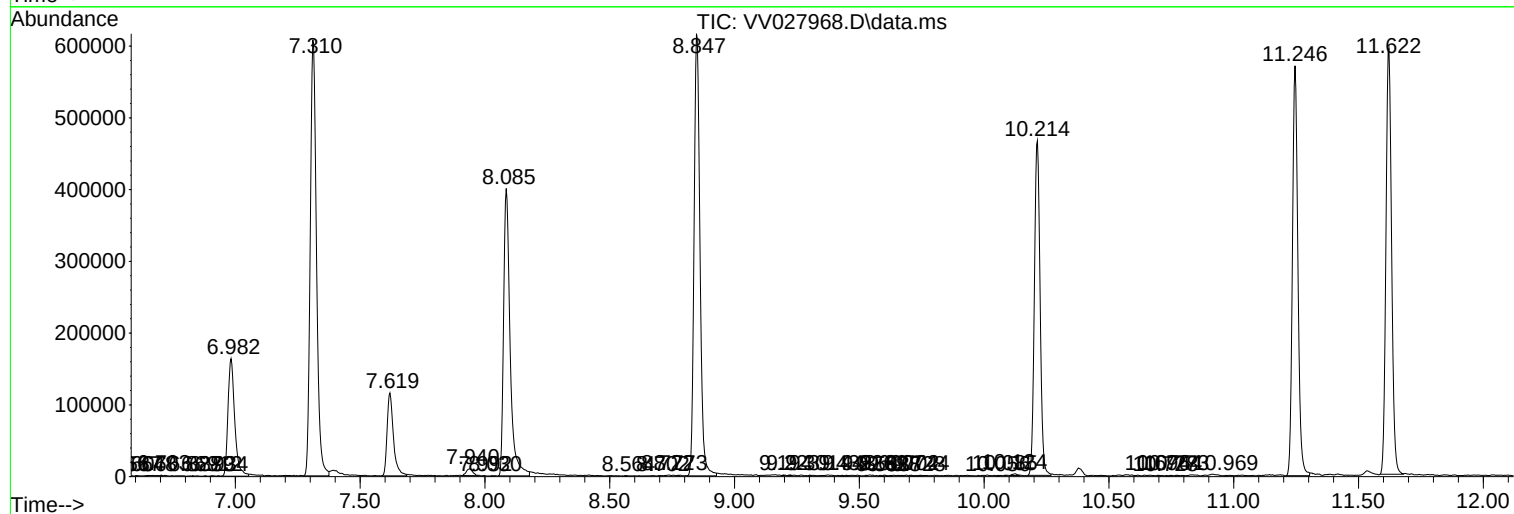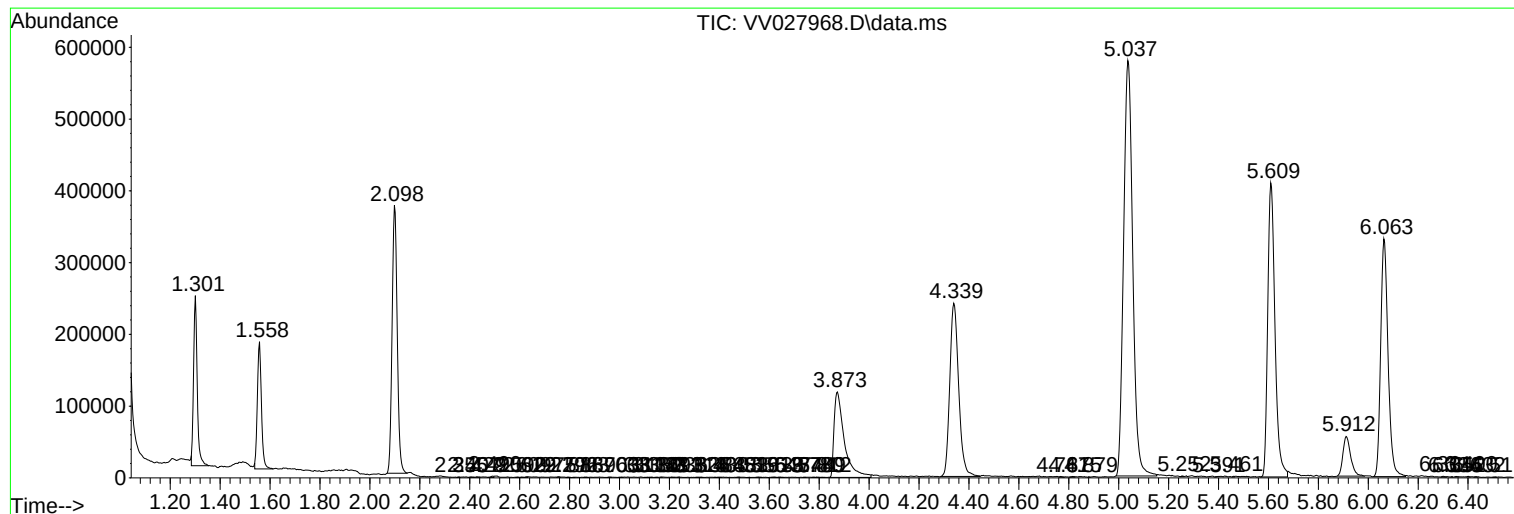

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027968.D
Acq On : 20 Sep 2022 17:34
Operator : SY/MD
Sample : N4619-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027968.D
Acq On : 20 Sep 2022 17:34
Operator : SY/MD
Sample : N4619-04
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E17

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
