

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027969.D
 Acq On : 20 Sep 2022 17:59
 Operator : SY/MD
 Sample : N4619-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027969.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	100	rVB	234649	244250	17.64%	2.261%
2	1.558	155	161	180	rVB	171101	200734	14.49%	1.858%
3	2.098	320	329	343	rBV	371201	529522	38.23%	4.902%
4	2.407	418	425	428	rBV4	987	903	0.07%	0.008%
5	2.709	517	519	521	rBV2	245	102	0.01%	0.001%
6	2.725	521	524	526	rBV	269	120	0.01%	0.001%
7	2.744	526	530	531	rBV2	442	368	0.03%	0.003%
8	2.783	539	542	543	rBV	161	92	0.01%	0.001%
9	2.789	543	544	546	rBV	269	110	0.01%	0.001%
10	2.857	563	565	568	rBV2	264	121	0.01%	0.001%
11	2.950	591	594	595	rBV2	554	318	0.02%	0.003%
12	2.973	599	601	603	rBV3	385	182	0.01%	0.002%
13	2.995	606	608	610	rVB3	426	126	0.01%	0.001%
14	3.011	610	613	616	rBV3	662	533	0.04%	0.005%
15	3.063	627	629	630	rBV3	276	96	0.01%	0.001%
16	3.149	655	656	660	rVB2	236	116	0.01%	0.001%
17	3.166	660	661	663	rBV2	327	128	0.01%	0.001%
18	3.178	663	665	668	rBV4	454	285	0.02%	0.003%
19	3.220	676	678	683	rVB2	454	333	0.02%	0.003%
20	3.246	683	686	687	rBV	566	299	0.02%	0.003%
21	3.304	702	704	706	rBV	464	209	0.02%	0.002%
22	3.336	712	714	717	rBV2	260	154	0.01%	0.001%
23	3.391	730	731	735	rBV2	414	217	0.02%	0.002%
24	3.413	735	738	739	rVV	156	67	0.00%	0.001%
25	3.445	745	748	752	rVB2	732	587	0.04%	0.005%
26	3.477	753	758	759	rBV2	363	261	0.02%	0.002%
27	3.519	767	771	775	rBV2	291	267	0.02%	0.002%
28	3.613	798	800	801	rBV2	666	245	0.02%	0.002%
29	3.622	801	803	804	rVV	281	112	0.01%	0.001%
30	3.658	811	814	816	rVB2	405	226	0.02%	0.002%
31	3.683	819	822	824	rBV	462	214	0.02%	0.002%
32	3.706	824	829	830	rBV2	291	191	0.01%	0.002%
33	3.715	830	832	833	rVV2	395	152	0.01%	0.001%
34	3.728	833	836	840	rVB2	260	220	0.02%	0.002%
35	3.870	871	880	920	rBV3	110001	325200	23.48%	3.010%
36	4.259	999	1001	1006	rBV4	699	597	0.04%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027969.D
 Acq On : 20 Sep 2022 17:59
 Operator : SY/MD
 Sample : N4619-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E19

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	4.339	1011	1026	1051	rVV	215639	545881	39.41%	5.053%
38	4.812	1170	1173	1178	rVB3	613	356	0.03%	0.003%
39	4.883	1192	1195	1196	rBV2	623	371	0.03%	0.003%
40	4.918	1204	1206	1211	rBV2	618	435	0.03%	0.004%
41	5.037	1227	1243	1274	rBV2	536890	1385000	100.00%	12.821%
42	5.468	1375	1377	1378	rBV	517	184	0.01%	0.002%
43	5.567	1407	1408	1409	rVB	379	73	0.01%	0.001%
44	5.609	1409	1421	1450	rBV	399030	815014	58.85%	7.545%
45	6.063	1549	1562	1593	rBV	328917	680118	49.11%	6.296%
46	6.837	1802	1803	1805	rBV	555	159	0.01%	0.001%
47	6.982	1838	1848	1872	rBV	175086	317697	22.94%	2.941%
48	7.313	1938	1951	1970	rBV	630808	1103720	79.69%	10.217%
49	7.571	2029	2031	2036	rBV3	1179	1063	0.08%	0.010%
50	7.619	2036	2046	2065	rBV	123360	218754	15.79%	2.025%
51	8.040	2174	2177	2180	rBV4	610	560	0.04%	0.005%
52	8.085	2181	2191	2218	rBV	428313	763026	55.09%	7.063%
53	8.847	2418	2428	2454	rBV	630224	1022765	73.85%	9.468%
54	9.320	2572	2575	2577	rBV3	728	420	0.03%	0.004%
55	9.529	2637	2640	2643	rBV2	909	650	0.05%	0.006%
56	9.599	2660	2662	2664	rBV2	698	287	0.02%	0.003%
57	9.976	2776	2779	2780	rBV2	1040	691	0.05%	0.006%
58	10.214	2842	2853	2871	rBV	478843	760072	54.88%	7.036%
59	11.181	3151	3154	3156	rBV2	1176	906	0.07%	0.008%
60	11.246	3162	3174	3193	rBV	586514	906256	65.43%	8.389%
61	11.622	3279	3291	3312	rBV	608230	965522	69.71%	8.938%
62	11.969	3396	3399	3400	rBV2	974	465	0.03%	0.004%
63	12.136	3447	3451	3455	rBV5	1068	916	0.07%	0.008%
64	12.165	3458	3460	3463	rBV3	739	509	0.04%	0.005%
65	12.586	3587	3591	3592	rBV3	1488	935	0.07%	0.009%
66	12.725	3632	3634	3635	rBV2	995	413	0.03%	0.004%
67	12.776	3646	3650	3654	rBV6	930	1117	0.08%	0.010%
68	13.229	3790	3791	3793	rBV3	745	358	0.03%	0.003%
69	13.406	3844	3846	3849	rBV3	687	388	0.03%	0.004%




Sum of corrected areas: 10802738

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027969.D
Acq On : 20 Sep 2022 17:59
Operator : SY/MD
Sample : N4619-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

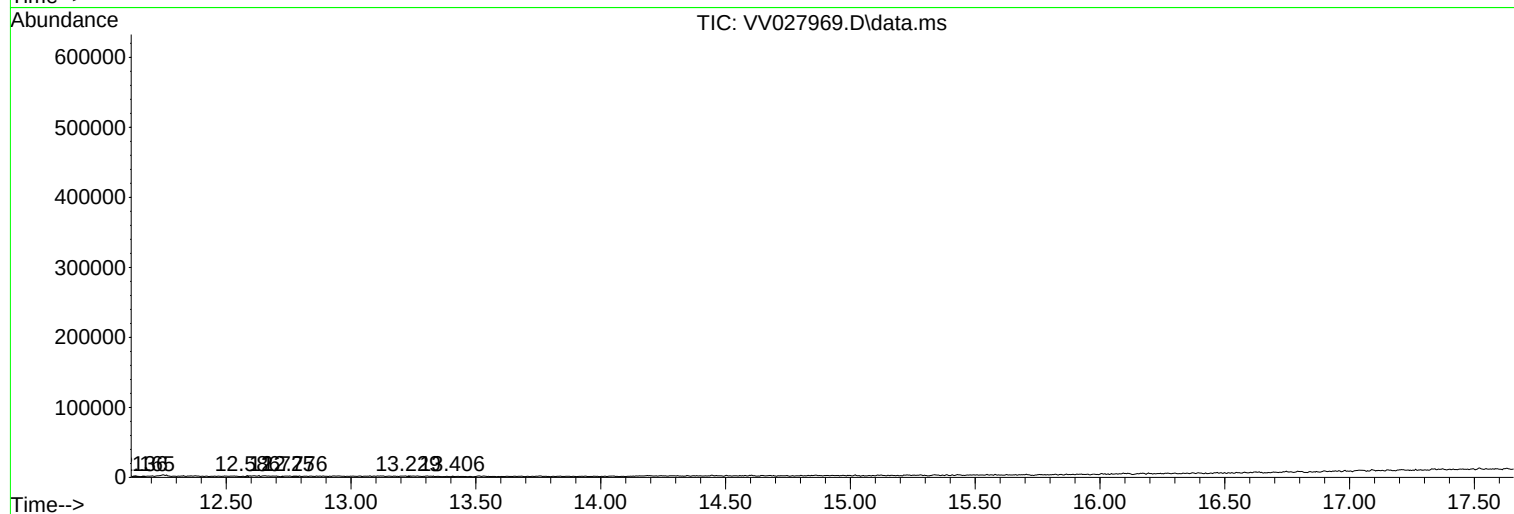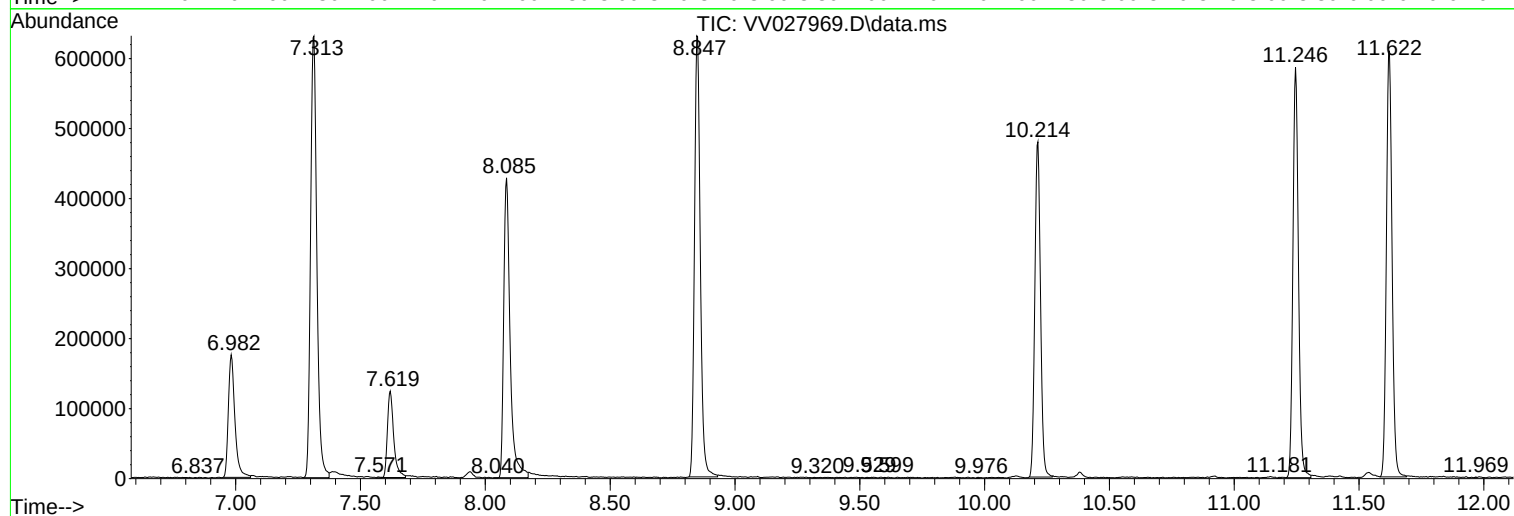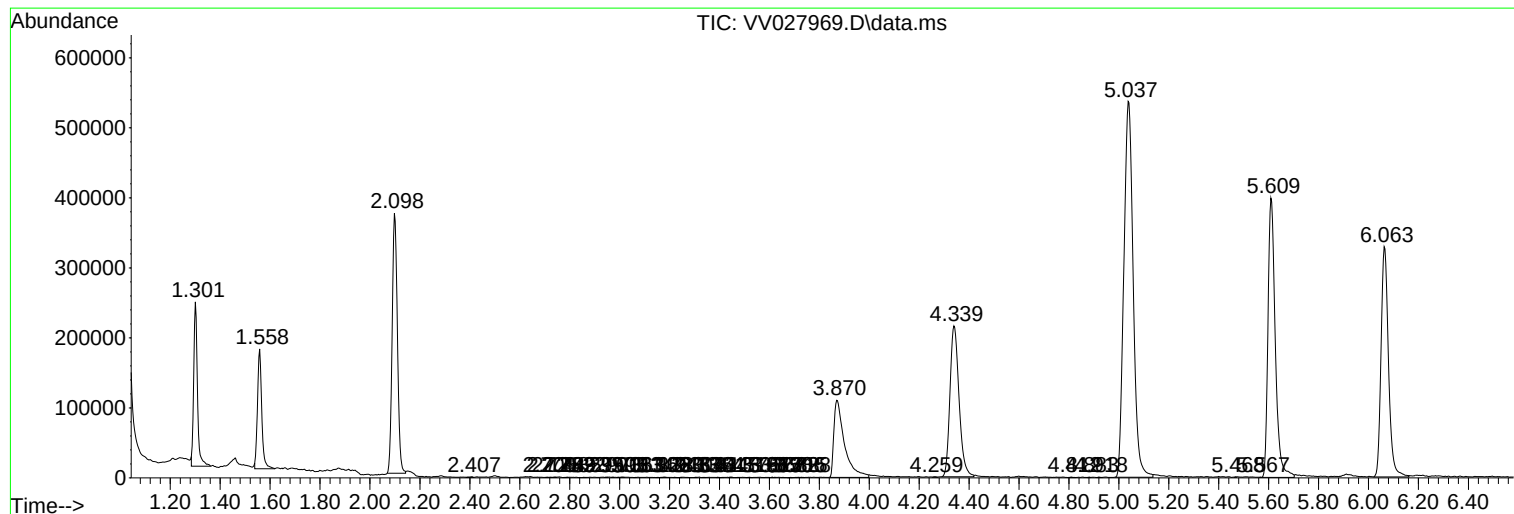

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027969.D
Acq On : 20 Sep 2022 17:59
Operator : SY/MD
Sample : N4619-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027969.D
Acq On : 20 Sep 2022 17:59
Operator : SY/MD
Sample : N4619-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 15 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E19

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc