

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027971.D
 Acq On : 20 Sep 2022 18:49
 Operator : SY/MD
 Sample : N4619-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027971.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	100	rVB	237291	243891	18.15%	2.296%
2	1.555	154	160	175	rVB	166323	194158	14.45%	1.828%
3	2.098	320	329	342	rBV	371932	528638	39.34%	4.977%
4	2.609	484	488	489	rBV3	892	622	0.05%	0.006%
5	2.693	513	514	515	rBV3	237	59	0.00%	0.001%
6	2.709	515	519	522	rVV3	443	411	0.03%	0.004%
7	2.793	542	545	548	rBV2	376	260	0.02%	0.002%
8	2.828	554	556	558	rVB2	408	159	0.01%	0.001%
9	2.886	570	574	575	rBV2	709	420	0.03%	0.004%
10	2.979	602	603	604	rBV2	295	88	0.01%	0.001%
11	3.002	607	610	611	rBV2	217	136	0.01%	0.001%
12	3.085	635	636	639	rBV2	216	124	0.01%	0.001%
13	3.133	645	651	654	rBV2	625	579	0.04%	0.005%
14	3.240	681	684	685	rBV2	471	223	0.02%	0.002%
15	3.285	696	698	699	rBV	248	88	0.01%	0.001%
16	3.310	704	706	707	rBV	218	89	0.01%	0.001%
17	3.346	715	717	720	rBV2	259	156	0.01%	0.001%
18	3.365	721	723	725	rVB2	458	150	0.01%	0.001%
19	3.384	725	729	731	rBV2	299	187	0.01%	0.002%
20	3.397	731	733	734	rBV	346	142	0.01%	0.001%
21	3.426	740	742	743	rVB	397	126	0.01%	0.001%
22	3.445	743	748	751	rBV3	317	360	0.03%	0.003%
23	3.503	763	766	771	rBV2	441	299	0.02%	0.003%
24	3.529	771	774	777	rBV	310	256	0.02%	0.002%
25	3.568	784	786	791	rVB3	421	261	0.02%	0.002%
26	3.596	791	795	798	rVB	275	172	0.01%	0.002%
27	3.619	799	802	809	rVB3	539	469	0.03%	0.004%
28	3.658	809	814	817	rBV2	373	366	0.03%	0.003%
29	3.677	817	820	823	rBV	296	162	0.01%	0.002%
30	3.693	823	825	827	rBV2	259	121	0.01%	0.001%
31	3.754	839	844	847	rBV2	534	445	0.03%	0.004%
32	3.786	851	854	855	rBV	83	45	0.00%	0.000%
33	3.796	855	857	863	rBV4	365	358	0.03%	0.003%
34	3.828	863	867	868	rBV	193	120	0.01%	0.001%
35	3.870	870	880	904	rBV	108018	299586	22.29%	2.820%
36	4.339	1008	1026	1055	rBV	221513	557322	41.47%	5.247%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027971.D
 Acq On : 20 Sep 2022 18:49
 Operator : SY/MD
 Sample : N4619-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	4.706	1136	1140	1143	rBB2	325	262	0.02%	0.002%
38	4.725	1143	1146	1149	rBV3	516	323	0.02%	0.003%
39	4.770	1157	1160	1161	rBV2	360	146	0.01%	0.001%
40	4.783	1162	1164	1167	rVB	379	165	0.01%	0.002%
41	4.879	1193	1194	1197	rBV2	246	96	0.01%	0.001%
42	4.895	1197	1199	1202	rVV3	664	360	0.03%	0.003%
43	4.921	1202	1207	1208	rVV3	386	214	0.02%	0.002%
44	4.940	1212	1213	1215	rBV3	259	130	0.01%	0.001%
45	4.973	1220	1223	1226	rBV3	494	438	0.03%	0.004%
46	5.037	1226	1243	1272	rBV3	525691	1343834	100.00%	12.651%
47	5.342	1336	1338	1340	rBV2	519	242	0.02%	0.002%
48	5.465	1372	1376	1378	rBV3	522	371	0.03%	0.003%
49	5.474	1378	1379	1381	rVV	636	257	0.02%	0.002%
50	5.500	1385	1387	1388	rBV	328	107	0.01%	0.001%
51	5.510	1388	1390	1394	rVB3	660	402	0.03%	0.004%
52	5.529	1394	1396	1399	rBV3	774	487	0.04%	0.005%
53	5.564	1404	1407	1410	rBV3	643	480	0.04%	0.005%
54	5.609	1410	1421	1448	rBV	384735	779474	58.00%	7.338%
55	5.860	1497	1499	1500	rBV	476	155	0.01%	0.001%
56	5.915	1505	1516	1532	rBV5	15888	35394	2.63%	0.333%
57	6.063	1549	1562	1591	rBV	293948	605204	45.04%	5.698%
58	6.339	1647	1648	1649	rBV	288	95	0.01%	0.001%
59	6.391	1662	1664	1665	rBV	367	176	0.01%	0.002%
60	6.423	1672	1674	1677	rVB2	332	176	0.01%	0.002%
61	6.439	1677	1679	1682	rBV2	333	201	0.01%	0.002%
62	6.493	1694	1696	1697	rBV	437	194	0.01%	0.002%
63	6.574	1719	1721	1722	rVB	418	106	0.01%	0.001%
64	6.616	1733	1734	1737	rVB	313	114	0.01%	0.001%
65	6.796	1784	1790	1794	rBV3	861	767	0.06%	0.007%
66	6.818	1794	1797	1798	rBV2	462	239	0.02%	0.002%
67	6.982	1836	1848	1870	rBV	163270	302030	22.48%	2.843%
68	7.310	1939	1950	1970	rBV	609189	1062483	79.06%	10.002%
69	7.619	2037	2046	2070	rBV	122552	215597	16.04%	2.030%
70	7.940	2137	2146	2158	rVB4	8129	14454	1.08%	0.136%
71	8.043	2176	2178	2179	rBV2	796	280	0.02%	0.003%
72	8.085	2181	2191	2216	rBV	450595	791272	58.88%	7.449%
73	8.622	2356	2358	2359	rBV2	958	401	0.03%	0.004%
74	8.847	2417	2428	2453	rBV	612298	1020306	75.93%	9.605%
75	9.960	2771	2774	2777	rBV3	655	500	0.04%	0.005%
76	10.214	2841	2853	2873	rBV	478739	757810	56.39%	7.134%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027971.D
 Acq On : 20 Sep 2022 18:49
 Operator : SY/MD
 Sample : N4619-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E22

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

77	10.381	2898	2905	2913	rBV3	7648	11007	0.82%	0.104%
78	10.448	2924	2926	2929	rBV2	764	474	0.04%	0.004%
79	10.570	2962	2964	2966	rBV3	1558	769	0.06%	0.007%
80	11.072	3117	3120	3122	rBV2	845	536	0.04%	0.005%
81	11.107	3129	3131	3133	rBV	1238	668	0.05%	0.006%
82	11.246	3163	3174	3192	rBV	579334	887853	66.07%	8.358%
83	11.622	3280	3291	3310	rBV	608945	952940	70.91%	8.971%
84	12.027	3416	3417	3419	rBV2	866	484	0.04%	0.005%
85	13.985	4024	4026	4030	rBV3	1154	699	0.05%	0.007%




Sum of corrected areas: 10622220

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027971.D
Acq On : 20 Sep 2022 18:49
Operator : SY/MD
Sample : N4619-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

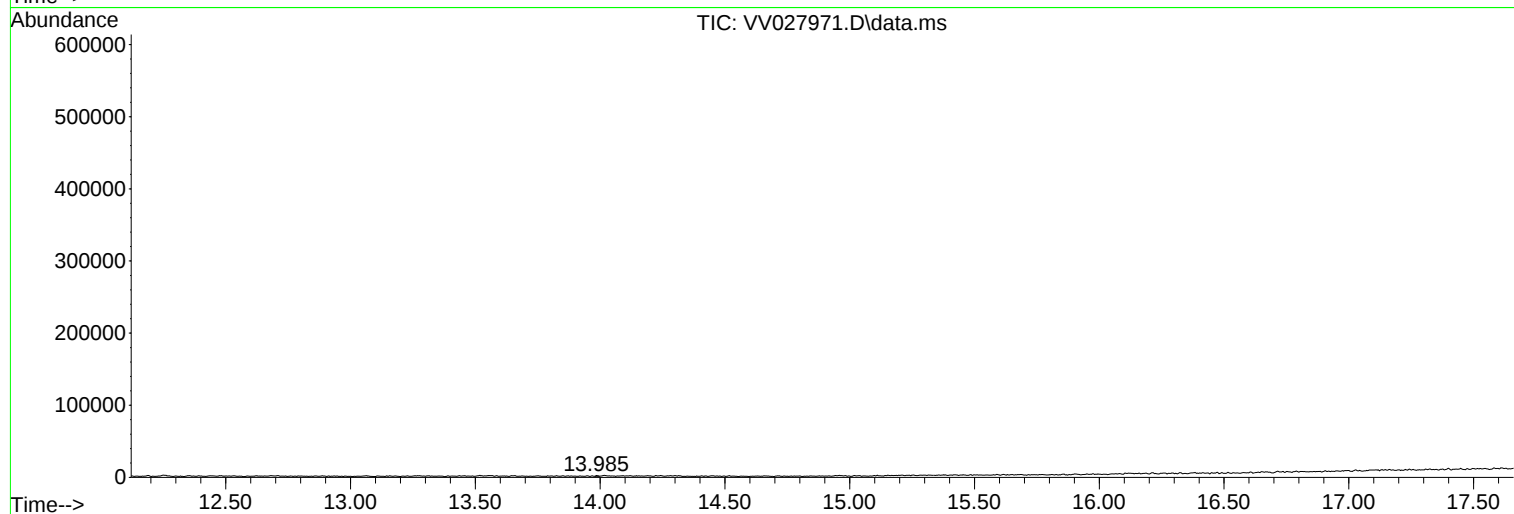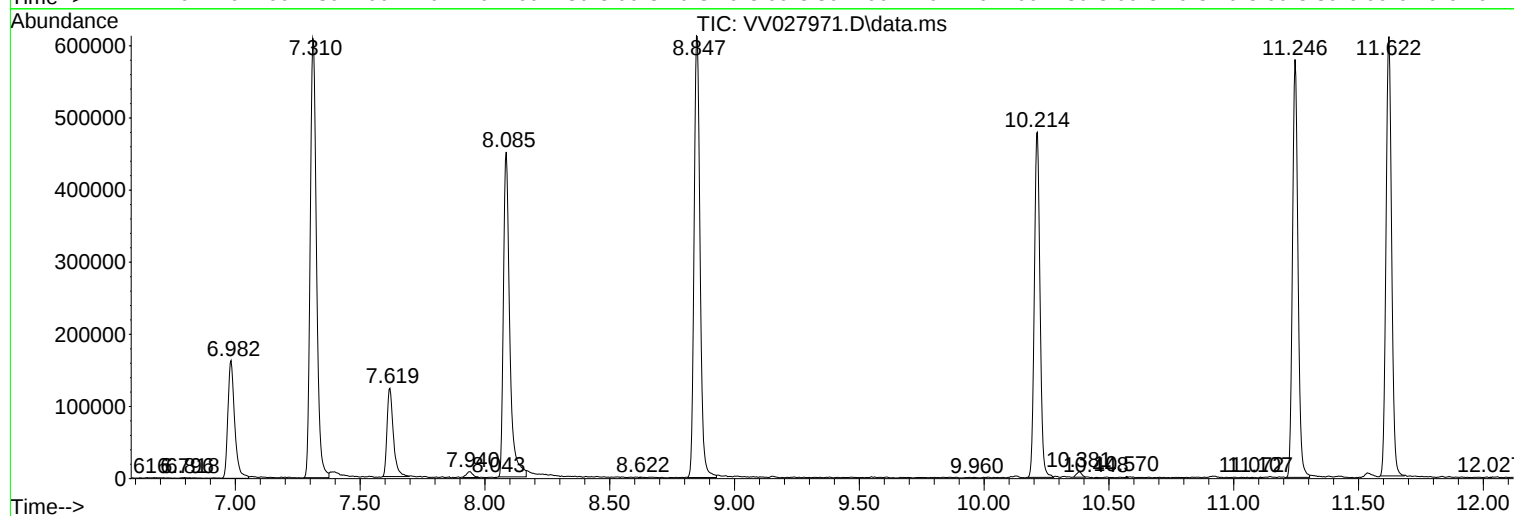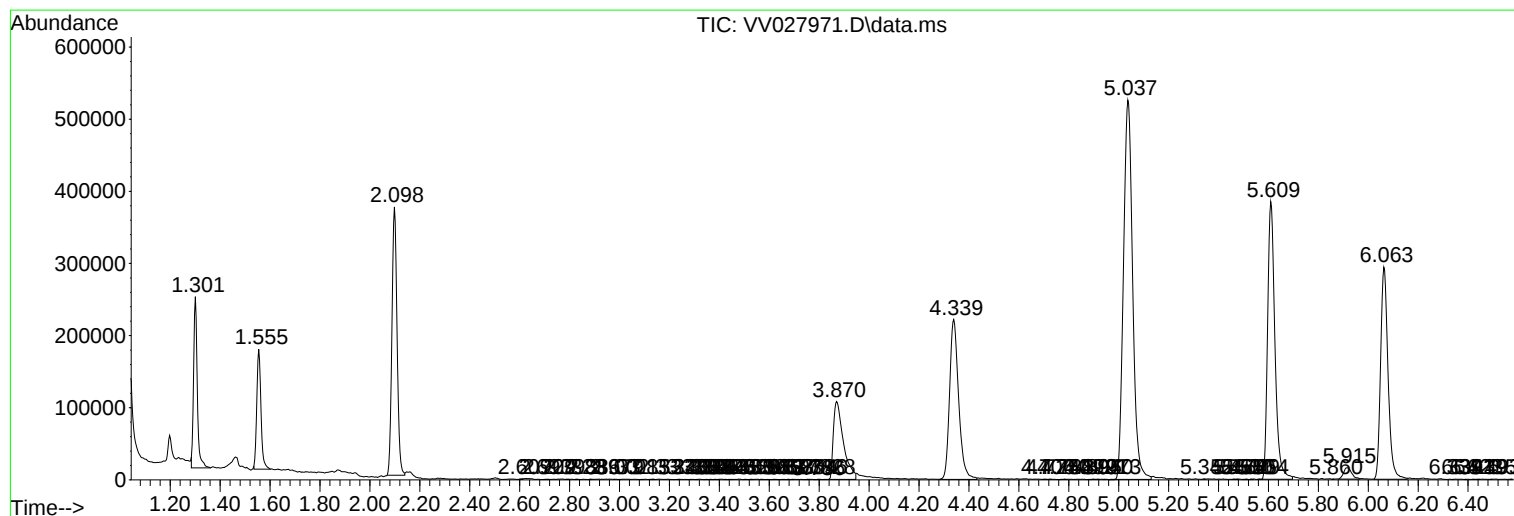

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027971.D
Acq On : 20 Sep 2022 18:49
Operator : SY/MD
Sample : N4619-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027971.D
Acq On : 20 Sep 2022 18:49
Operator : SY/MD
Sample : N4619-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E22

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------