

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027972.D
 Acq On : 20 Sep 2022 19:14
 Operator : SY/MD
 Sample : N4619-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027972.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	100	rVB	226634	232905	15.86%	2.124%
2	1.555	154	160	176	rVB	164447	189992	12.94%	1.733%
3	2.098	320	329	345	rBV	368634	528713	36.01%	4.822%
4	2.278	378	385	389	rBV6	1203	1820	0.12%	0.017%
5	2.352	403	408	413	rBV2	584	738	0.05%	0.007%
6	2.429	429	432	436	rBV2	557	503	0.03%	0.005%
7	2.494	445	452	453	rBV4	1517	1410	0.10%	0.013%
8	2.542	464	467	468	rBV	423	266	0.02%	0.002%
9	2.597	480	484	485	rBV2	432	235	0.02%	0.002%
10	2.629	490	494	495	rBV2	700	508	0.03%	0.005%
11	2.687	506	512	516	rVB3	443	413	0.03%	0.004%
12	2.716	518	521	522	rBV	491	321	0.02%	0.003%
13	2.744	527	530	533	rBV	487	420	0.03%	0.004%
14	2.783	538	542	543	rBV2	419	262	0.02%	0.002%
15	2.825	551	555	558	rBV2	232	206	0.01%	0.002%
16	2.863	565	567	569	rBV	391	229	0.02%	0.002%
17	3.037	619	621	623	rBV2	596	275	0.02%	0.003%
18	3.143	650	654	658	rBV3	316	295	0.02%	0.003%
19	3.175	661	664	667	rBV2	327	231	0.02%	0.002%
20	3.227	676	680	682	rBV	531	460	0.03%	0.004%
21	3.326	707	711	713	rBV4	738	453	0.03%	0.004%
22	3.355	718	720	722	rVV	448	226	0.02%	0.002%
23	3.407	732	736	739	rBV	727	495	0.03%	0.005%
24	3.439	742	746	748	rBV2	617	352	0.02%	0.003%
25	3.474	753	757	762	rVB3	891	580	0.04%	0.005%
26	3.539	774	777	779	rBV2	424	264	0.02%	0.002%
27	3.716	830	832	835	rBV3	433	332	0.02%	0.003%
28	3.870	870	880	913	rBV2	119559	357527	24.35%	3.261%
29	4.339	1011	1026	1052	rBV	236757	594745	40.51%	5.425%
30	4.789	1162	1166	1168	rBV3	697	703	0.05%	0.006%
31	4.857	1185	1187	1189	rVB2	618	206	0.01%	0.002%
32	4.896	1197	1199	1201	rVB2	924	391	0.03%	0.004%
33	4.921	1201	1207	1209	rBV4	816	918	0.06%	0.008%
34	5.037	1227	1243	1276	rBV2	572374	1468268	100.00%	13.392%
35	5.551	1399	1403	1406	rBV5	910	673	0.05%	0.006%
36	5.609	1410	1421	1454	rVV	418003	851253	57.98%	7.764%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027972.D
 Acq On : 20 Sep 2022 19:14
 Operator : SY/MD
 Sample : N4619-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.063	1550	1562	1583	rBV	329628	665097	45.30%	6.066%
38	6.458	1683	1685	1686	rBV2	828	327	0.02%	0.003%
39	6.606	1728	1731	1732	rBV2	618	367	0.02%	0.003%
40	6.812	1793	1795	1799	rBV4	949	846	0.06%	0.008%
41	6.867	1810	1812	1813	rBV2	647	229	0.02%	0.002%
42	6.982	1838	1848	1868	rBV	167600	309739	21.10%	2.825%
43	7.310	1937	1950	1968	rBV	608552	1065597	72.58%	9.719%
44	7.619	2036	2046	2070	rBV	114392	206241	14.05%	1.881%
45	7.937	2138	2145	2155	rVB3	5971	10152	0.69%	0.093%
46	8.085	2181	2191	2215	rBV	448559	791082	53.88%	7.215%
47	8.583	2340	2346	2348	rBV3	932	862	0.06%	0.008%
48	8.706	2381	2384	2385	rBV2	1000	537	0.04%	0.005%
49	8.850	2417	2429	2449	rBV	630937	1027320	69.97%	9.370%
50	9.355	2584	2586	2587	rBV	398	218	0.01%	0.002%
51	9.394	2595	2598	2600	rBV4	903	519	0.04%	0.005%
52	9.548	2643	2646	2649	rBV4	909	692	0.05%	0.006%
53	9.677	2683	2686	2687	rBV2	690	502	0.03%	0.005%
54	9.699	2691	2693	2695	rBV3	817	365	0.02%	0.003%
55	9.876	2745	2748	2752	rBV2	961	902	0.06%	0.008%
56	9.937	2764	2767	2770	rBV3	1064	590	0.04%	0.005%
57	9.956	2770	2773	2775	rBV3	840	371	0.03%	0.003%
58	10.214	2841	2853	2869	rBV	475805	760404	51.79%	6.935%
59	10.381	2899	2905	2917	rVB3	6677	11302	0.77%	0.103%
60	10.426	2917	2919	2924	rVB3	1291	863	0.06%	0.008%
61	10.448	2924	2926	2927	rBV2	760	370	0.03%	0.003%
62	10.815	3038	3040	3043	rBV2	923	580	0.04%	0.005%
63	10.966	3085	3087	3088	rBV2	823	353	0.02%	0.003%
64	11.146	3140	3143	3146	rBV3	1093	803	0.05%	0.007%
65	11.246	3163	3174	3192	rBV	581440	896281	61.04%	8.175%
66	11.622	3279	3291	3306	rBV	612929	959936	65.38%	8.755%
67	11.921	3381	3384	3386	rBV3	1077	582	0.04%	0.005%
68	12.037	3417	3420	3421	rBV3	474	239	0.02%	0.002%
69	12.079	3431	3433	3436	rBV2	534	325	0.02%	0.003%
70	12.130	3447	3449	3451	rBV2	543	273	0.02%	0.002%
71	12.243	3482	3484	3486	rBV2	1096	706	0.05%	0.006%
72	12.352	3516	3518	3524	rBV6	476	382	0.03%	0.003%
73	12.439	3542	3545	3549	rBV3	407	262	0.02%	0.002%
74	12.461	3549	3552	3556	rBV2	303	245	0.02%	0.002%
75	12.622	3599	3602	3605	rBV3	441	259	0.02%	0.002%
76	12.751	3640	3642	3644	rBV	390	220	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027972.D
 Acq On : 20 Sep 2022 19:14
 Operator : SY/MD
 Sample : N4619-08
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E23

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	12.805	3657	3659	3663	rBV3	568	383	0.03%	0.003%
78	12.902	3685	3689	3694	rBV3	479	536	0.04%	0.005%
79	12.985	3711	3715	3718	rBV2	564	510	0.03%	0.005%
80	13.056	3733	3737	3738	rBV2	446	367	0.02%	0.003%
81	13.143	3759	3764	3765	rBV	430	340	0.02%	0.003%
82	13.210	3783	3785	3789	rVB3	582	336	0.02%	0.003%
83	13.323	3817	3820	3822	rVB2	574	330	0.02%	0.003%
84	13.342	3822	3826	3828	rBV3	517	415	0.03%	0.004%
85	13.406	3841	3846	3849	rVB2	498	448	0.03%	0.004%
86	13.426	3849	3852	3854	rBV2	549	216	0.01%	0.002%
87	13.442	3854	3857	3858	rBV	705	393	0.03%	0.004%
88	13.480	3865	3869	3871	rBV	460	309	0.02%	0.003%
89	13.503	3873	3876	3878	rBV	592	465	0.03%	0.004%
90	13.538	3885	3887	3892	rVB2	561	423	0.03%	0.004%
91	13.580	3895	3900	3903	rBV3	556	374	0.03%	0.003%
92	13.619	3908	3912	3916	rVB2	468	483	0.03%	0.004%
93	13.651	3916	3922	3924	rBV4	753	714	0.05%	0.007%
94	13.728	3944	3946	3950	rBV	633	439	0.03%	0.004%
95	13.747	3950	3952	3954	rBV3	487	279	0.02%	0.003%
96	13.802	3967	3969	3971	rBV	353	184	0.01%	0.002%
97	13.902	3998	4000	4003	rVB2	540	218	0.01%	0.002%
98	14.156	4076	4079	4080	rBV2	531	302	0.02%	0.003%
99	14.255	4108	4110	4114	rVB3	850	575	0.04%	0.005%
100	14.918	4313	4316	4317	rBV2	869	417	0.03%	0.004%




Sum of corrected areas: 10963984

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027972.D
Acq On : 20 Sep 2022 19:14
Operator : SY/MD
Sample : N4619-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

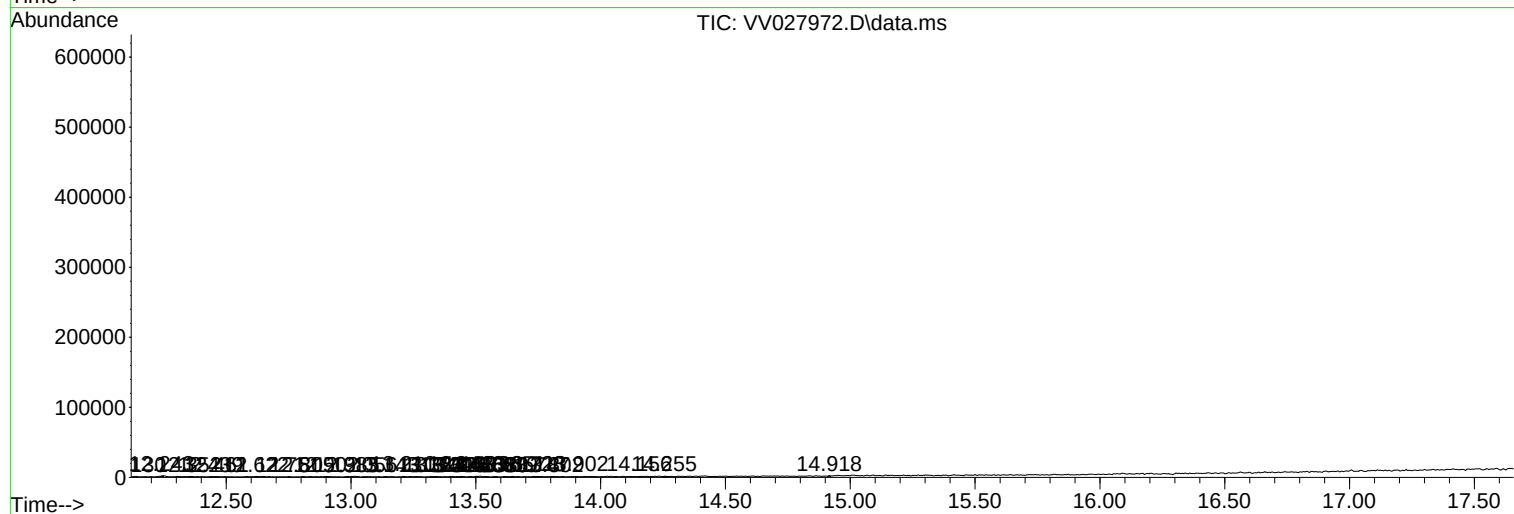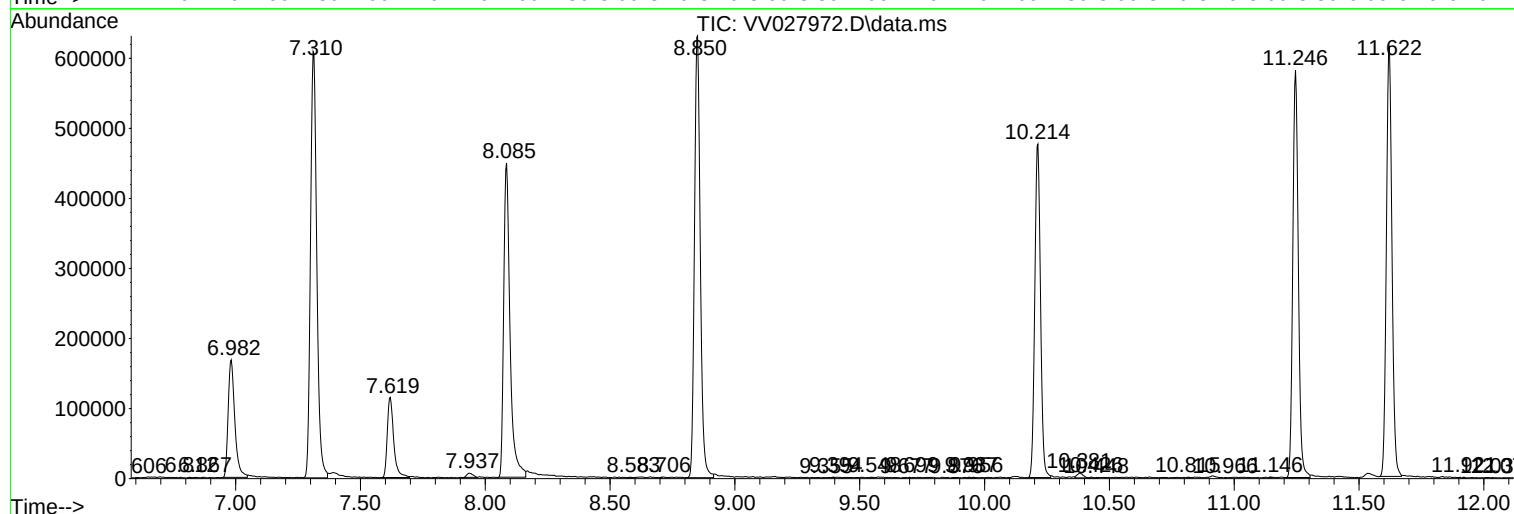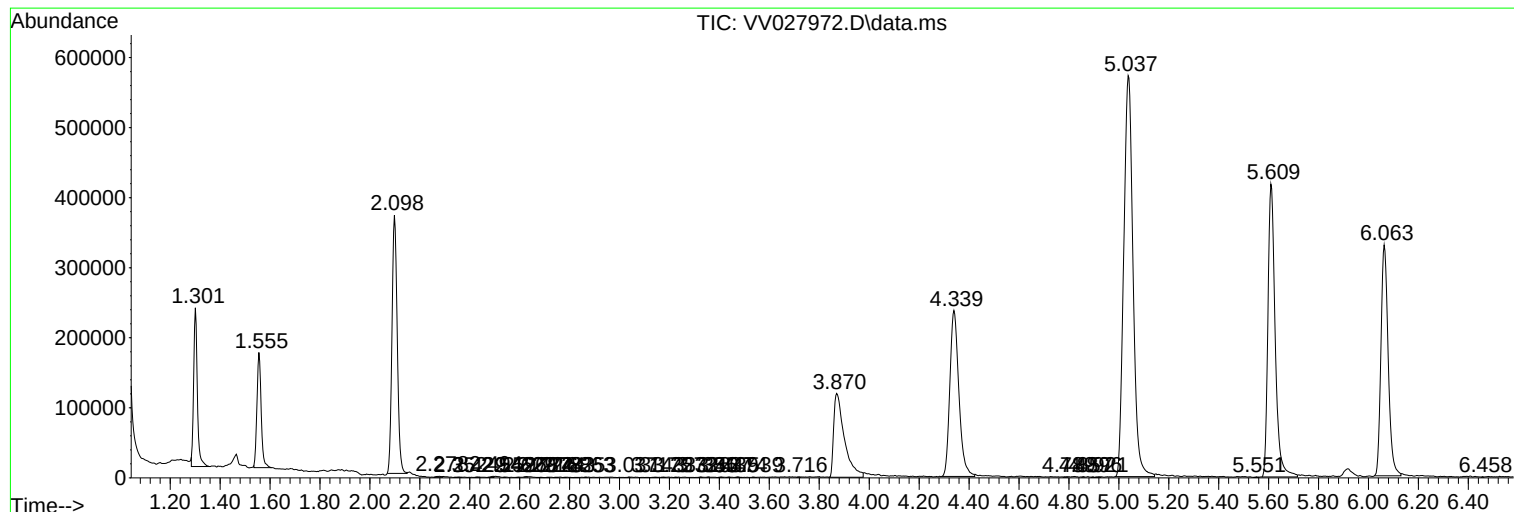

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027972.D
Acq On : 20 Sep 2022 19:14
Operator : SY/MD
Sample : N4619-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027972.D
Acq On : 20 Sep 2022 19:14
Operator : SY/MD
Sample : N4619-08
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E23

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc