

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027974.D
 Acq On : 20 Sep 2022 20:03
 Operator : SY/MD
 Sample : N4619-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV027974.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	238014	242787	17.79%	2.315%
2	1.558	155	161	176	rVB	174484	202037	14.81%	1.926%
3	2.098	320	329	343	rBV	378597	540771	39.63%	5.156%
4	2.355	407	409	411	rVB2	559	237	0.02%	0.002%
5	2.368	411	413	416	rBV2	548	304	0.02%	0.003%
6	2.384	416	418	423	rVV3	491	292	0.02%	0.003%
7	2.497	447	453	456	rBV7	1438	1793	0.13%	0.017%
8	2.587	477	481	483	rBV2	371	285	0.02%	0.003%
9	2.600	483	485	487	rBV	469	284	0.02%	0.003%
10	2.703	514	517	521	rBV5	539	442	0.03%	0.004%
11	2.722	521	523	526	rVB2	400	253	0.02%	0.002%
12	2.760	533	535	536	rBV	494	217	0.02%	0.002%
13	2.825	551	555	558	rBV2	400	302	0.02%	0.003%
14	2.883	569	573	574	rBV	340	219	0.02%	0.002%
15	3.021	614	616	617	rBV2	523	174	0.01%	0.002%
16	3.031	617	619	624	rVB3	584	326	0.02%	0.003%
17	3.079	629	634	637	rVB2	300	264	0.02%	0.003%
18	3.095	637	639	641	rBV2	262	139	0.01%	0.001%
19	3.117	644	646	651	rVB2	586	420	0.03%	0.004%
20	3.182	665	666	669	rBV2	383	160	0.01%	0.002%
21	3.281	692	697	700	rVB4	460	418	0.03%	0.004%
22	3.297	700	702	707	rBV3	469	432	0.03%	0.004%
23	3.416	736	739	742	rVB	449	305	0.02%	0.003%
24	3.432	742	744	748	rBV2	382	323	0.02%	0.003%
25	3.487	758	761	764	rBV2	400	251	0.02%	0.002%
26	3.616	794	801	804	rBV4	422	453	0.03%	0.004%
27	3.651	807	812	815	rBV2	264	288	0.02%	0.003%
28	3.674	815	819	821	rBV2	453	251	0.02%	0.002%
29	3.709	828	830	834	rBV2	444	307	0.02%	0.003%
30	3.751	840	843	845	rBV	479	292	0.02%	0.003%
31	3.780	850	852	855	rVB2	286	171	0.01%	0.002%
32	3.873	871	881	918	rBV	114906	320463	23.49%	3.056%
33	4.339	1011	1026	1051	rBV	225315	555539	40.71%	5.297%
34	4.821	1174	1176	1179	rVB2	274	146	0.01%	0.001%
35	4.902	1198	1201	1202	rBV	325	151	0.01%	0.001%
36	4.944	1212	1214	1217	rVB2	372	145	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027974.D
 Acq On : 20 Sep 2022 20:03
 Operator : SY/MD
 Sample : N4619-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.040	1227	1244	1273	rBV2	531978	1364487	100.00%	13.010%
38	5.310	1325	1328	1332	rVB3	916	630	0.05%	0.006%
39	5.329	1332	1334	1336	rBV2	583	334	0.02%	0.003%
40	5.429	1361	1365	1370	rBB4	718	718	0.05%	0.007%
41	5.458	1371	1374	1382	rBV3	575	477	0.03%	0.005%
42	5.497	1384	1386	1392	rBV3	710	620	0.05%	0.006%
43	5.545	1396	1401	1402	rBV2	425	209	0.02%	0.002%
44	5.609	1410	1421	1458	rBV	382762	775491	56.83%	7.394%
45	5.915	1504	1516	1532	rBV6	23630	50855	3.73%	0.485%
46	6.063	1549	1562	1595	rVV	301900	615755	45.13%	5.871%
47	6.178	1595	1598	1600	rBV4	998	548	0.04%	0.005%
48	6.278	1627	1629	1632	rBV3	651	422	0.03%	0.004%
49	6.384	1657	1662	1665	rBV3	389	408	0.03%	0.004%
50	6.410	1668	1670	1677	rVB2	825	779	0.06%	0.007%
51	6.445	1677	1681	1685	rBV3	674	755	0.06%	0.007%
52	6.516	1699	1703	1705	rBV2	780	437	0.03%	0.004%
53	6.673	1750	1752	1753	rBV2	353	185	0.01%	0.002%
54	6.751	1773	1776	1779	rBV2	472	264	0.02%	0.003%
55	6.764	1779	1780	1784	rVB2	244	153	0.01%	0.001%
56	6.825	1798	1799	1801	rVB2	391	139	0.01%	0.001%
57	6.847	1801	1806	1809	rBV4	593	501	0.04%	0.005%
58	6.899	1819	1822	1825	rBV	406	263	0.02%	0.003%
59	6.931	1829	1832	1836	rBV2	412	403	0.03%	0.004%
60	6.982	1836	1848	1874	rBV2	155374	290594	21.30%	2.771%
61	7.310	1936	1950	1970	rBV	599406	1042521	76.40%	9.940%
62	7.619	2036	2046	2066	rBV	117772	202831	14.87%	1.934%
63	7.805	2100	2104	2107	rVB2	621	543	0.04%	0.005%
64	7.821	2107	2109	2110	rBV	486	201	0.01%	0.002%
65	7.905	2133	2135	2137	rBV2	805	332	0.02%	0.003%
66	8.085	2181	2191	2224	rBV	408639	725167	53.15%	6.914%
67	8.487	2314	2316	2317	rVB	601	183	0.01%	0.002%
68	8.503	2317	2321	2324	rBV5	662	603	0.04%	0.006%
69	8.567	2339	2341	2344	rBV2	517	332	0.02%	0.003%
70	8.599	2350	2351	2353	rBV	537	247	0.02%	0.002%
71	8.702	2381	2383	2385	rBV3	535	343	0.03%	0.003%
72	8.847	2417	2428	2452	rBV	573891	939129	68.83%	8.955%
73	9.197	2534	2537	2540	rBV3	881	629	0.05%	0.006%
74	9.278	2559	2562	2563	rBV2	383	231	0.02%	0.002%
75	9.316	2571	2574	2575	rBV2	627	349	0.03%	0.003%
76	9.339	2579	2581	2585	rVB4	721	380	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027974.D
 Acq On : 20 Sep 2022 20:03
 Operator : SY/MD
 Sample : N4619-10
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E26

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.387	2594	2596	2599	rBV3	411	254	0.02%	0.002%
78	9.400	2599	2600	2603	rVB3	371	157	0.01%	0.001%
79	9.464	2616	2620	2623	rBV2	546	402	0.03%	0.004%
80	9.480	2623	2625	2628	rVB2	401	170	0.01%	0.002%
81	9.609	2661	2665	2668	rBV3	688	600	0.04%	0.006%
82	9.628	2668	2671	2672	rBV2	440	261	0.02%	0.002%
83	9.677	2684	2686	2689	rBV3	677	456	0.03%	0.004%
84	9.722	2698	2700	2703	rVB2	487	210	0.02%	0.002%
85	9.744	2703	2707	2710	rBV5	725	527	0.04%	0.005%
86	9.892	2751	2753	2755	rBV3	894	470	0.03%	0.004%
87	10.114	2818	2822	2823	rBV3	1483	1136	0.08%	0.011%
88	10.214	2841	2853	2871	rBV	476933	760958	55.77%	7.256%
89	10.442	2922	2924	2927	rBV	748	520	0.04%	0.005%
90	10.538	2950	2954	2956	rBV4	1262	1069	0.08%	0.010%
91	10.979	3086	3091	3094	rBV5	1562	1396	0.10%	0.013%
92	11.246	3163	3174	3194	rBV	555268	857159	62.82%	8.173%
93	11.532	3257	3263	3272	rBV5	10200	17819	1.31%	0.170%
94	11.622	3280	3291	3308	rBV	609372	949428	69.58%	9.053%
95	12.156	3454	3457	3460	rBV3	902	626	0.05%	0.006%
96	12.204	3469	3472	3476	rBV6	1253	1010	0.07%	0.010%
97	12.284	3496	3497	3501	rVB3	988	423	0.03%	0.004%
98	12.580	3587	3589	3591	rBV3	941	409	0.03%	0.004%
99	12.644	3607	3609	3613	rBV3	1226	985	0.07%	0.009%
100	13.570	3895	3897	3899	rBV2	582	246	0.02%	0.002%




Sum of corrected areas: 10487780

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027974.D
Acq On : 20 Sep 2022 20:03
Operator : SY/MD
Sample : N4619-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

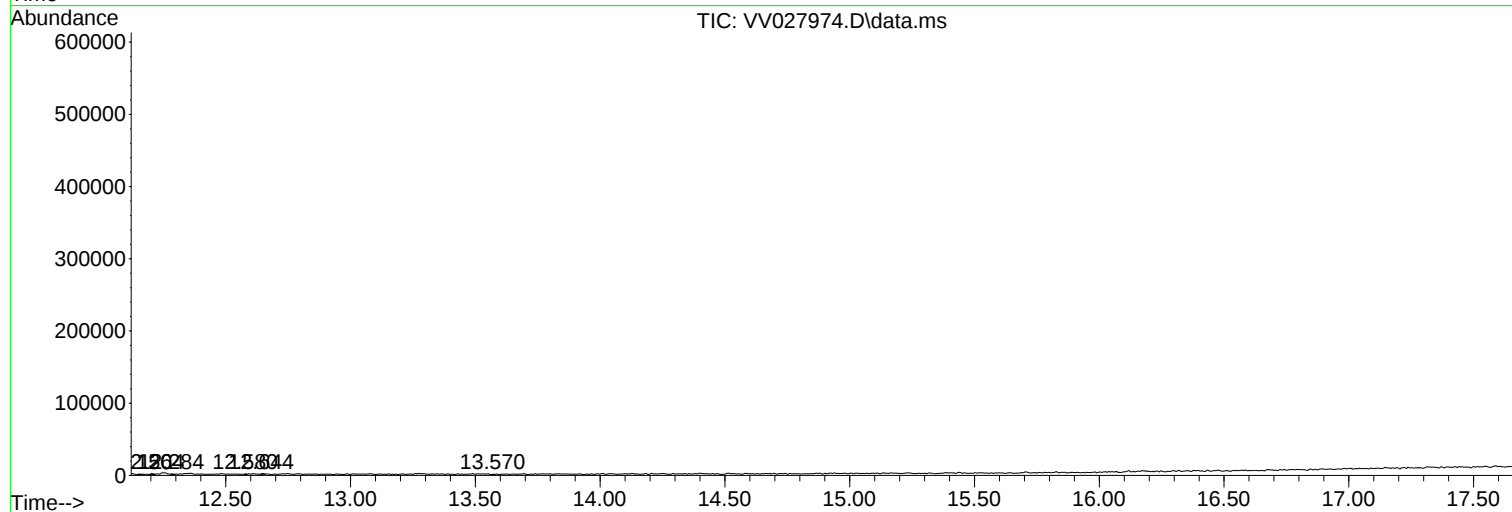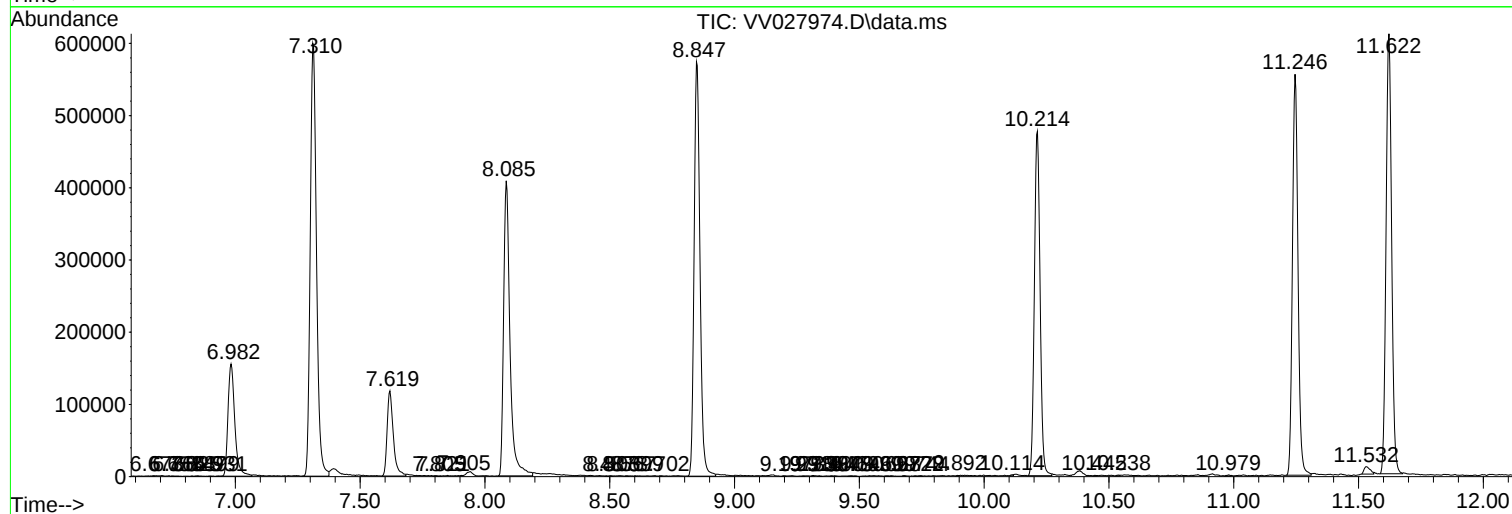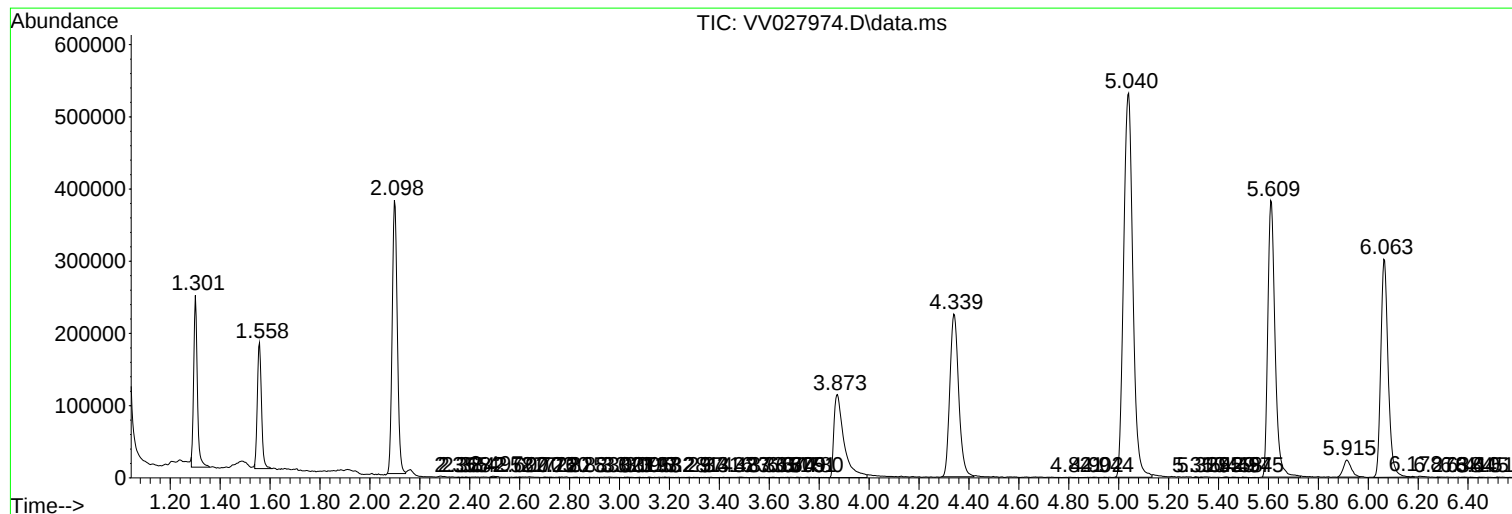

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027974.D
Acq On : 20 Sep 2022 20:03
Operator : SY/MD
Sample : N4619-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027974.D
Acq On : 20 Sep 2022 20:03
Operator : SY/MD
Sample : N4619-10
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E26

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------