

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027975.D
 Acq On : 20 Sep 2022 20:28
 Operator : SY/MD
 Sample : N4619-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027975.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	237240	244744	16.24%	2.183%
2	1.558	155	161	176	rVB	174519	201662	13.38%	1.799%
3	2.098	320	329	348	rBV2	399309	603492	40.03%	5.383%
4	2.246	374	375	378	rBV	544	363	0.02%	0.003%
5	2.320	397	398	402	rVB4	546	225	0.01%	0.002%
6	2.378	413	416	419	rBV2	651	602	0.04%	0.005%
7	2.436	429	434	436	rBV5	1111	891	0.06%	0.008%
8	2.507	448	456	461	rBV7	1587	2135	0.14%	0.019%
9	2.690	510	513	516	rVB3	575	357	0.02%	0.003%
10	2.732	523	526	528	rVV2	422	286	0.02%	0.003%
11	2.870	565	569	572	rBV4	1049	887	0.06%	0.008%
12	2.886	572	574	577	rVV2	518	258	0.02%	0.002%
13	2.947	591	593	594	rBV	795	299	0.02%	0.003%
14	3.073	630	632	634	rBV3	734	398	0.03%	0.004%
15	3.127	647	649	650	rBV	627	236	0.02%	0.002%
16	3.282	694	697	700	rBV3	643	544	0.04%	0.005%
17	3.368	720	724	729	rBV5	623	519	0.03%	0.005%
18	3.439	743	746	747	rBV2	563	352	0.02%	0.003%
19	3.516	768	770	772	rBV	545	294	0.02%	0.003%
20	3.558	781	783	786	rBV2	1086	400	0.03%	0.004%
21	3.674	818	819	824	rVB	454	279	0.02%	0.002%
22	3.699	824	827	830	rBV3	683	548	0.04%	0.005%
23	3.873	871	881	917	rBV	135306	436775	28.97%	3.896%
24	4.278	1005	1007	1010	rBV3	775	495	0.03%	0.004%
25	4.339	1011	1026	1048	rBV2	243472	609677	40.44%	5.438%
26	4.706	1138	1140	1142	rVB2	887	354	0.02%	0.003%
27	4.719	1142	1144	1148	rBV2	418	248	0.02%	0.002%
28	4.896	1197	1199	1202	rVB2	923	450	0.03%	0.004%
29	4.915	1204	1205	1208	rBV	595	279	0.02%	0.002%
30	5.037	1227	1243	1278	rBV2	579088	1507454	100.00%	13.446%
31	5.375	1345	1348	1350	rBV3	1210	695	0.05%	0.006%
32	5.471	1376	1378	1379	rBV	695	256	0.02%	0.002%
33	5.609	1408	1421	1449	rBV	411206	837432	55.55%	7.470%
34	5.883	1502	1506	1507	rBV3	1437	999	0.07%	0.009%
35	6.063	1550	1562	1596	rVB	338506	686768	45.56%	6.126%
36	6.346	1648	1650	1655	rVB3	1188	832	0.06%	0.007%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027975.D
 Acq On : 20 Sep 2022 20:28
 Operator : SY/MD
 Sample : N4619-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.400	1665	1667	1670	rVB4	1036	485	0.03%	0.004%
38	6.439	1676	1679	1681	rBV3	885	589	0.04%	0.005%
39	6.481	1690	1692	1694	rBV4	674	331	0.02%	0.003%
40	6.503	1697	1699	1700	rVB2	751	238	0.02%	0.002%
41	6.526	1700	1706	1709	rBV5	986	1196	0.08%	0.011%
42	6.571	1715	1720	1723	rVB4	965	664	0.04%	0.006%
43	6.658	1740	1747	1748	rBV5	1256	1432	0.09%	0.013%
44	6.802	1789	1792	1794	rBV2	647	382	0.03%	0.003%
45	6.828	1798	1800	1803	rVB3	771	355	0.02%	0.003%
46	6.860	1805	1810	1813	rBV4	946	672	0.04%	0.006%
47	6.892	1818	1820	1822	rVB	528	240	0.02%	0.002%
48	6.921	1822	1829	1830	rBV2	678	643	0.04%	0.006%
49	6.982	1837	1848	1866	rBV	163197	299749	19.88%	2.674%
50	7.310	1939	1950	1969	rBV	627754	1097352	72.80%	9.788%
51	7.619	2036	2046	2064	rBV	121861	218187	14.47%	1.946%
52	8.085	2181	2191	2227	rBV	458952	827298	54.88%	7.379%
53	8.432	2297	2299	2301	rBV3	1402	634	0.04%	0.006%
54	8.696	2379	2381	2384	rVB4	1134	663	0.04%	0.006%
55	8.751	2396	2398	2401	rBV	655	400	0.03%	0.004%
56	8.847	2417	2428	2452	rBV	620440	1009628	66.98%	9.006%
57	9.172	2526	2529	2536	rBV7	895	786	0.05%	0.007%
58	9.297	2565	2568	2570	rBV3	809	361	0.02%	0.003%
59	9.355	2583	2586	2587	rBV	931	456	0.03%	0.004%
60	9.461	2614	2619	2620	rBV3	839	611	0.04%	0.005%
61	9.484	2624	2626	2630	rBV2	712	506	0.03%	0.005%
62	9.516	2634	2636	2638	rBV3	560	329	0.02%	0.003%
63	9.677	2684	2686	2687	rBV2	931	360	0.02%	0.003%
64	9.725	2698	2701	2703	rBV2	759	475	0.03%	0.004%
65	9.902	2754	2756	2758	rVB2	591	246	0.02%	0.002%
66	10.027	2789	2795	2797	rBV5	1150	1075	0.07%	0.010%
67	10.069	2806	2808	2812	rVB2	564	405	0.03%	0.004%
68	10.092	2812	2815	2816	rBV2	475	285	0.02%	0.003%
69	10.124	2818	2825	2829	rVB7	1702	2188	0.15%	0.020%
70	10.214	2837	2853	2871	rBV	454033	718452	47.66%	6.408%
71	10.349	2893	2895	2897	rBV3	602	393	0.03%	0.004%
72	10.384	2898	2906	2915	rVV2	5823	10079	0.67%	0.090%
73	10.481	2934	2936	2940	rVB2	390	239	0.02%	0.002%
74	10.526	2948	2950	2955	rVB4	460	250	0.02%	0.002%
75	10.574	2963	2965	2967	rVV2	957	543	0.04%	0.005%
76	10.596	2970	2972	2975	rVB2	566	344	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027975.D
 Acq On : 20 Sep 2022 20:28
 Operator : SY/MD
 Sample : N4619-11
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E28

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.683	2996	2999	3002	rBV2	346	249	0.02%	0.002%
78	10.735	3011	3015	3016	rBV	523	338	0.02%	0.003%
79	10.744	3016	3018	3022	rVV4	763	461	0.03%	0.004%
80	10.841	3047	3048	3053	rVB4	634	418	0.03%	0.004%
81	10.863	3053	3055	3058	rBV	540	271	0.02%	0.002%
82	10.876	3058	3059	3063	rBV3	502	336	0.02%	0.003%
83	11.056	3114	3115	3118	rBV2	458	210	0.01%	0.002%
84	11.114	3131	3133	3134	rBV	771	364	0.02%	0.003%
85	11.140	3137	3141	3145	rVV5	1440	1341	0.09%	0.012%
86	11.246	3163	3174	3195	rBV	568720	872320	57.87%	7.781%
87	11.426	3227	3230	3233	rBV5	1748	1365	0.09%	0.012%
88	11.468	3240	3243	3244	rBV2	1015	553	0.04%	0.005%
89	11.535	3252	3264	3279	rBV4	11222	26470	1.76%	0.236%
90	11.622	3280	3291	3312	rVB	607975	958067	63.56%	8.546%
91	12.181	3464	3465	3467	rBV2	781	252	0.02%	0.002%
92	12.304	3501	3503	3508	rVB4	612	336	0.02%	0.003%
93	12.333	3508	3512	3515	rBV4	1355	1086	0.07%	0.010%
94	12.464	3551	3553	3558	rVB4	1193	740	0.05%	0.007%
95	12.503	3560	3565	3569	rBV6	961	1193	0.08%	0.011%
96	12.908	3688	3691	3693	rBV3	925	484	0.03%	0.004%
97	13.603	3905	3907	3910	rBV2	802	562	0.04%	0.005%
98	13.680	3929	3931	3934	rBV2	841	489	0.03%	0.004%
99	13.773	3957	3960	3961	rBV2	819	417	0.03%	0.004%
100	14.349	4137	4139	4144	rBV5	998	788	0.05%	0.007%




Sum of corrected areas: 11211116

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027975.D
Acq On : 20 Sep 2022 20:28
Operator : SY/MD
Sample : N4619-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

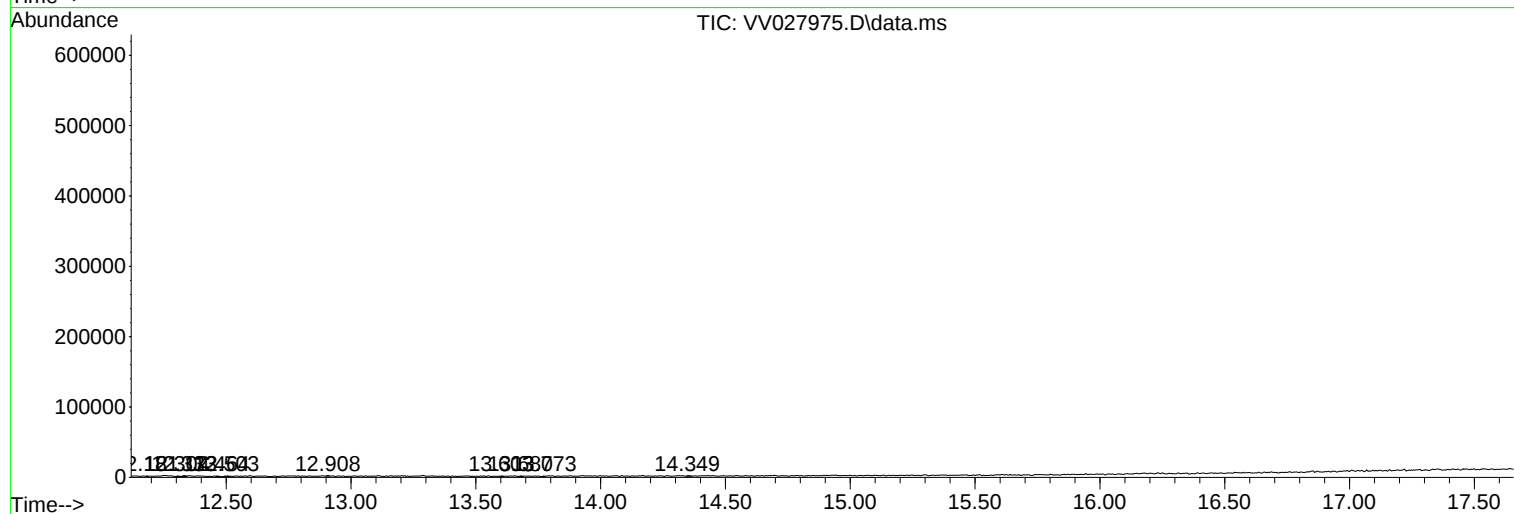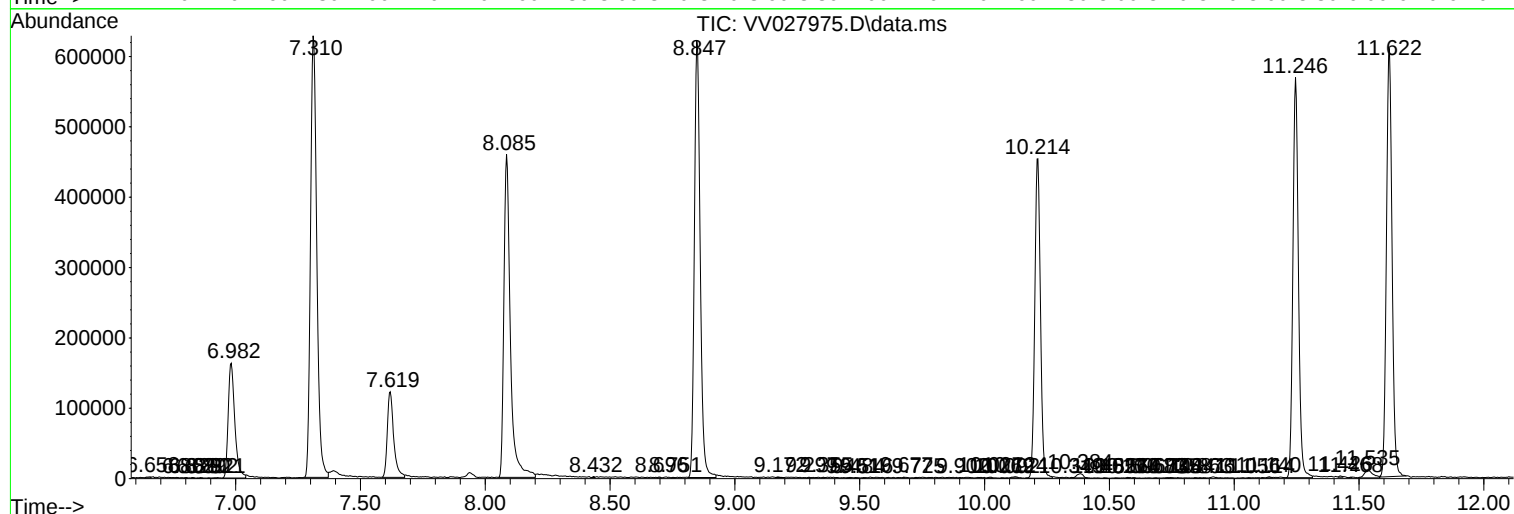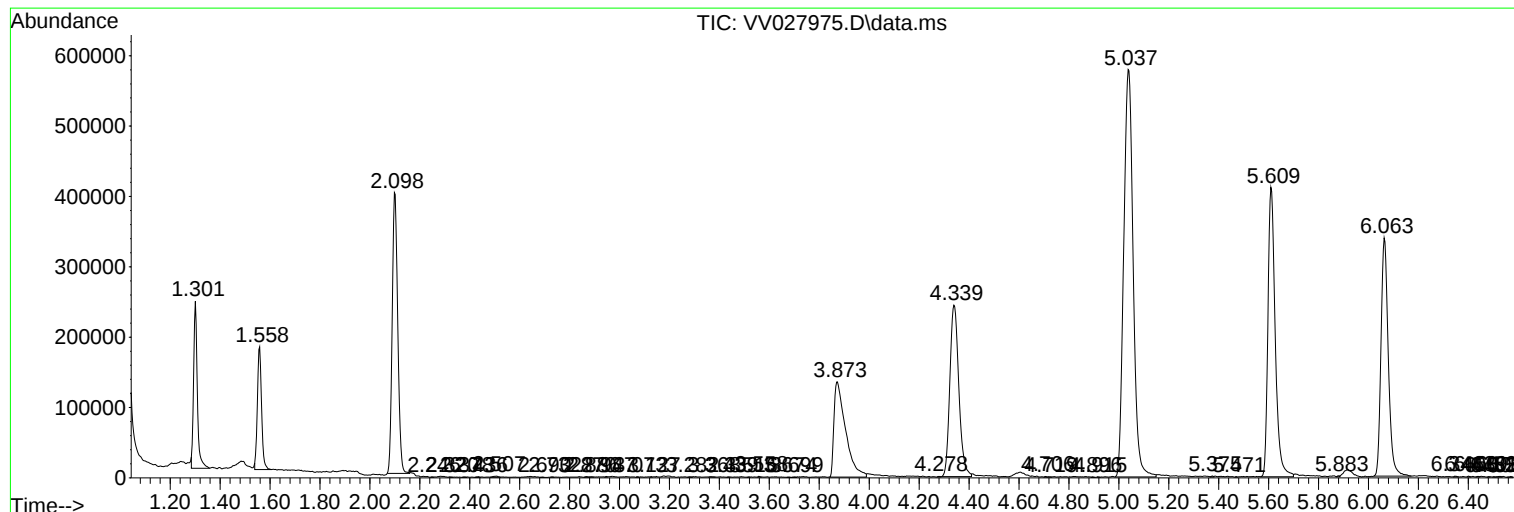

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027975.D
Acq On : 20 Sep 2022 20:28
Operator : SY/MD
Sample : N4619-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027975.D
Acq On : 20 Sep 2022 20:28
Operator : SY/MD
Sample : N4619-11
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E28

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------