

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027976.D
 Acq On : 20 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4619-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV027976.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	98	rVB	233671	238480	15.91%	2.038%
2	1.558	155	161	176	rVB	173369	199982	13.34%	1.709%
3	2.098	320	329	346	rBV	369979	534691	35.66%	4.570%
4	2.461	440	442	444	rBV2	526	297	0.02%	0.003%
5	2.551	468	470	474	rBV3	559	421	0.03%	0.004%
6	2.580	477	479	481	rVB3	320	91	0.01%	0.001%
7	2.757	527	534	547	rVB6	3824	6856	0.46%	0.059%
8	2.854	562	564	565	rBV2	203	106	0.01%	0.001%
9	2.873	569	570	571	rVV	350	86	0.01%	0.001%
10	2.886	571	574	577	rVV2	450	235	0.02%	0.002%
11	2.908	577	581	582	rVV2	253	145	0.01%	0.001%
12	2.934	586	589	591	rBV2	403	257	0.02%	0.002%
13	2.985	601	605	609	rBV2	351	299	0.02%	0.003%
14	3.005	609	611	614	rVB	374	217	0.01%	0.002%
15	3.047	622	624	628	rBV2	239	206	0.01%	0.002%
16	3.069	628	631	632	rVB	350	167	0.01%	0.001%
17	3.166	659	661	663	rBV3	401	206	0.01%	0.002%
18	3.227	676	680	682	rBV2	307	228	0.02%	0.002%
19	3.265	688	692	694	rBV	276	169	0.01%	0.001%
20	3.275	694	695	698	rVV2	402	232	0.02%	0.002%
21	3.288	698	699	704	rVB2	602	255	0.02%	0.002%
22	3.313	704	707	708	rBV	315	203	0.01%	0.002%
23	3.336	712	714	715	rBV	364	126	0.01%	0.001%
24	3.355	718	720	722	rBV	308	174	0.01%	0.001%
25	3.423	737	741	742	rBV	401	235	0.02%	0.002%
26	3.432	742	744	750	rVB2	614	467	0.03%	0.004%
27	3.465	751	754	756	rBV	338	175	0.01%	0.001%
28	3.493	762	763	764	rBV	331	113	0.01%	0.001%
29	3.526	771	773	776	rVB2	456	190	0.01%	0.002%
30	3.564	783	785	787	rVB	214	92	0.01%	0.001%
31	3.587	790	792	793	rVB	230	81	0.01%	0.001%
32	3.641	804	809	811	rVB	557	268	0.02%	0.002%
33	3.657	811	814	815	rBV	320	174	0.01%	0.001%
34	3.712	826	831	833	rBV3	500	388	0.03%	0.003%
35	3.735	836	838	841	rBV2	250	169	0.01%	0.001%
36	3.812	860	862	865	rVB	506	239	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027976.D
 Acq On : 20 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4619-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.838	865	870	871	rBV2	721	452	0.03%	0.004%
38	3.873	871	881	908	rBV	119738	353272	23.56%	3.020%
39	4.339	1012	1026	1052	rBV	243112	591669	39.46%	5.057%
40	4.686	1132	1134	1136	rBV3	812	555	0.04%	0.005%
41	4.818	1173	1175	1176	rVB2	775	181	0.01%	0.002%
42	5.037	1226	1243	1271	rBV2	581082	1499390	100.00%	12.816%
43	5.326	1330	1333	1334	rBV3	1016	561	0.04%	0.005%
44	5.358	1340	1343	1348	rBV5	1451	1265	0.08%	0.011%
45	5.554	1401	1404	1408	rVB2	1235	895	0.06%	0.008%
46	5.609	1409	1421	1445	rBV	404844	826137	55.10%	7.062%
47	5.908	1501	1514	1540	rBV	383468	760728	50.74%	6.502%
48	6.063	1551	1562	1586	rVB	336040	671873	44.81%	5.743%
49	6.390	1661	1664	1665	rBV2	946	564	0.04%	0.005%
50	6.837	1801	1803	1805	rBV	939	308	0.02%	0.003%
51	6.982	1837	1848	1877	rBV	170507	322104	21.48%	2.753%
52	7.310	1939	1950	1971	rBV	639902	1115264	74.38%	9.533%
53	7.619	2036	2046	2065	rBV	122998	216678	14.45%	1.852%
54	7.940	2135	2146	2155	rBV3	5425	10529	0.70%	0.090%
55	8.085	2181	2191	2219	rBV	444451	796617	53.13%	6.809%
56	8.773	2402	2405	2406	rBV2	952	455	0.03%	0.004%
57	8.847	2418	2428	2452	rBV	615073	999697	66.67%	8.545%
58	9.574	2653	2654	2657	rVB3	825	313	0.02%	0.003%
59	9.596	2657	2661	2664	rVB4	1255	850	0.06%	0.007%
60	9.615	2665	2667	2669	rBV3	488	155	0.01%	0.001%
61	9.712	2695	2697	2699	rVB2	861	330	0.02%	0.003%
62	9.731	2700	2703	2704	rBV3	712	415	0.03%	0.004%
63	9.831	2732	2734	2737	rBV3	743	362	0.02%	0.003%
64	9.992	2782	2784	2786	rBV3	673	352	0.02%	0.003%
65	10.101	2814	2818	2819	rBV3	952	577	0.04%	0.005%
66	10.213	2840	2853	2871	rBV	474803	756173	50.43%	6.464%
67	10.455	2926	2928	2931	rBV4	945	615	0.04%	0.005%
68	10.557	2958	2960	2963	rBV4	1210	700	0.05%	0.006%
69	10.686	2998	3000	3004	rVB3	787	494	0.03%	0.004%
70	10.709	3004	3007	3009	rBV3	606	324	0.02%	0.003%
71	10.776	3024	3028	3030	rBV3	919	552	0.04%	0.005%
72	10.828	3041	3044	3045	rBV2	701	330	0.02%	0.003%
73	10.959	3083	3085	3088	rBV3	731	460	0.03%	0.004%
74	11.024	3103	3105	3107	rVB3	628	190	0.01%	0.002%
75	11.066	3115	3118	3119	rBV	398	246	0.02%	0.002%
76	11.098	3126	3128	3132	rVB3	679	384	0.03%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027976.D
 Acq On : 20 Sep 2022 20:53
 Operator : SY/MD
 Sample : N4619-12
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E29

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.130	3136	3138	3140	rBV	643	375	0.03%	0.003%
78	11.178	3150	3153	3155	rBV	542	298	0.02%	0.003%
79	11.246	3163	3174	3197	rBV	534698	833409	55.58%	7.124%
80	11.458	3238	3240	3241	rBV	397	191	0.01%	0.002%
81	11.493	3250	3251	3253	rBV2	665	251	0.02%	0.002%
82	11.532	3255	3263	3278	rVV4	8182	17329	1.16%	0.148%
83	11.622	3279	3291	3313	rVV	586660	919169	61.30%	7.857%
84	11.850	3360	3362	3366	rVB3	933	546	0.04%	0.005%
85	11.901	3375	3378	3381	rBV2	778	429	0.03%	0.004%
86	12.011	3410	3412	3414	rVB	483	205	0.01%	0.002%
87	12.107	3438	3442	3444	rBV4	533	481	0.03%	0.004%
88	12.120	3444	3446	3451	rVV2	714	499	0.03%	0.004%
89	12.146	3452	3454	3459	rVB2	723	519	0.03%	0.004%
90	12.239	3480	3483	3485	rBV	1095	798	0.05%	0.007%
91	12.709	3627	3629	3631	rVB2	815	256	0.02%	0.002%
92	12.850	3671	3673	3676	rVB3	1128	402	0.03%	0.003%
93	12.901	3688	3689	3693	rVB2	1075	518	0.03%	0.004%
94	12.918	3693	3694	3695	rBV	683	250	0.02%	0.002%
95	13.229	3788	3791	3793	rBV3	1345	718	0.05%	0.006%
96	13.374	3834	3836	3839	rBV4	817	343	0.02%	0.003%
97	13.551	3889	3891	3893	rBV	1185	609	0.04%	0.005%
98	13.879	3991	3993	4000	rBV7	936	936	0.06%	0.008%
99	13.979	4022	4024	4027	rBV3	777	281	0.02%	0.002%
100	14.654	4232	4234	4237	rBV2	1185	515	0.03%	0.004%




Sum of corrected areas: 11699063

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027976.D
Acq On : 20 Sep 2022 20:53
Operator : SY/MD
Sample : N4619-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

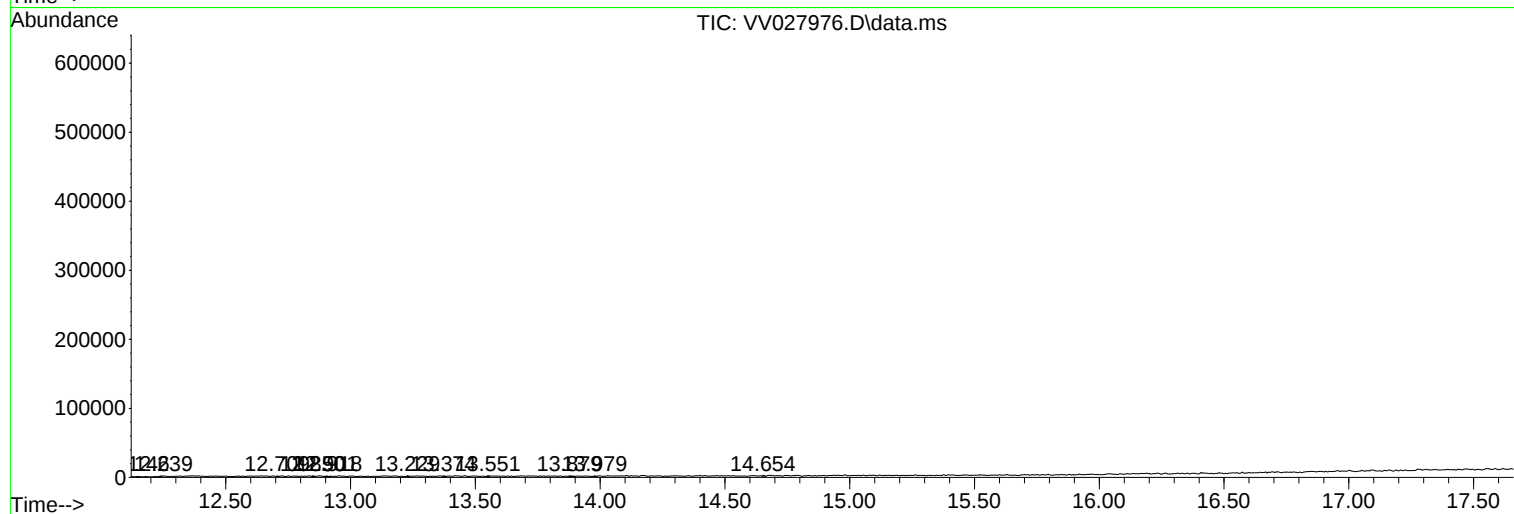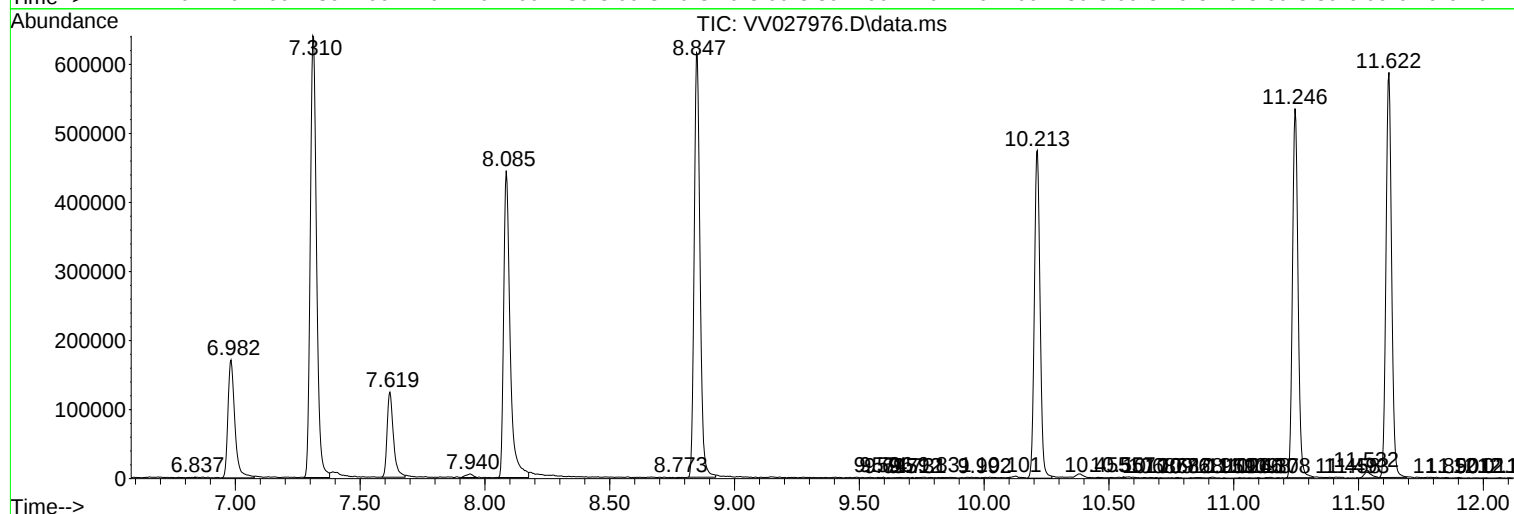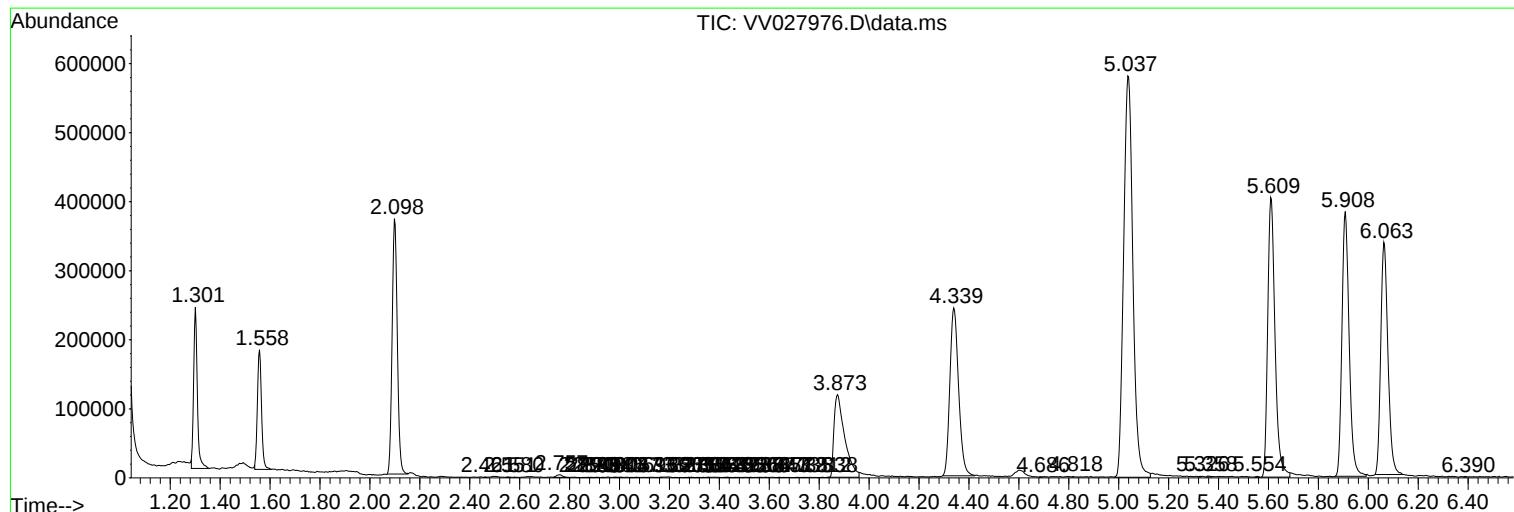

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027976.D
Acq On : 20 Sep 2022 20:53
Operator : SY/MD
Sample : N4619-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027976.D
Acq On : 20 Sep 2022 20:53
Operator : SY/MD
Sample : N4619-12
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 22 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E29

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc