

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027977.D
 Acq On : 20 Sep 2022 21:18
 Operator : SY/MD
 Sample : N4619-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027977.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	217718	227058	16.83%	2.183%
2	1.558	155	161	172	rVB	166613	191829	14.22%	1.844%
3	2.098	320	329	345	rBV	367984	523123	38.77%	5.029%
4	2.394	418	421	423	rBV4	494	319	0.02%	0.003%
5	2.484	446	449	450	rBV2	934	482	0.04%	0.005%
6	2.551	469	470	472	rBV2	399	173	0.01%	0.002%
7	2.664	504	505	508	rBV2	500	249	0.02%	0.002%
8	2.712	516	520	525	rBV2	256	232	0.02%	0.002%
9	2.767	533	537	540	rBV	472	302	0.02%	0.003%
10	2.818	551	553	559	rVB2	648	528	0.04%	0.005%
11	2.844	559	561	564	rBV	368	269	0.02%	0.003%
12	2.953	590	595	596	rBV2	830	686	0.05%	0.007%
13	3.082	632	635	638	rVB3	430	268	0.02%	0.003%
14	3.111	641	644	647	rVV3	340	261	0.02%	0.003%
15	3.127	647	649	655	rVB	414	340	0.03%	0.003%
16	3.156	655	658	661	rBV2	697	420	0.03%	0.004%
17	3.252	684	688	689	rBV2	337	197	0.01%	0.002%
18	3.285	694	698	702	rVB2	200	219	0.02%	0.002%
19	3.313	702	707	709	rBV	457	363	0.03%	0.003%
20	3.349	716	718	721	rVB2	334	189	0.01%	0.002%
21	3.420	737	740	743	rBV2	313	231	0.02%	0.002%
22	3.516	768	770	775	rVB2	450	364	0.03%	0.003%
23	3.539	775	777	781	rBV3	292	209	0.02%	0.002%
24	3.629	800	805	808	rVB2	293	198	0.01%	0.002%
25	3.712	825	831	835	rBV4	371	344	0.03%	0.003%
26	3.748	839	842	844	rBV2	406	206	0.02%	0.002%
27	3.799	854	858	861	rBV2	325	289	0.02%	0.003%
28	3.818	861	864	866	rVB	327	178	0.01%	0.002%
29	3.870	871	880	916	rBV	113891	312279	23.15%	3.002%
30	4.188	978	979	983	rVB3	509	190	0.01%	0.002%
31	4.339	1011	1026	1051	rBV2	221272	546479	40.50%	5.253%
32	4.571	1095	1098	1106	rBV6	1131	1268	0.09%	0.012%
33	4.622	1112	1114	1119	rVB4	462	265	0.02%	0.003%
34	4.677	1127	1131	1137	rVB4	942	810	0.06%	0.008%
35	4.834	1176	1180	1182	rBV3	356	267	0.02%	0.003%
36	4.879	1189	1194	1198	rBV2	689	563	0.04%	0.005%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027977.D
 Acq On : 20 Sep 2022 21:18
 Operator : SY/MD
 Sample : N4619-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.037	1222	1243	1270	rBV2	525050	1349228	100.00%	12.970%
38	5.346	1336	1339	1343	rVB4	680	527	0.04%	0.005%
39	5.365	1343	1345	1346	rBV	520	185	0.01%	0.002%
40	5.420	1356	1362	1364	rBV4	745	724	0.05%	0.007%
41	5.455	1370	1373	1375	rBV3	422	263	0.02%	0.003%
42	5.487	1378	1383	1386	rVB2	744	606	0.04%	0.006%
43	5.526	1393	1395	1398	rBV2	262	180	0.01%	0.002%
44	5.609	1409	1421	1445	rBV	389205	791000	58.63%	7.604%
45	5.860	1498	1499	1504	rBV4	579	377	0.03%	0.004%
46	5.998	1540	1542	1546	rVB2	617	421	0.03%	0.004%
47	6.063	1546	1562	1589	rBV	299126	616991	45.73%	5.931%
48	6.201	1602	1605	1607	rBV3	1311	1049	0.08%	0.010%
49	6.259	1621	1623	1624	rBV2	506	179	0.01%	0.002%
50	6.288	1629	1632	1636	rBV4	700	502	0.04%	0.005%
51	6.371	1655	1658	1661	rBV4	655	431	0.03%	0.004%
52	6.397	1664	1666	1669	rVB3	378	174	0.01%	0.002%
53	6.419	1671	1673	1674	rBV	399	191	0.01%	0.002%
54	6.471	1688	1689	1692	rVB2	553	270	0.02%	0.003%
55	6.497	1692	1697	1698	rBV	455	261	0.02%	0.003%
56	6.509	1698	1701	1703	rBV3	294	202	0.01%	0.002%
57	6.526	1703	1706	1709	rVV3	387	249	0.02%	0.002%
58	6.580	1720	1723	1726	rVB3	521	267	0.02%	0.003%
59	6.606	1729	1731	1733	rBV2	353	202	0.01%	0.002%
60	6.690	1755	1757	1762	rVB4	566	417	0.03%	0.004%
61	6.770	1779	1782	1785	rVB3	492	288	0.02%	0.003%
62	6.789	1786	1788	1790	rBV2	577	226	0.02%	0.002%
63	6.828	1798	1800	1801	rBV	431	188	0.01%	0.002%
64	6.982	1836	1848	1869	rBV	154865	285111	21.13%	2.741%
65	7.310	1938	1950	1970	rBV	579905	1022248	75.77%	9.827%
66	7.542	2018	2022	2025	rBV4	695	740	0.05%	0.007%
67	7.619	2036	2046	2066	rBV	112169	199965	14.82%	1.922%
68	8.085	2181	2191	2222	rBV	435919	787986	58.40%	7.575%
69	8.747	2395	2397	2399	rBV2	824	405	0.03%	0.004%
70	8.850	2418	2429	2454	rBV	611075	1002664	74.31%	9.638%
71	9.297	2566	2568	2570	rBV2	791	400	0.03%	0.004%
72	9.477	2621	2624	2626	rBV4	1174	685	0.05%	0.007%
73	9.734	2701	2704	2707	rBV4	717	471	0.03%	0.005%
74	9.754	2708	2710	2714	rVV3	881	500	0.04%	0.005%
75	9.844	2736	2738	2741	rBV3	540	242	0.02%	0.002%
76	9.950	2769	2771	2774	rBV2	596	375	0.03%	0.004%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027977.D
 Acq On : 20 Sep 2022 21:18
 Operator : SY/MD
 Sample : N4619-13
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 23 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E31

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.992	2782	2784	2786	rBV3	720	426	0.03%	0.004%
78	10.066	2804	2807	2809	rBV3	824	566	0.04%	0.005%
79	10.214	2841	2853	2876	rBV	461455	730412	54.14%	7.021%
80	10.519	2946	2948	2950	rBV2	637	379	0.03%	0.004%
81	10.664	2988	2993	2997	rBV3	876	851	0.06%	0.008%
82	10.773	3024	3027	3028	rBV4	963	499	0.04%	0.005%
83	10.905	3064	3068	3069	rBV2	1316	929	0.07%	0.009%
84	10.988	3092	3094	3095	rBV	600	254	0.02%	0.002%
85	11.098	3125	3128	3131	rVB4	997	634	0.05%	0.006%
86	11.246	3163	3174	3197	rBV	561118	859029	63.67%	8.258%
87	11.532	3256	3263	3274	rBV4	7725	14736	1.09%	0.142%
88	11.622	3280	3291	3310	rBV	584268	909745	67.43%	8.745%
89	12.085	3430	3435	3436	rBV3	1203	1064	0.08%	0.010%
90	12.422	3539	3540	3542	rBV	597	247	0.02%	0.002%
91	12.747	3637	3641	3642	rBV2	887	560	0.04%	0.005%
92	12.824	3663	3665	3672	rVB4	755	580	0.04%	0.006%
93	12.857	3673	3675	3677	rBV2	682	236	0.02%	0.002%
94	12.905	3688	3690	3692	rBV	791	306	0.02%	0.003%
95	12.947	3701	3703	3705	rBV2	824	318	0.02%	0.003%
96	12.975	3710	3712	3713	rBV	451	231	0.02%	0.002%
97	12.985	3713	3715	3721	rVB3	998	687	0.05%	0.007%
98	13.201	3778	3782	3785	rBV2	576	389	0.03%	0.004%
99	13.242	3792	3795	3799	rBV4	736	543	0.04%	0.005%
100	13.432	3852	3854	3856	rBV2	607	206	0.02%	0.002%




Sum of corrected areas: 10402864

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027977.D
Acq On : 20 Sep 2022 21:18
Operator : SY/MD
Sample : N4619-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

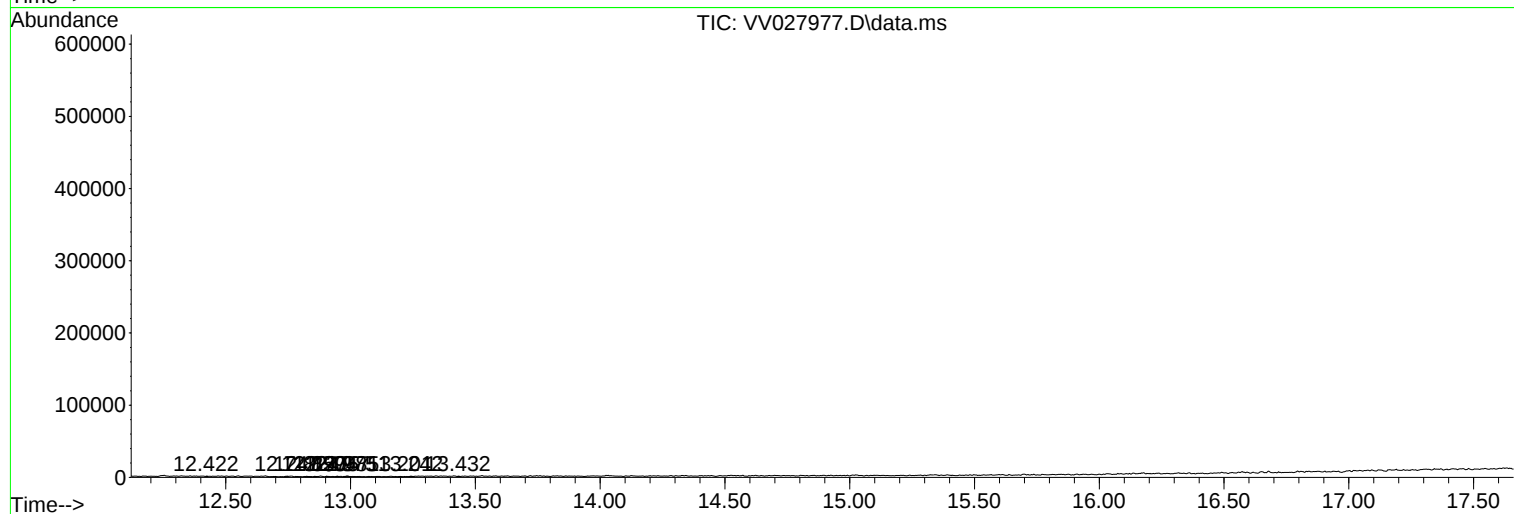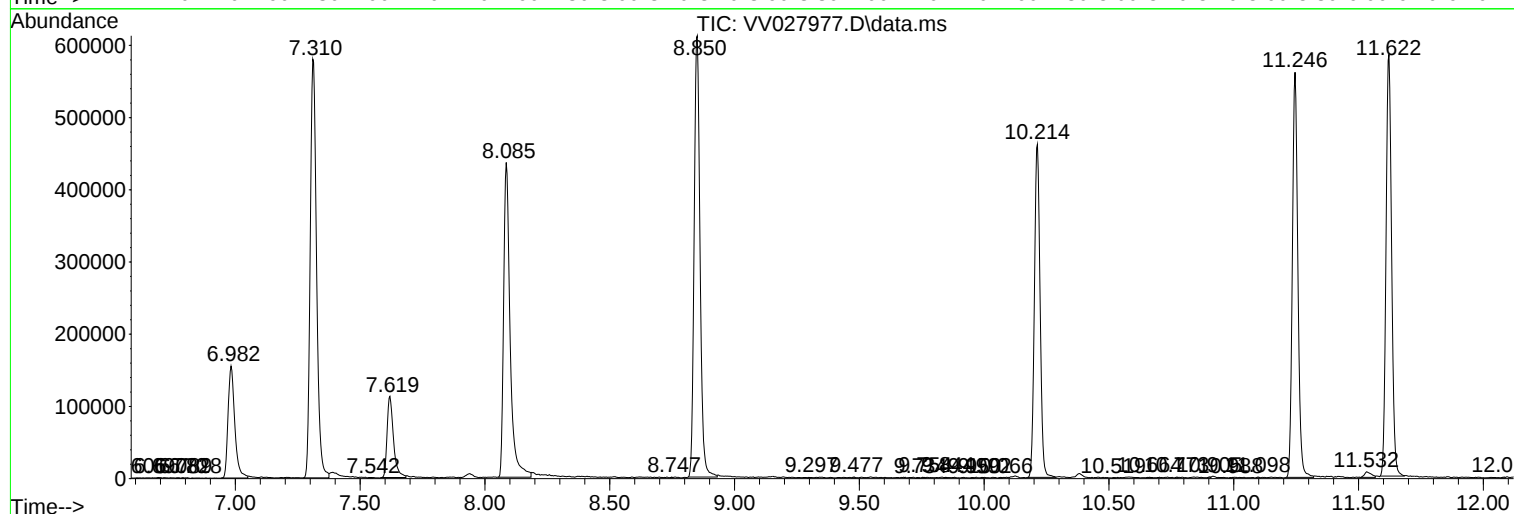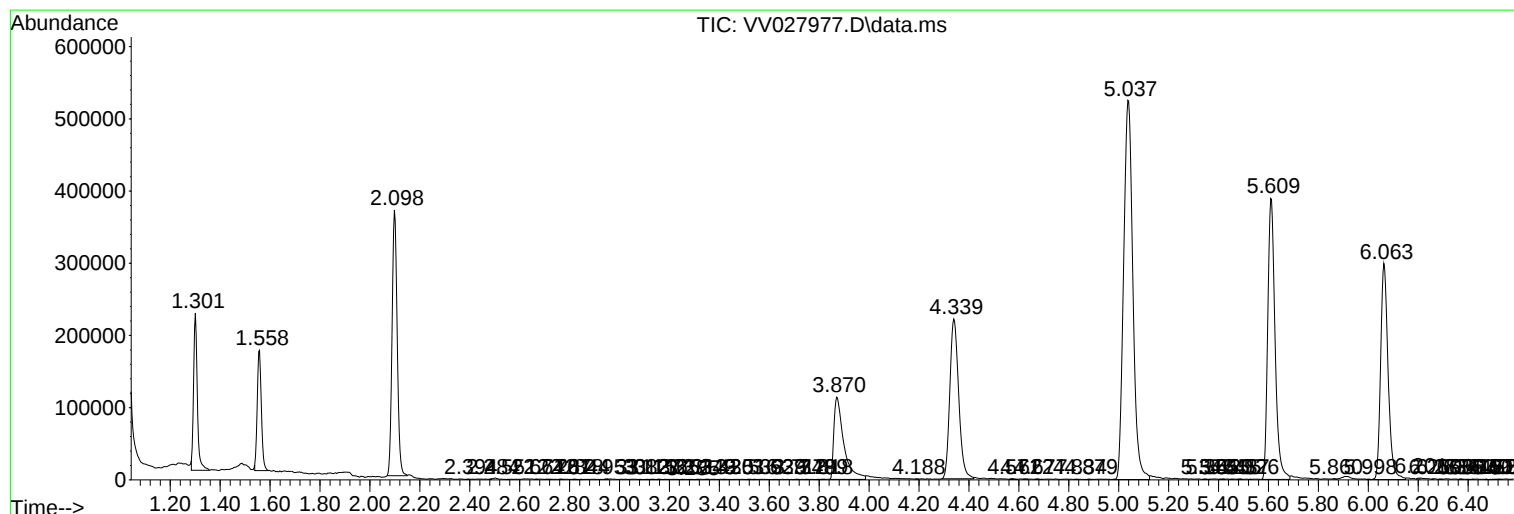

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027977.D
Acq On : 20 Sep 2022 21:18
Operator : SY/MD
Sample : N4619-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027977.D
Acq On : 20 Sep 2022 21:18
Operator : SY/MD
Sample : N4619-13
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 23 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E31

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc