

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027978.D
 Acq On : 20 Sep 2022 21:43
 Operator : SY/MD
 Sample : N4619-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027978.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	102	rVB	219928	235872	15.96%	2.191%
2	1.555	155	160	185	rVB	181576	214872	14.54%	1.996%
3	2.098	319	329	345	rBV	362539	523967	35.45%	4.867%
4	2.272	379	383	385	rVB3	662	512	0.03%	0.005%
5	2.352	405	408	413	rVB3	1039	831	0.06%	0.008%
6	2.381	413	417	420	rBV4	339	284	0.02%	0.003%
7	2.400	420	423	425	rBV	622	395	0.03%	0.004%
8	2.497	445	453	463	rVB7	2336	3702	0.25%	0.034%
9	2.574	473	477	480	rBV3	568	444	0.03%	0.004%
10	2.606	484	487	490	rBV2	418	293	0.02%	0.003%
11	2.622	490	492	494	rBV2	682	383	0.03%	0.004%
12	2.738	525	528	531	rBV3	358	346	0.02%	0.003%
13	2.761	531	535	538	rVV3	751	554	0.04%	0.005%
14	2.924	583	586	590	rBV3	425	314	0.02%	0.003%
15	2.944	590	592	593	rBV2	879	504	0.03%	0.005%
16	3.027	616	618	621	rBV2	381	258	0.02%	0.002%
17	3.056	626	627	631	rVB3	495	247	0.02%	0.002%
18	3.088	634	637	642	rBV3	580	497	0.03%	0.005%
19	3.207	671	674	677	rVB3	551	386	0.03%	0.004%
20	3.227	677	680	682	rBV3	448	285	0.02%	0.003%
21	3.272	690	694	695	rBV2	563	355	0.02%	0.003%
22	3.346	714	717	719	rBV3	1052	801	0.05%	0.007%
23	3.436	742	745	749	rVB5	1014	621	0.04%	0.006%
24	3.571	782	787	789	rBV2	885	695	0.05%	0.006%
25	3.622	801	803	806	rBV2	678	473	0.03%	0.004%
26	3.732	834	837	839	rBV	520	281	0.02%	0.003%
27	3.799	856	858	862	rVB3	607	390	0.03%	0.004%
28	3.873	872	881	910	rBV	127671	349377	23.64%	3.245%
29	4.339	1011	1026	1052	rBV	244071	600973	40.66%	5.582%
30	4.654	1122	1124	1129	rBV3	656	552	0.04%	0.005%
31	4.712	1137	1142	1143	rBV3	922	768	0.05%	0.007%
32	4.757	1154	1156	1159	rBV4	572	372	0.03%	0.003%
33	4.805	1168	1171	1174	rBV4	551	355	0.02%	0.003%
34	4.828	1174	1178	1181	rVB4	717	581	0.04%	0.005%
35	4.969	1218	1222	1225	rBV5	640	492	0.03%	0.005%
36	5.037	1226	1243	1272	rBV2	576242	1478125	100.00%	13.730%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027978.D
 Acq On : 20 Sep 2022 21:43
 Operator : SY/MD
 Sample : N4619-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.413	1358	1360	1363	rBV2	947	319	0.02%	0.003%
38	5.465	1374	1376	1378	rBV2	713	340	0.02%	0.003%
39	5.513	1388	1391	1392	rBV3	623	384	0.03%	0.004%
40	5.609	1410	1421	1455	rBV	398857	814473	55.10%	7.565%
41	5.998	1537	1542	1544	rBV4	901	750	0.05%	0.007%
42	6.063	1549	1562	1591	rVV	329364	681327	46.09%	6.328%
43	6.387	1661	1663	1665	rBV2	678	312	0.02%	0.003%
44	6.442	1678	1680	1681	rBV2	651	252	0.02%	0.002%
45	6.567	1717	1719	1721	rBV4	895	426	0.03%	0.004%
46	6.622	1734	1736	1739	rBB3	489	254	0.02%	0.002%
47	6.821	1796	1798	1802	rBV3	564	404	0.03%	0.004%
48	6.854	1802	1808	1811	rVB7	851	973	0.07%	0.009%
49	6.883	1815	1817	1820	rBV	568	268	0.02%	0.002%
50	6.924	1828	1830	1833	rBV	523	342	0.02%	0.003%
51	6.944	1833	1836	1837	rBV	745	366	0.02%	0.003%
52	6.982	1837	1848	1868	rBV	159566	292308	19.78%	2.715%
53	7.310	1936	1950	1972	rBV	608995	1086735	73.52%	10.094%
54	7.619	2036	2046	2068	rBV	120934	214733	14.53%	1.995%
55	7.825	2108	2110	2113	rVB3	1248	558	0.04%	0.005%
56	7.844	2113	2116	2118	rBV4	1034	758	0.05%	0.007%
57	8.085	2180	2191	2216	rBV	443863	807928	54.66%	7.504%
58	8.632	2358	2361	2363	rBV2	1099	723	0.05%	0.007%
59	8.725	2388	2390	2394	rBV3	956	554	0.04%	0.005%
60	8.847	2416	2428	2459	rBV	602227	995035	67.32%	9.242%
61	9.214	2539	2542	2544	rBV3	1049	686	0.05%	0.006%
62	9.284	2562	2564	2566	rBV2	860	328	0.02%	0.003%
63	9.362	2586	2588	2590	rBV3	742	305	0.02%	0.003%
64	9.529	2636	2640	2643	rBV4	1123	916	0.06%	0.009%
65	9.616	2665	2667	2670	rBV2	968	619	0.04%	0.006%
66	9.738	2703	2705	2707	rBV2	577	301	0.02%	0.003%
67	9.879	2746	2749	2753	rVB5	801	590	0.04%	0.005%
68	9.902	2753	2756	2758	rVB3	613	363	0.02%	0.003%
69	9.921	2758	2762	2764	rBV3	1389	929	0.06%	0.009%
70	10.017	2790	2792	2795	rBV3	642	370	0.03%	0.003%
71	10.091	2814	2815	2818	rBV2	847	459	0.03%	0.004%
72	10.214	2841	2853	2876	rBV	453262	715671	48.42%	6.647%
73	10.378	2894	2904	2918	rVB2	5227	9773	0.66%	0.091%
74	10.471	2931	2933	2937	rVB4	800	386	0.03%	0.004%
75	10.506	2942	2944	2947	rVB2	563	329	0.02%	0.003%
76	10.542	2952	2955	2956	rBV2	735	320	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027978.D
 Acq On : 20 Sep 2022 21:43
 Operator : SY/MD
 Sample : N4619-14
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E32

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.632	2979	2983	2986	rBV2	474	397	0.03%	0.004%
78	10.699	2999	3004	3007	rBV2	401	335	0.02%	0.003%
79	10.725	3009	3012	3016	rVV4	475	320	0.02%	0.003%
80	10.757	3020	3022	3027	rVB3	559	360	0.02%	0.003%
81	10.860	3051	3054	3056	rBV2	708	367	0.02%	0.003%
82	10.911	3064	3070	3077	rBV6	1280	2052	0.14%	0.019%
83	10.969	3086	3088	3092	rBV2	355	289	0.02%	0.003%
84	10.998	3092	3097	3099	rVV3	502	458	0.03%	0.004%
85	11.027	3102	3106	3109	rBV3	596	479	0.03%	0.004%
86	11.140	3135	3141	3144	rBV4	950	981	0.07%	0.009%
87	11.246	3163	3174	3193	rBV	519371	804485	54.43%	7.472%
88	11.532	3251	3263	3274	rBV4	8466	17577	1.19%	0.163%
89	11.622	3280	3291	3309	rBV	567234	880442	59.56%	8.178%
90	11.841	3356	3359	3365	rVB4	759	542	0.04%	0.005%
91	11.863	3365	3366	3368	rBV2	547	238	0.02%	0.002%
92	11.956	3391	3395	3397	rBV4	530	502	0.03%	0.005%
93	11.998	3404	3408	3409	rBV2	505	276	0.02%	0.003%
94	12.037	3418	3420	3423	rVB2	1029	442	0.03%	0.004%
95	12.111	3439	3443	3445	rVV2	415	292	0.02%	0.003%
96	12.146	3452	3454	3457	rVB3	561	264	0.02%	0.002%
97	12.159	3457	3458	3461	rBV	567	252	0.02%	0.002%
98	12.210	3471	3474	3476	rBV	498	361	0.02%	0.003%
99	13.799	3965	3968	3970	rBV3	1053	509	0.03%	0.005%
100	13.837	3976	3980	3983	rBV3	1040	791	0.05%	0.007%




Sum of corrected areas: 10766035

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027978.D
Acq On : 20 Sep 2022 21:43
Operator : SY/MD
Sample : N4619-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

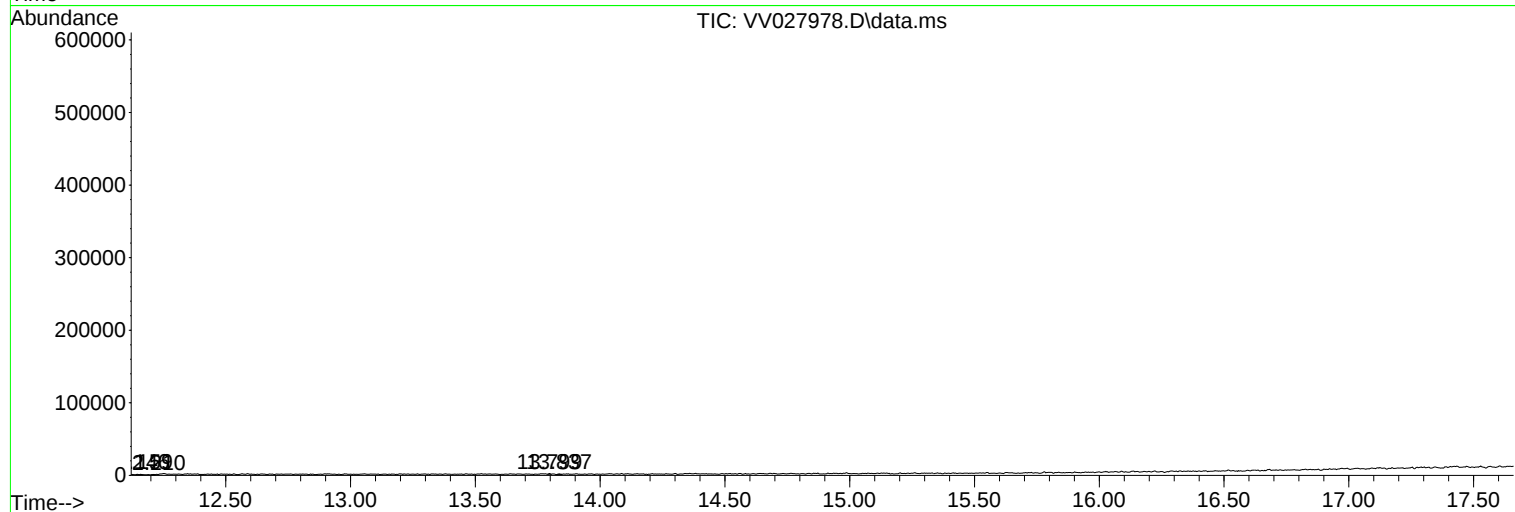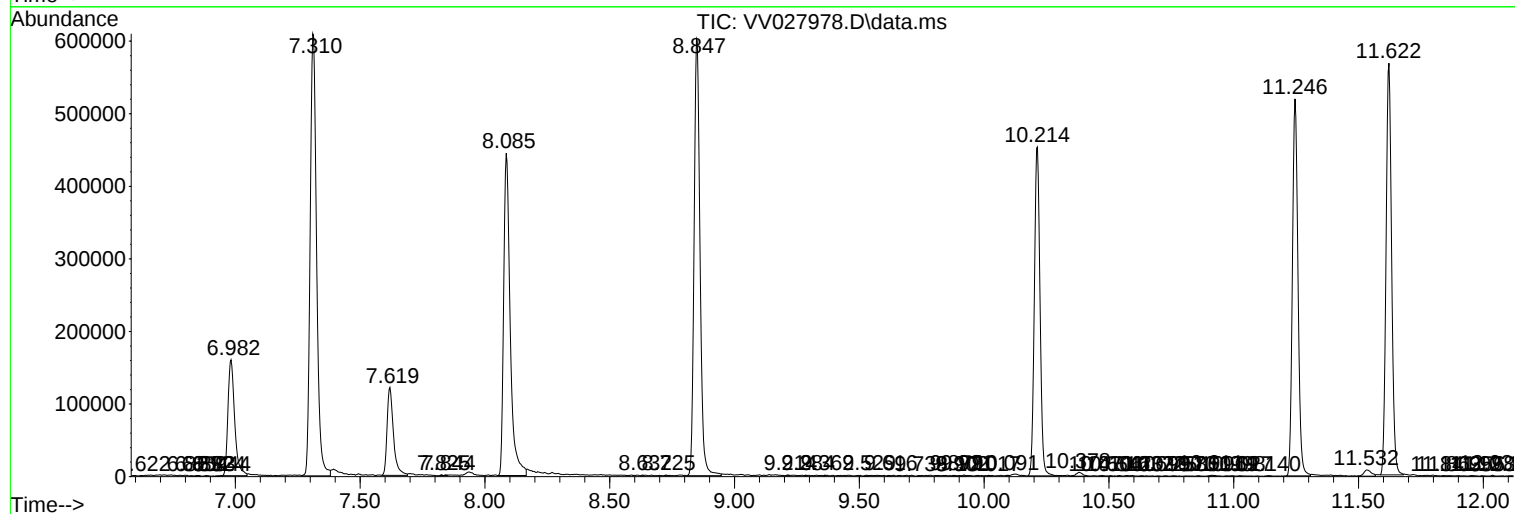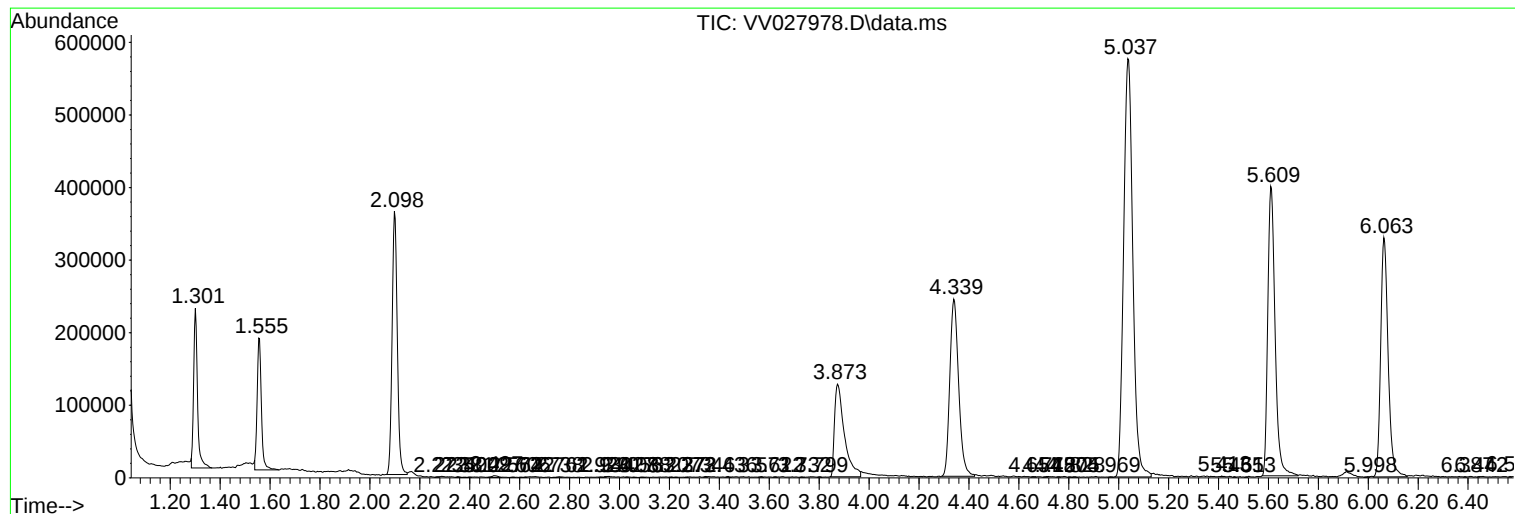

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027978.D
Acq On : 20 Sep 2022 21:43
Operator : SY/MD
Sample : N4619-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027978.D
Acq On : 20 Sep 2022 21:43
Operator : SY/MD
Sample : N4619-14
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 24 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E32

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc
