

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027980.D
 Acq On : 20 Sep 2022 22:32
 Operator : SY/MD
 Sample : N4619-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027980.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	101	rVB	225609	240616	16.91%	2.196%
2	1.558	155	161	176	rVB	180297	206206	14.49%	1.882%
3	2.098	320	329	344	rBV	374995	541288	38.03%	4.940%
4	2.265	379	381	383	rBV2	647	364	0.03%	0.003%
5	2.413	424	427	428	rBV2	395	225	0.02%	0.002%
6	2.545	467	468	469	rBV	191	54	0.00%	0.000%
7	2.564	469	474	477	rVV3	536	445	0.03%	0.004%
8	2.577	477	478	481	rVV2	268	126	0.01%	0.001%
9	2.629	491	494	495	rBV2	796	488	0.03%	0.004%
10	2.725	521	524	526	rBV2	603	395	0.03%	0.004%
11	2.744	528	530	532	rBV3	213	100	0.01%	0.001%
12	2.793	543	545	548	rBV	399	213	0.01%	0.002%
13	2.809	548	550	554	rVB2	491	243	0.02%	0.002%
14	2.831	554	557	560	rBV2	427	289	0.02%	0.003%
15	2.873	568	570	573	rBV2	220	164	0.01%	0.001%
16	2.908	578	581	582	rBV	318	156	0.01%	0.001%
17	2.931	585	588	590	rBV2	429	313	0.02%	0.003%
18	2.973	599	601	602	rBV	174	82	0.01%	0.001%
19	2.982	602	604	606	rVB2	436	147	0.01%	0.001%
20	3.005	606	611	617	rVB2	524	625	0.04%	0.006%
21	3.037	617	621	624	rBV3	683	659	0.05%	0.006%
22	3.053	624	626	628	rVV	309	134	0.01%	0.001%
23	3.063	628	629	634	rVB3	392	305	0.02%	0.003%
24	3.101	638	641	642	rBV	504	205	0.01%	0.002%
25	3.191	668	669	670	rBV	266	63	0.00%	0.001%
26	3.201	670	672	676	rVB2	533	285	0.02%	0.003%
27	3.233	680	682	683	rVB	157	47	0.00%	0.000%
28	3.243	683	685	688	rBV	196	118	0.01%	0.001%
29	3.259	688	690	694	rBV3	399	352	0.02%	0.003%
30	3.323	705	710	714	rBV4	536	532	0.04%	0.005%
31	3.368	720	724	726	rVB3	478	329	0.02%	0.003%
32	3.391	726	731	732	rBV3	451	308	0.02%	0.003%
33	3.416	737	739	743	rVB2	526	282	0.02%	0.003%
34	3.442	743	747	748	rBV2	329	218	0.02%	0.002%
35	3.468	754	755	757	rBV2	128	33	0.00%	0.000%
36	3.481	757	759	760	rVB2	157	36	0.00%	0.000%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027980.D
 Acq On : 20 Sep 2022 22:32
 Operator : SY/MD
 Sample : N4619-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.490	760	762	763	rBV2	321	154	0.01%	0.001%
38	3.523	768	772	778	rVB4	362	370	0.03%	0.003%
39	3.564	782	785	787	rBV	355	205	0.01%	0.002%
40	3.580	787	790	791	rVB2	519	223	0.02%	0.002%
41	3.590	791	793	794	rBV	192	78	0.01%	0.001%
42	3.613	798	800	801	rVB2	142	38	0.00%	0.000%
43	3.632	801	806	807	rBV2	439	388	0.03%	0.004%
44	3.667	815	817	818	rBV2	253	127	0.01%	0.001%
45	3.712	829	831	835	rVB2	209	115	0.01%	0.001%
46	3.732	835	837	838	rBV	213	94	0.01%	0.001%
47	3.789	852	855	858	rBV2	451	315	0.02%	0.003%
48	3.809	858	861	864	rVV3	305	229	0.02%	0.002%
49	3.873	872	881	915	rBV	119805	328822	23.10%	3.001%
50	4.339	1011	1026	1051	rBV	229243	560902	39.41%	5.119%
51	4.635	1115	1118	1120	rBV3	503	299	0.02%	0.003%
52	4.654	1123	1124	1125	rBV3	216	44	0.00%	0.000%
53	4.664	1125	1127	1129	rBV2	586	243	0.02%	0.002%
54	4.754	1153	1155	1157	rBV2	598	297	0.02%	0.003%
55	4.822	1174	1176	1179	rBV2	403	203	0.01%	0.002%
56	4.857	1183	1187	1189	rBV2	483	354	0.02%	0.003%
57	4.889	1193	1197	1199	rBV	480	344	0.02%	0.003%
58	4.915	1202	1205	1206	rBV2	222	141	0.01%	0.001%
59	4.969	1221	1222	1223	rBV	476	139	0.01%	0.001%
60	5.040	1227	1244	1274	rBV2	551820	1423214	100.00%	12.989%
61	5.609	1410	1421	1442	rBV	409860	835907	58.73%	7.629%
62	6.063	1549	1562	1584	rBV	334305	692436	48.65%	6.320%
63	6.612	1731	1733	1735	rBV2	690	389	0.03%	0.004%
64	6.770	1780	1782	1784	rBV2	561	303	0.02%	0.003%
65	6.821	1796	1798	1800	rBV2	799	359	0.03%	0.003%
66	6.918	1826	1828	1829	rBV2	814	359	0.03%	0.003%
67	6.982	1837	1848	1868	rBV	168177	313271	22.01%	2.859%
68	7.310	1939	1950	1970	rBV	628053	1098615	77.19%	10.027%
69	7.619	2035	2046	2068	rBV	123305	222133	15.61%	2.027%
70	8.085	2181	2191	2221	rBV	460081	830679	58.37%	7.581%
71	8.847	2417	2428	2449	rBV	620973	1018813	71.59%	9.299%
72	9.423	2605	2607	2611	rVB2	465	273	0.02%	0.002%
73	9.458	2616	2618	2619	rBV	470	157	0.01%	0.001%
74	9.484	2624	2626	2627	rBV	515	199	0.01%	0.002%
75	9.731	2701	2703	2704	rVB2	300	102	0.01%	0.001%
76	9.751	2704	2709	2711	rBV2	394	334	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027980.D
 Acq On : 20 Sep 2022 22:32
 Operator : SY/MD
 Sample : N4619-16
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E35

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.763	2711	2713	2717	rBV3	511	240	0.02%	0.002%
78	9.780	2717	2718	2721	rBV2	245	97	0.01%	0.001%
79	9.796	2721	2723	2724	rBV2	325	89	0.01%	0.001%
80	9.805	2724	2726	2727	rBV2	712	269	0.02%	0.002%
81	9.911	2757	2759	2763	rBV5	496	397	0.03%	0.004%
82	9.953	2768	2772	2773	rBV2	881	606	0.04%	0.006%
83	9.976	2776	2779	2782	rBV3	614	440	0.03%	0.004%
84	10.124	2817	2825	2830	rBV5	1768	2722	0.19%	0.025%
85	10.214	2841	2853	2879	rBV	489774	769099	54.04%	7.019%
86	10.445	2921	2925	2927	rBV3	807	639	0.04%	0.006%
87	10.779	3027	3029	3032	rBV2	866	488	0.03%	0.004%
88	11.127	3135	3137	3140	rBV2	898	601	0.04%	0.005%
89	11.246	3163	3174	3194	rBV	566538	875947	61.55%	7.995%
90	11.535	3254	3264	3276	rBV6	9749	20720	1.46%	0.189%
91	11.622	3280	3291	3309	rVV	609811	951540	66.86%	8.685%
92	12.178	3462	3464	3466	rBV3	852	441	0.03%	0.004%
93	12.294	3497	3500	3503	rVB3	1439	1009	0.07%	0.009%
94	12.567	3582	3585	3588	rBV4	913	862	0.06%	0.008%
95	12.728	3633	3635	3638	rBV	847	414	0.03%	0.004%
96	13.143	3761	3764	3768	rBV3	945	646	0.05%	0.006%
97	13.394	3840	3842	3844	rVB3	935	375	0.03%	0.003%
98	13.471	3863	3866	3868	rBV	771	550	0.04%	0.005%
99	13.586	3900	3902	3904	rBV3	876	441	0.03%	0.004%




Sum of corrected areas: 10956744

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027980.D
Acq On : 20 Sep 2022 22:32
Operator : SY/MD
Sample : N4619-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

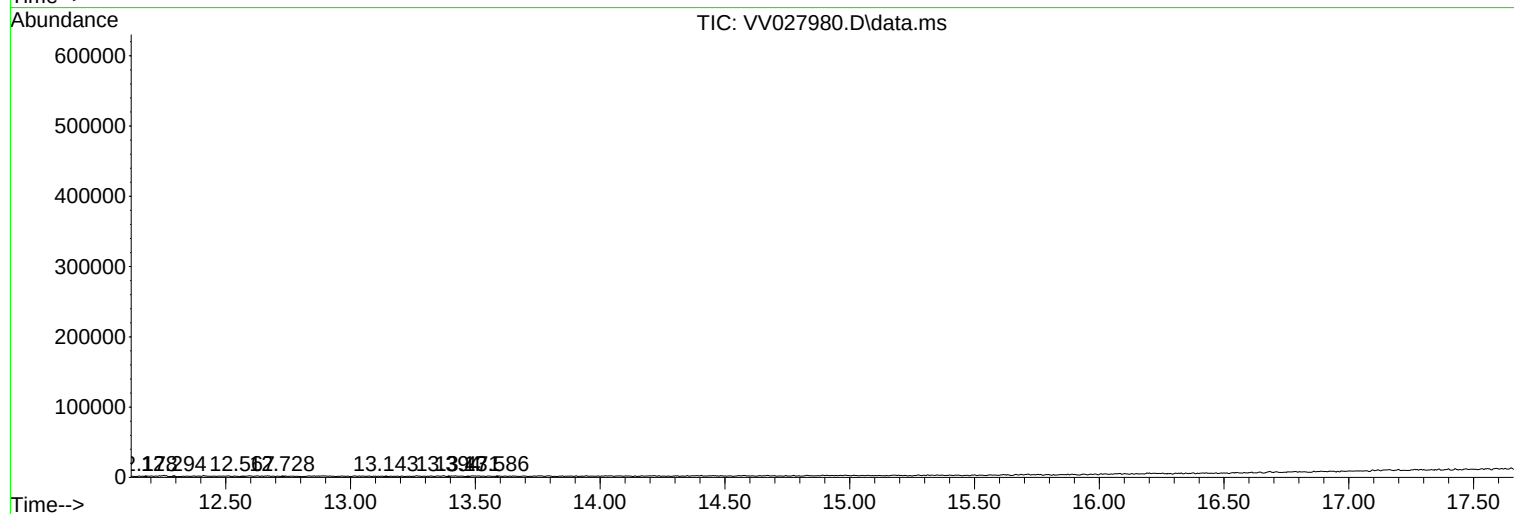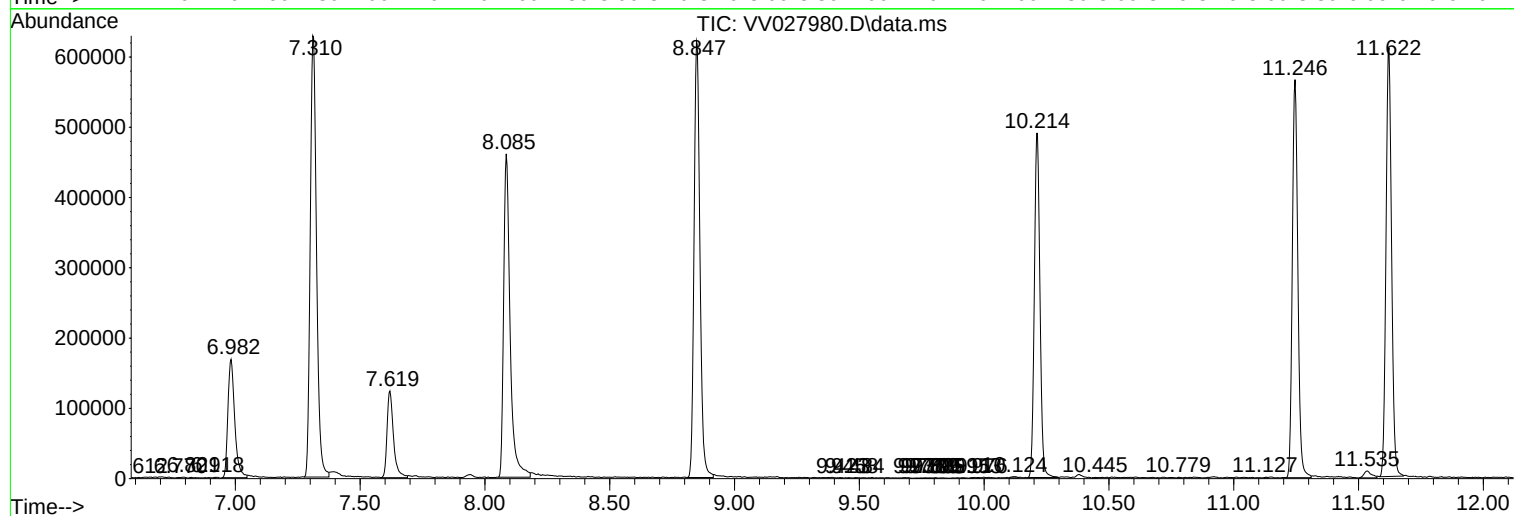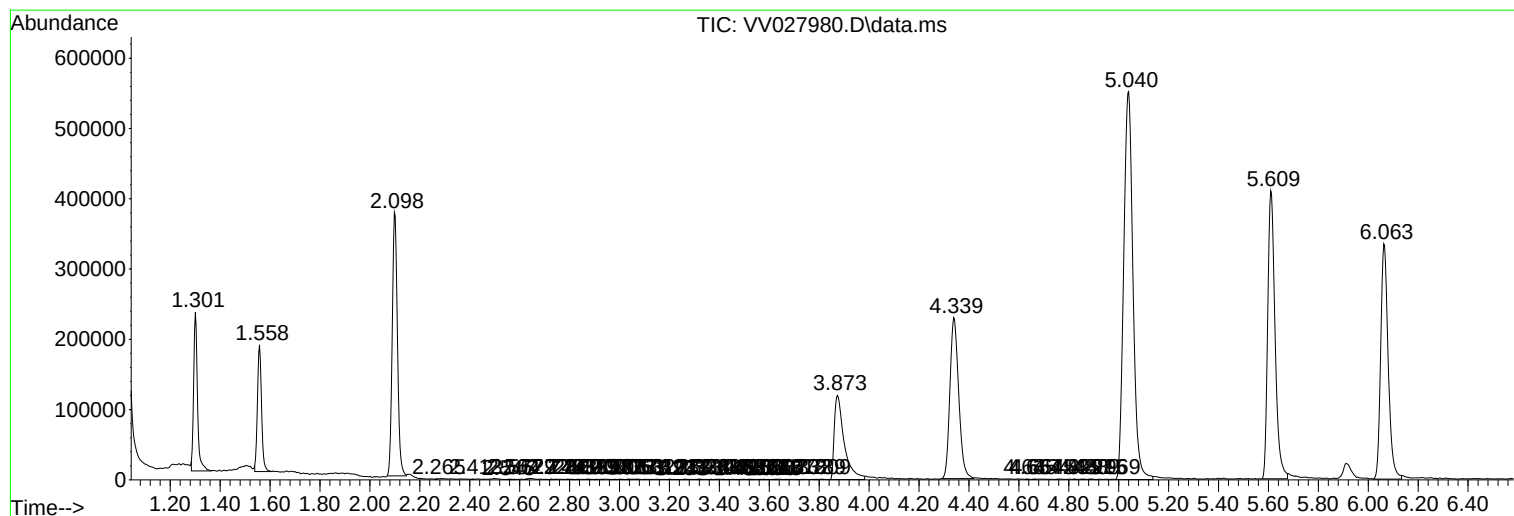

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027980.D
Acq On : 20 Sep 2022 22:32
Operator : SY/MD
Sample : N4619-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027980.D
Acq On : 20 Sep 2022 22:32
Operator : SY/MD
Sample : N4619-16
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 26 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E35

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc