

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027981.D
 Acq On : 20 Sep 2022 22:57
 Operator : SY/MD
 Sample : N4619-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV027981.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	100	rVB	233718	233153	15.51%	2.120%
2	1.555	154	160	175	rVB	168815	198992	13.24%	1.809%
3	2.098	319	329	342	rBV	377499	546876	36.38%	4.972%
4	2.388	416	419	420	rBV2	469	304	0.02%	0.003%
5	2.503	449	455	460	rBV5	1403	1807	0.12%	0.016%
6	2.674	506	508	510	rVB	169	37	0.00%	0.000%
7	2.719	520	522	528	rVB2	334	259	0.02%	0.002%
8	2.751	528	532	535	rBV3	455	464	0.03%	0.004%
9	2.805	547	549	550	rBV	259	86	0.01%	0.001%
10	2.838	557	559	561	rBV	301	189	0.01%	0.002%
11	2.924	583	586	587	rBV	298	123	0.01%	0.001%
12	2.950	589	594	605	rVB5	1216	2026	0.13%	0.018%
13	3.002	607	610	614	rVB2	345	247	0.02%	0.002%
14	3.031	618	619	620	rBV2	264	82	0.01%	0.001%
15	3.095	636	639	643	rBV2	321	193	0.01%	0.002%
16	3.117	643	646	647	rBV	429	221	0.01%	0.002%
17	3.130	647	650	653	rVB2	298	212	0.01%	0.002%
18	3.150	653	656	659	rBV2	298	171	0.01%	0.002%
19	3.195	668	670	672	rBV	235	115	0.01%	0.001%
20	3.220	674	678	682	rVV2	304	252	0.02%	0.002%
21	3.249	685	687	689	rVB	239	97	0.01%	0.001%
22	3.265	690	692	693	rBV	204	71	0.00%	0.001%
23	3.307	703	705	707	rBV	313	151	0.01%	0.001%
24	3.336	711	714	715	rBV	122	53	0.00%	0.000%
25	3.359	719	721	722	rVB2	334	78	0.01%	0.001%
26	3.368	722	724	726	rBV	182	104	0.01%	0.001%
27	3.381	726	728	730	rVV2	231	102	0.01%	0.001%
28	3.407	734	736	743	rVB2	373	328	0.02%	0.003%
29	3.442	743	747	751	rBV	497	308	0.02%	0.003%
30	3.465	751	754	758	rVB	196	119	0.01%	0.001%
31	3.500	758	765	770	rVB2	395	483	0.03%	0.004%
32	3.529	770	774	776	rBV2	429	365	0.02%	0.003%
33	3.568	784	786	787	rBV2	152	53	0.00%	0.000%
34	3.580	787	790	795	rVB2	457	323	0.02%	0.003%
35	3.638	806	808	810	rBV	172	91	0.01%	0.001%
36	3.651	810	812	813	rBV	318	121	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027981.D
 Acq On : 20 Sep 2022 22:57
 Operator : SY/MD
 Sample : N4619-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.696	822	826	827	rBV	373	207	0.01%	0.002%
38	3.764	844	847	852	rBV2	424	340	0.02%	0.003%
39	3.805	859	860	861	rBV	222	53	0.00%	0.000%
40	3.815	861	863	866	rVB2	352	176	0.01%	0.002%
41	3.867	870	879	916	rBV	114183	310841	20.68%	2.826%
42	4.339	1008	1026	1051	rBV	232791	573263	38.13%	5.212%
43	4.558	1091	1094	1099	rBV5	684	488	0.03%	0.004%
44	4.619	1109	1113	1117	rBV6	969	962	0.06%	0.009%
45	4.883	1193	1195	1198	rBV	612	422	0.03%	0.004%
46	5.037	1227	1243	1270	rBV2	584501	1503402	100.00%	13.669%
47	5.365	1343	1345	1350	rBV4	1003	698	0.05%	0.006%
48	5.609	1409	1421	1446	rBV	405112	827225	55.02%	7.521%
49	6.063	1549	1562	1596	rBV	339083	697477	46.39%	6.342%
50	6.529	1700	1707	1710	rBV5	1544	1724	0.11%	0.016%
51	6.567	1715	1719	1721	rBV3	1049	831	0.06%	0.008%
52	6.645	1736	1743	1749	rBV6	1999	2783	0.19%	0.025%
53	6.982	1837	1848	1875	rBV	163904	313876	20.88%	2.854%
54	7.268	1935	1937	1938	rBV2	1102	445	0.03%	0.004%
55	7.310	1939	1950	1971	rVV	638799	1112730	74.01%	10.117%
56	7.616	2035	2045	2065	rBV	120753	217278	14.45%	1.976%
57	7.770	2090	2093	2096	rBV3	1333	892	0.06%	0.008%
58	8.085	2181	2191	2216	rBV	441012	780004	51.88%	7.092%
59	8.702	2381	2383	2385	rBV2	684	453	0.03%	0.004%
60	8.847	2418	2428	2453	rBV	620837	1013676	67.43%	9.217%
61	9.525	2636	2639	2641	rBV3	769	553	0.04%	0.005%
62	9.628	2668	2671	2673	rBV3	559	404	0.03%	0.004%
63	9.696	2690	2692	2694	rBV2	900	407	0.03%	0.004%
64	9.738	2701	2705	2709	rBV5	494	496	0.03%	0.005%
65	9.757	2709	2711	2714	rVB2	643	308	0.02%	0.003%
66	9.773	2714	2716	2717	rBV2	575	272	0.02%	0.002%
67	9.844	2735	2738	2740	rBV2	593	336	0.02%	0.003%
68	9.905	2755	2757	2760	rBV2	620	362	0.02%	0.003%
69	9.931	2760	2765	2767	rBV2	575	497	0.03%	0.005%
70	9.943	2767	2769	2772	rVV3	1013	519	0.03%	0.005%
71	9.972	2776	2778	2780	rBV2	574	239	0.02%	0.002%
72	10.124	2821	2825	2831	rVB4	1511	1689	0.11%	0.015%
73	10.210	2839	2852	2875	rBV	461428	736459	48.99%	6.696%
74	10.423	2915	2918	2920	rBV3	357	198	0.01%	0.002%
75	10.477	2931	2935	2938	rBV3	692	521	0.03%	0.005%
76	10.535	2952	2953	2954	rBV	450	167	0.01%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027981.D
 Acq On : 20 Sep 2022 22:57
 Operator : SY/MD
 Sample : N4619-17
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E37

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.632	2981	2983	2986	rBV	849	504	0.03%	0.005%
78	10.660	2991	2992	2993	rBV	264	96	0.01%	0.001%
79	10.722	3009	3011	3014	rVB3	878	391	0.03%	0.004%
80	11.011	3099	3101	3105	rVB4	1120	595	0.04%	0.005%
81	11.037	3106	3109	3110	rBV2	862	399	0.03%	0.004%
82	11.104	3127	3130	3133	rBV4	1295	848	0.06%	0.008%
83	11.140	3137	3141	3143	rBV4	769	511	0.03%	0.005%
84	11.246	3163	3174	3194	rBV	568536	890567	59.24%	8.097%
85	11.535	3256	3264	3275	rBV3	12027	22916	1.52%	0.208%
86	11.622	3280	3291	3311	rVV	639684	984854	65.51%	8.955%
87	12.554	3577	3581	3583	rBV3	899	684	0.05%	0.006%
88	12.680	3618	3620	3623	rBV2	668	446	0.03%	0.004%
89	12.815	3658	3662	3663	rBV3	733	424	0.03%	0.004%
90	13.667	3924	3927	3934	rVB5	1056	1256	0.08%	0.011%
91	14.985	4335	4337	4344	rVB6	2047	1478	0.10%	0.013%




Sum of corrected areas: 10998298

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027981.D
Acq On : 20 Sep 2022 22:57
Operator : SY/MD
Sample : N4619-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

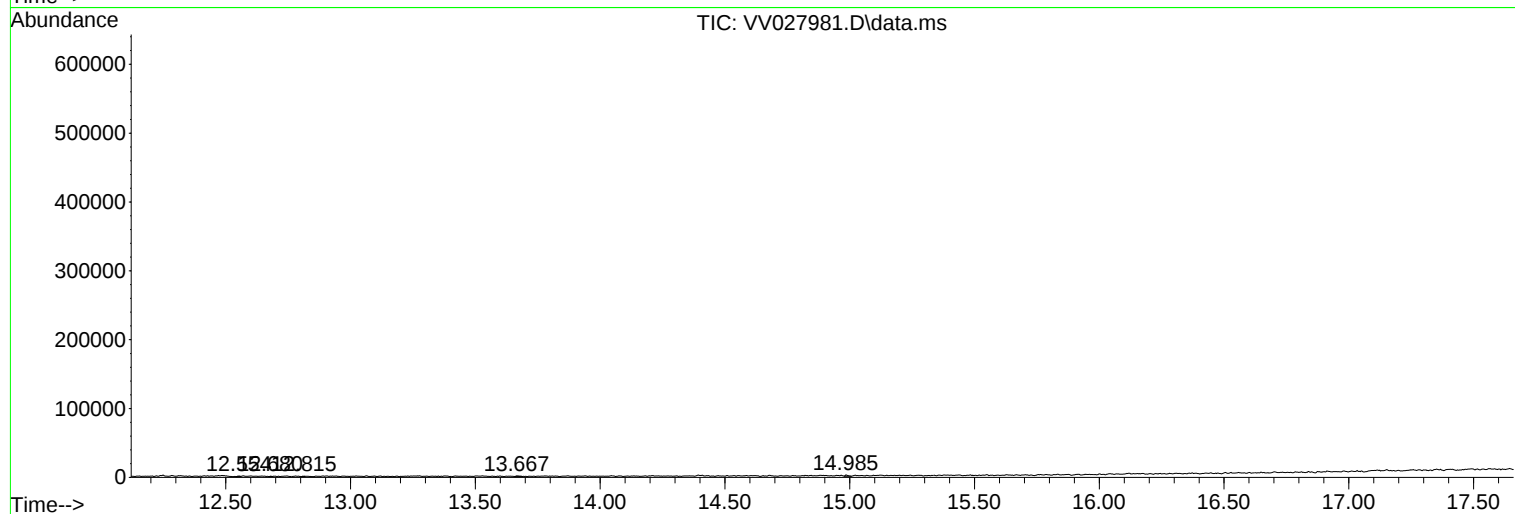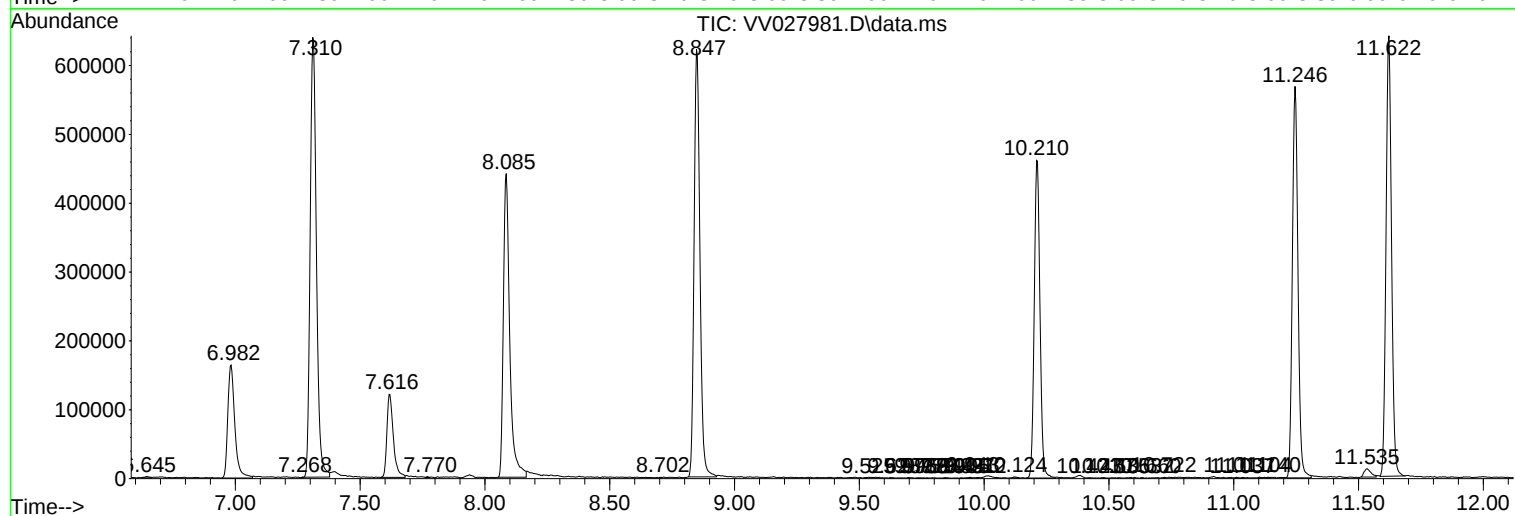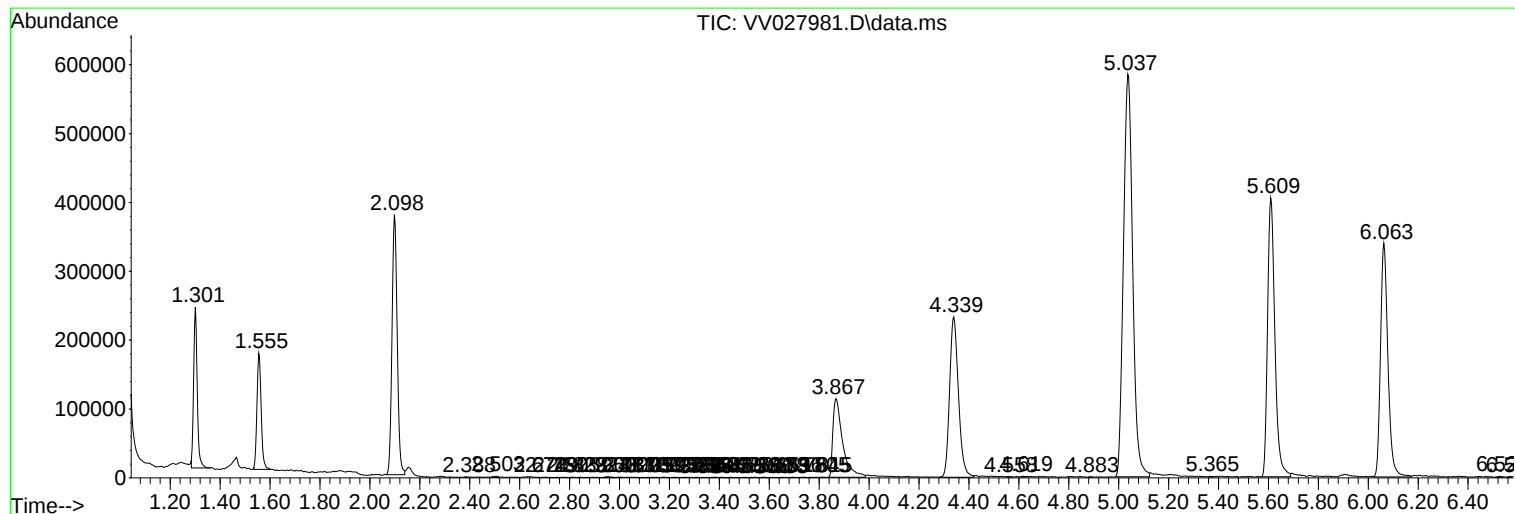

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027981.D
Acq On : 20 Sep 2022 22:57
Operator : SY/MD
Sample : N4619-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027981.D
Acq On : 20 Sep 2022 22:57
Operator : SY/MD
Sample : N4619-17
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E37

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------