

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027983.D
 Acq On : 20 Sep 2022 23:46
 Operator : SY/MD
 Sample : N4620-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027983.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	103	rVB	247467	256334	17.85%	2.272%
2	1.558	155	161	177	rVB	195354	223888	15.59%	1.984%
3	2.101	320	330	349	rBV2	437303	666255	46.39%	5.906%
4	2.320	396	398	401	rBV3	628	272	0.02%	0.002%
5	2.349	405	407	410	rBV	668	289	0.02%	0.003%
6	2.420	427	429	432	rBV	520	322	0.02%	0.003%
7	2.484	446	449	451	rBV3	1185	728	0.05%	0.006%
8	2.580	475	479	480	rBV2	311	202	0.01%	0.002%
9	2.613	487	489	490	rBV	469	161	0.01%	0.001%
10	2.699	513	516	520	rVB2	500	378	0.03%	0.003%
11	2.728	520	525	527	rBV2	293	259	0.02%	0.002%
12	2.754	530	533	535	rBV2	559	367	0.03%	0.003%
13	2.879	570	572	575	rVB3	480	258	0.02%	0.002%
14	2.902	575	579	580	rVB	238	149	0.01%	0.001%
15	2.944	591	592	594	rBV	514	225	0.02%	0.002%
16	2.998	608	609	610	rBV	358	103	0.01%	0.001%
17	3.011	610	613	616	rVV3	461	301	0.02%	0.003%
18	3.085	631	636	637	rBV2	353	246	0.02%	0.002%
19	3.140	652	653	655	rVB	355	127	0.01%	0.001%
20	3.175	661	664	666	rBV2	847	549	0.04%	0.005%
21	3.252	687	688	692	rVB2	207	149	0.01%	0.001%
22	3.275	692	695	697	rBV2	355	238	0.02%	0.002%
23	3.297	700	702	704	rVV	462	252	0.02%	0.002%
24	3.326	708	711	714	rBV2	494	296	0.02%	0.003%
25	3.375	724	726	729	rBV	290	172	0.01%	0.002%
26	3.391	729	731	733	rVV	244	127	0.01%	0.001%
27	3.413	736	738	741	rBV2	441	258	0.02%	0.002%
28	3.474	754	757	759	rVV2	438	263	0.02%	0.002%
29	3.503	763	766	767	rBV2	222	144	0.01%	0.001%
30	3.529	772	774	776	rVB3	347	138	0.01%	0.001%
31	3.558	781	783	784	rBV3	499	156	0.01%	0.001%
32	3.625	799	804	807	rBV2	250	310	0.02%	0.003%
33	3.667	813	817	818	rBV	158	100	0.01%	0.001%
34	3.728	834	836	840	rBV2	475	143	0.01%	0.001%
35	3.760	844	846	848	rVB2	285	133	0.01%	0.001%
36	3.776	848	851	852	rBV	295	141	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027983.D
 Acq On : 20 Sep 2022 23:46
 Operator : SY/MD
 Sample : N4620-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.802	858	859	864	rVB2	464	229	0.02%	0.002%
38	3.831	864	868	870	rBV2	149	119	0.01%	0.001%
39	3.873	872	881	923	rBV	118776	393081	27.37%	3.484%
40	4.339	1010	1026	1052	rBV	235991	585479	40.77%	5.190%
41	4.535	1085	1087	1091	rBV3	553	261	0.02%	0.002%
42	4.606	1096	1109	1123	rVV6	6635	15482	1.08%	0.137%
43	4.670	1127	1129	1130	rBV	469	182	0.01%	0.002%
44	4.702	1136	1139	1141	rVB2	508	281	0.02%	0.002%
45	4.725	1144	1146	1147	rVV	464	160	0.01%	0.001%
46	4.735	1147	1149	1152	rVB2	503	199	0.01%	0.002%
47	4.754	1153	1155	1156	rVV	341	117	0.01%	0.001%
48	4.780	1160	1163	1164	rBV2	345	180	0.01%	0.002%
49	4.802	1168	1170	1172	rBV	235	129	0.01%	0.001%
50	4.828	1176	1178	1181	rVB	434	201	0.01%	0.002%
51	4.850	1181	1185	1189	rVB3	398	259	0.02%	0.002%
52	4.870	1189	1191	1192	rBV	331	113	0.01%	0.001%
53	4.902	1199	1201	1205	rVB2	703	535	0.04%	0.005%
54	4.982	1224	1226	1227	rBV	415	182	0.01%	0.002%
55	5.040	1227	1244	1277	rVV2	560679	1436128	100.00%	12.729%
56	5.297	1322	1324	1326	rBV2	429	246	0.02%	0.002%
57	5.374	1345	1348	1349	rBV	413	223	0.02%	0.002%
58	5.407	1356	1358	1360	rBV	657	414	0.03%	0.004%
59	5.436	1364	1367	1369	rBV	488	360	0.03%	0.003%
60	5.477	1377	1380	1383	rBV2	909	795	0.06%	0.007%
61	5.519	1392	1393	1398	rVB2	540	236	0.02%	0.002%
62	5.542	1398	1400	1401	rBV2	533	214	0.01%	0.002%
63	5.551	1401	1403	1405	rBV	303	179	0.01%	0.002%
64	5.609	1409	1421	1451	rBV	404473	822636	57.28%	7.292%
65	5.915	1504	1516	1532	rBV8	9226	23574	1.64%	0.209%
66	6.011	1543	1546	1548	rBV2	494	294	0.02%	0.003%
67	6.063	1548	1562	1588	rBV	316249	648121	45.13%	5.745%
68	6.281	1625	1630	1632	rBV4	1011	699	0.05%	0.006%
69	6.352	1648	1652	1654	rBV	544	329	0.02%	0.003%
70	6.477	1689	1691	1692	rBV	787	277	0.02%	0.002%
71	6.632	1734	1739	1740	rBV3	1026	647	0.05%	0.006%
72	6.648	1740	1744	1746	rBV5	1106	863	0.06%	0.008%
73	6.886	1812	1818	1820	rBV6	1316	1276	0.09%	0.011%
74	6.982	1837	1848	1871	rBV	169747	321279	22.37%	2.848%
75	7.313	1939	1951	1971	rBV	664606	1156503	80.53%	10.251%
76	7.619	2037	2046	2071	rBV	124227	219014	15.25%	1.941%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027983.D
 Acq On : 20 Sep 2022 23:46
 Operator : SY/MD
 Sample : N4620-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E50

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	8.085	2180	2191	2216	rBV	447834	810024	56.40%	7.180%
78	8.683	2375	2377	2384	rVB6	1058	1097	0.08%	0.010%
79	8.712	2384	2386	2387	rBV	672	264	0.02%	0.002%
80	8.757	2398	2400	2402	rBV2	1008	703	0.05%	0.006%
81	8.847	2417	2428	2453	rBV	649252	1049211	73.06%	9.300%
82	9.104	2506	2508	2510	rBV2	1002	433	0.03%	0.004%
83	9.239	2548	2550	2553	rBV4	997	666	0.05%	0.006%
84	9.439	2610	2612	2619	rBV6	871	811	0.06%	0.007%
85	9.763	2707	2713	2718	rBV5	857	1155	0.08%	0.010%
86	9.805	2722	2726	2728	rBV3	970	668	0.05%	0.006%
87	9.982	2778	2781	2782	rBV2	798	443	0.03%	0.004%
88	10.213	2841	2853	2873	rBV	495084	766524	53.37%	6.794%
89	10.718	3009	3010	3012	rBV	874	308	0.02%	0.003%
90	10.914	3065	3071	3080	rVB8	2751	3784	0.26%	0.034%
91	11.201	3158	3160	3161	rBV	560	272	0.02%	0.002%
92	11.246	3163	3174	3195	rVV	579525	883135	61.49%	7.828%
93	11.622	3280	3291	3311	rVB	628827	971489	67.65%	8.611%
94	12.313	3503	3506	3512	rBV3	1249	1298	0.09%	0.012%
95	12.840	3666	3670	3672	rBV3	1081	877	0.06%	0.008%
96	13.188	3775	3778	3780	rBV3	513	375	0.03%	0.003%
97	13.213	3783	3786	3791	rVB5	1140	976	0.07%	0.009%
98	13.284	3806	3808	3813	rVB4	987	650	0.05%	0.006%
99	13.474	3865	3867	3869	rBV2	857	473	0.03%	0.004%
100	13.561	3893	3894	3896	rBV	798	338	0.02%	0.003%

Sum of corrected areas: 11281903




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027983.D
Acq On : 20 Sep 2022 23:46
Operator : SY/MD
Sample : N4620-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L

TIC Integration Parameters: LSCINT.P

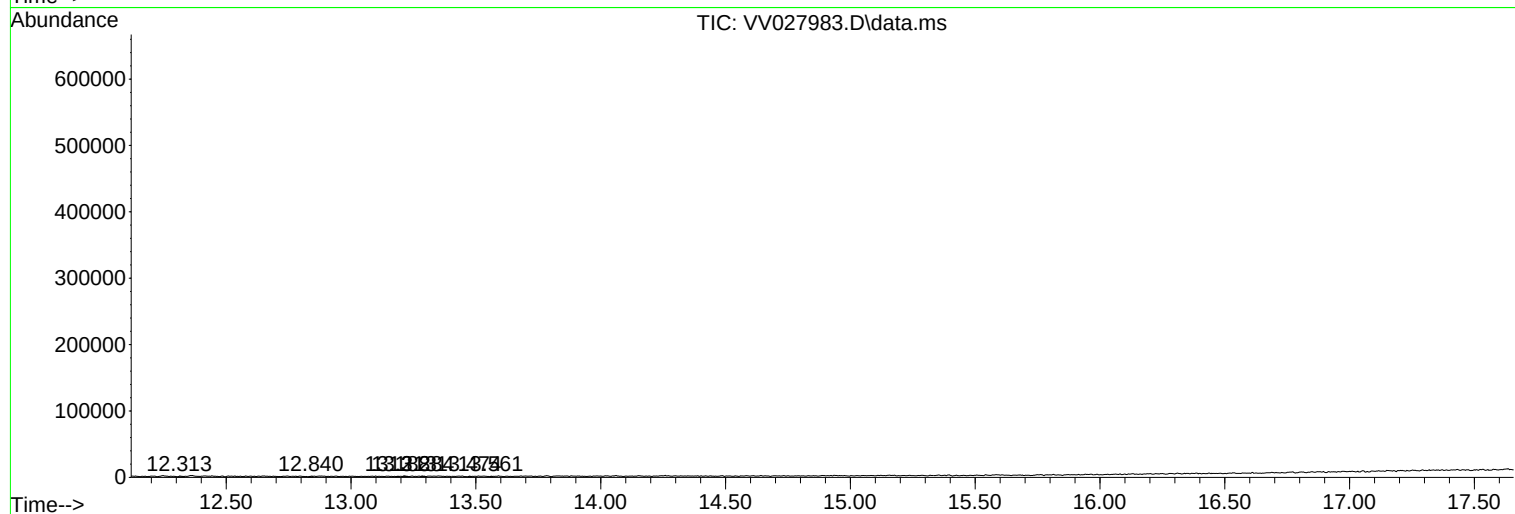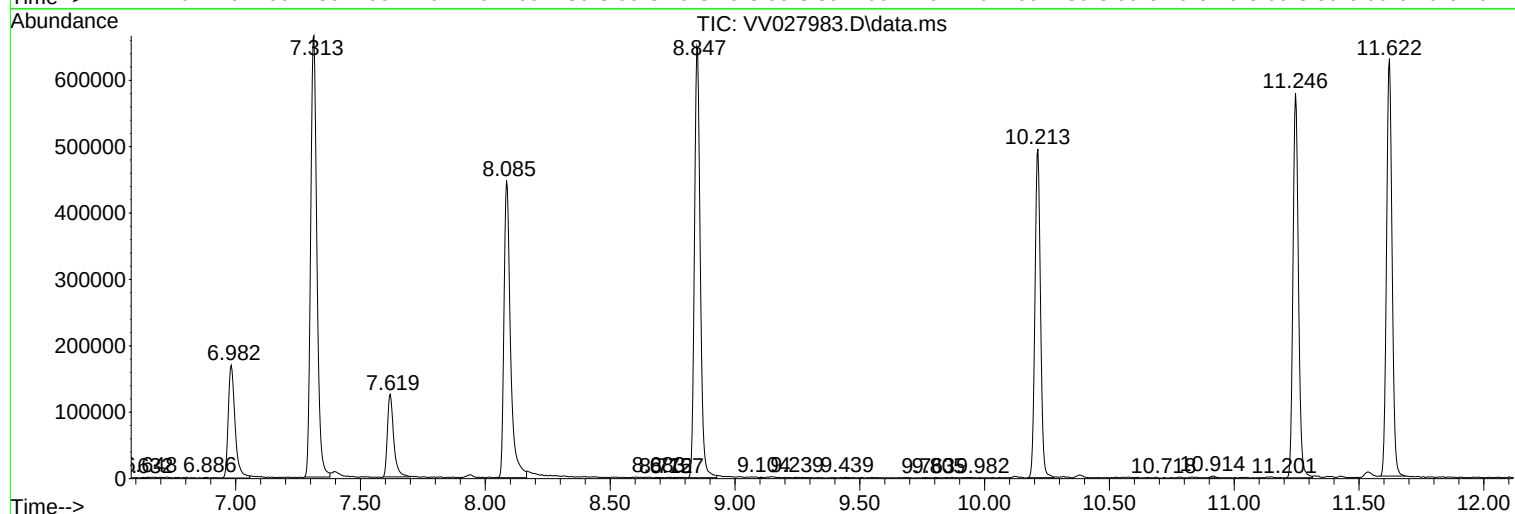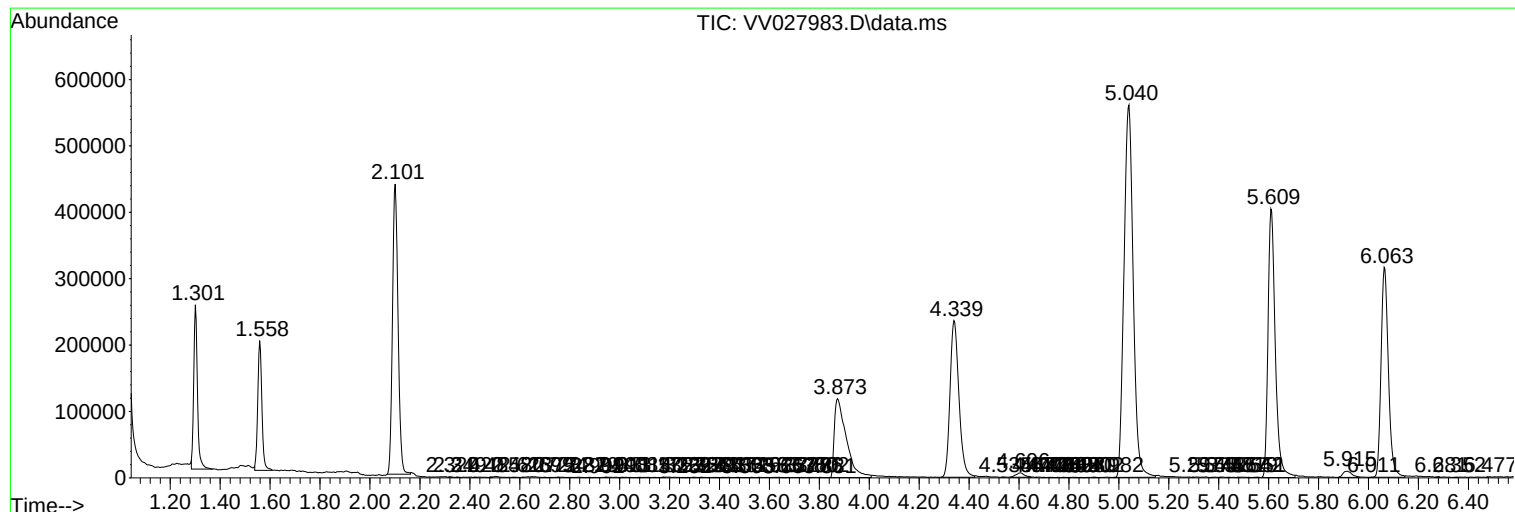

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027983.D
Acq On : 20 Sep 2022 23:46
Operator : SY/MD
Sample : N4620-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027983.D
Acq On : 20 Sep 2022 23:46
Operator : SY/MD
Sample : N4620-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 29 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E50

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc