

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027984.D
 Acq On : 21 Sep 2022 00:11
 Operator : SY/MD
 Sample : N4620-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M

Title : VOC Analysis

Signal : TIC: VV027984.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	97	rVB	242306	253816	16.44%	2.268%
2	1.558	155	161	175	rVB	196289	219666	14.23%	1.963%
3	2.098	320	329	345	rBV	402183	580173	37.58%	5.185%
4	2.404	422	424	426	rBV	423	236	0.02%	0.002%
5	2.532	462	464	468	rBV3	258	208	0.01%	0.002%
6	2.577	475	478	483	rVB2	402	333	0.02%	0.003%
7	2.596	483	484	485	rBV	295	80	0.01%	0.001%
8	2.619	489	491	494	rVV2	493	189	0.01%	0.002%
9	2.757	531	534	540	rBV3	757	792	0.05%	0.007%
10	2.796	544	546	548	rVV	361	189	0.01%	0.002%
11	2.822	550	554	556	rVV2	503	359	0.02%	0.003%
12	2.847	560	562	564	rBV	255	176	0.01%	0.002%
13	2.876	569	571	574	rVB	492	270	0.02%	0.002%
14	2.895	574	577	579	rBV2	478	318	0.02%	0.003%
15	2.976	599	602	605	rVB	399	279	0.02%	0.002%
16	2.992	605	607	610	rBV2	353	160	0.01%	0.001%
17	3.008	610	612	613	rBV	217	82	0.01%	0.001%
18	3.021	613	616	619	rBV	266	228	0.01%	0.002%
19	3.188	666	668	674	rVB2	443	355	0.02%	0.003%
20	3.214	674	676	677	rBV	205	93	0.01%	0.001%
21	3.239	682	684	685	rBV	166	48	0.00%	0.000%
22	3.288	696	699	700	rBV	191	105	0.01%	0.001%
23	3.320	707	709	714	rBV2	272	135	0.01%	0.001%
24	3.342	714	716	717	rBV	230	76	0.00%	0.001%
25	3.349	717	718	720	rBV	269	100	0.01%	0.001%
26	3.368	723	724	725	rBV	278	91	0.01%	0.001%
27	3.394	731	732	733	rVB	124	24	0.00%	0.000%
28	3.407	734	736	738	rBV2	467	191	0.01%	0.002%
29	3.420	738	740	744	rVB	414	202	0.01%	0.002%
30	3.436	744	745	746	rBV	170	58	0.00%	0.001%
31	3.458	750	752	753	rBV	90	34	0.00%	0.000%
32	3.522	770	772	774	rBV	219	81	0.01%	0.001%
33	3.574	786	788	791	rBV	448	227	0.01%	0.002%
34	3.590	791	793	795	rVV2	407	186	0.01%	0.002%
35	3.612	799	800	801	rVV	150	37	0.00%	0.000%
36	3.632	802	806	810	rVB4	496	383	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027984.D
 Acq On : 21 Sep 2022 00:11
 Operator : SY/MD
 Sample : N4620-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 30 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E51

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.654	810	813	815	rBV	209	109	0.01%	0.001%
38	3.677	815	820	825	rVB2	424	483	0.03%	0.004%
39	3.699	825	827	831	rBV	276	235	0.02%	0.002%
40	3.725	833	835	840	rVB2	319	154	0.01%	0.001%
41	3.744	840	841	843	rBV2	235	89	0.01%	0.001%
42	3.786	850	854	858	rVB4	463	427	0.03%	0.004%
43	3.805	858	860	862	rBV2	299	201	0.01%	0.002%
44	3.873	871	881	916	rBV	116359	322923	20.91%	2.886%
45	4.339	1011	1026	1052	rBV	250707	620462	40.19%	5.545%
46	4.664	1126	1127	1129	rBV2	646	188	0.01%	0.002%
47	4.931	1208	1210	1213	rBV4	879	591	0.04%	0.005%
48	5.037	1226	1243	1269	rBV2	604232	1543986	100.00%	13.798%
49	5.397	1353	1355	1362	rBV5	1145	895	0.06%	0.008%
50	5.609	1410	1421	1455	rBV	409589	848355	54.95%	7.581%
51	6.063	1549	1562	1583	rBV	342492	706081	45.73%	6.310%
52	6.342	1647	1649	1651	rBV3	566	203	0.01%	0.002%
53	6.368	1655	1657	1661	rVV4	1172	535	0.03%	0.005%
54	6.841	1801	1804	1805	rBV2	627	303	0.02%	0.003%
55	6.921	1827	1829	1832	rVB2	800	452	0.03%	0.004%
56	6.937	1832	1834	1836	rBV2	602	395	0.03%	0.004%
57	6.982	1838	1848	1870	rVV	166648	309258	20.03%	2.764%
58	7.310	1939	1950	1971	rBV	662093	1153144	74.69%	10.305%
59	7.619	2037	2046	2063	rBV	118906	205152	13.29%	1.833%
60	8.085	2181	2191	2216	rBV	447108	799268	51.77%	7.143%
61	8.847	2417	2428	2453	rBV	629905	1019371	66.02%	9.109%
62	9.146	2515	2521	2527	rBV9	1612	2260	0.15%	0.020%
63	9.551	2642	2647	2648	rBV4	1172	967	0.06%	0.009%
64	9.911	2757	2759	2760	rBV	411	159	0.01%	0.001%
65	10.114	2819	2822	2824	rBV3	2368	1754	0.11%	0.016%
66	10.213	2841	2853	2871	rBV	477406	755233	48.91%	6.749%
67	10.699	3002	3004	3005	rBV	553	250	0.02%	0.002%
68	10.712	3006	3008	3011	rVV3	621	329	0.02%	0.003%
69	11.101	3127	3129	3132	rBV3	1234	785	0.05%	0.007%
70	11.246	3163	3174	3192	rBV	567201	870769	56.40%	7.781%
71	11.622	3279	3291	3309	rBV	606084	958932	62.11%	8.569%
72	11.824	3351	3354	3355	rBV3	1198	716	0.05%	0.006%
73	11.882	3370	3372	3375	rBV3	774	423	0.03%	0.004%
74	11.998	3404	3408	3409	rBV3	946	578	0.04%	0.005%
75	12.123	3445	3447	3448	rBV	763	355	0.02%	0.003%
76	12.596	3591	3594	3596	rBV4	1325	930	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027984.D
Acq On : 21 Sep 2022 00:11
Operator : SY/MD
Sample : N4620-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E51

Integration Parameters: LSCINT.P
Integrator: RTE
Smoothing : OFF Filtering: 5
Sampling : 1 Min Area: 0 % of largest Peak
Start Thrs: 0.2 Max Peaks: 100
Stop Thrs : 0 Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >
Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Title : VOC Analysis

77	12.876	3679	3681	3688	rVB4	937	988	0.06%	0.009%
78	13.027	3726	3728	3733	rBV4	1030	835	0.05%	0.007%
79	13.326	3818	3821	3824	rBV2	1000	798	0.05%	0.007%




Sum of corrected areas: 11190301

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027984.D
Acq On : 21 Sep 2022 00:11
Operator : SY/MD
Sample : N4620-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

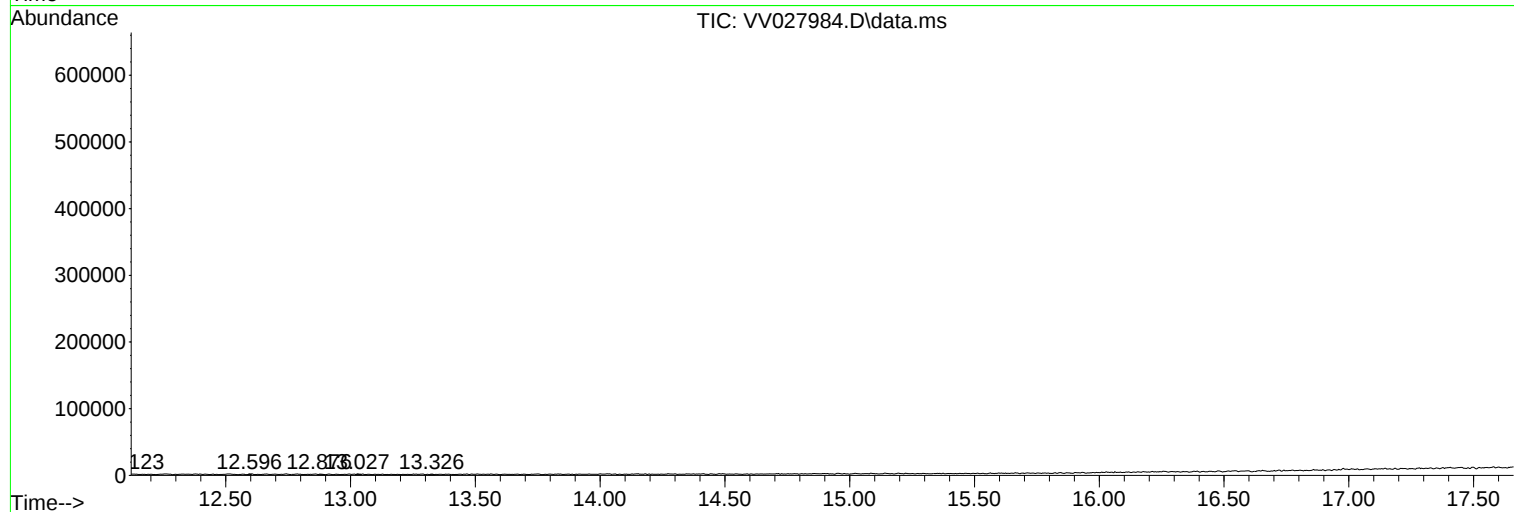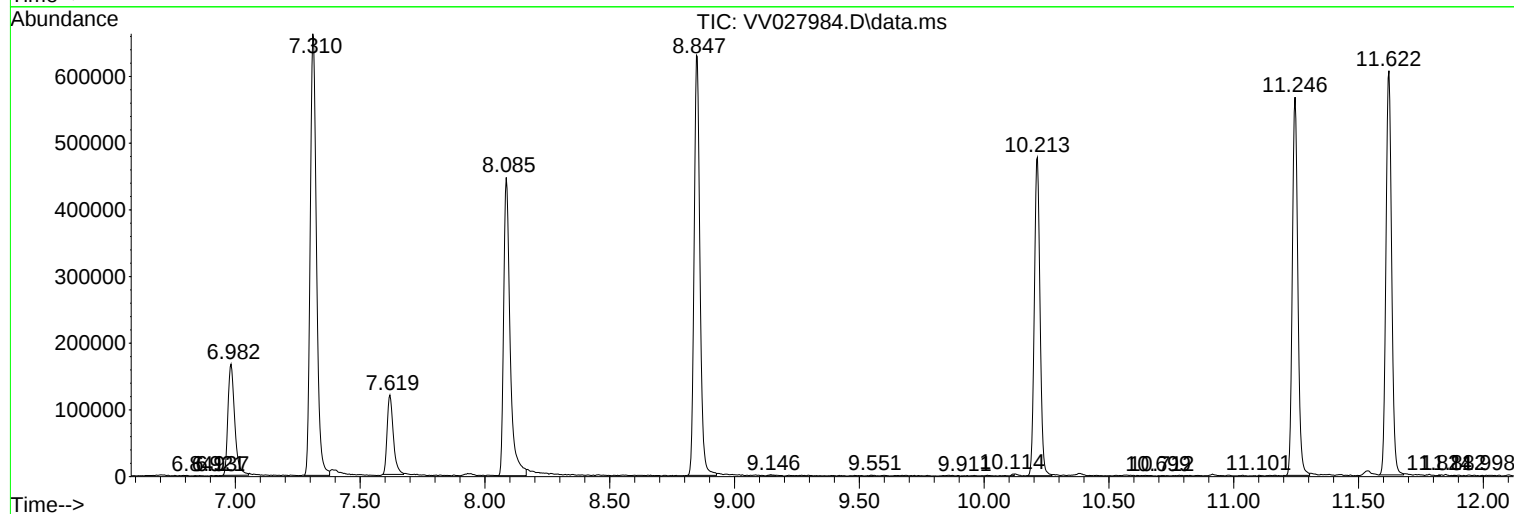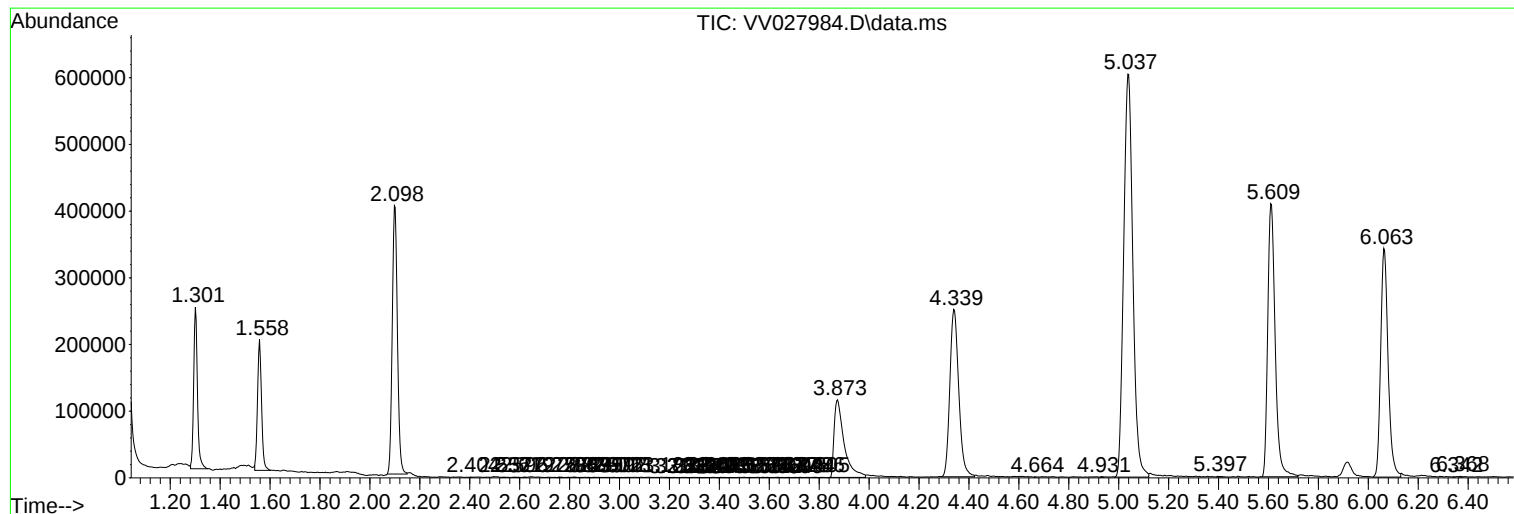

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027984.D
Acq On : 21 Sep 2022 00:11
Operator : SY/MD
Sample : N4620-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027984.D
Acq On : 21 Sep 2022 00:11
Operator : SY/MD
Sample : N4620-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 30 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E51

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc