

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027988.D
 Acq On : 21 Sep 2022 02:15
 Operator : SY/MD
 Sample : N4674-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027988.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	101	rVB	223382	240735	16.14%	2.181%
2	1.561	156	162	178	rVB	181226	211183	14.15%	1.913%
3	2.101	320	330	346	rBV	371569	536466	35.96%	4.860%
4	2.275	380	384	385	rBV3	1220	760	0.05%	0.007%
5	2.497	449	453	462	rVB8	1936	3178	0.21%	0.029%
6	2.532	462	464	465	rBV8	422	186	0.01%	0.002%
7	2.555	469	471	474	rVB3	308	150	0.01%	0.001%
8	2.571	474	476	479	rBV2	478	301	0.02%	0.003%
9	2.590	480	482	486	rVV3	642	415	0.03%	0.004%
10	2.609	486	488	493	rVB4	680	539	0.04%	0.005%
11	2.635	493	496	498	rBV	336	189	0.01%	0.002%
12	2.658	500	503	504	rBV	274	129	0.01%	0.001%
13	2.693	511	514	515	rBV	375	192	0.01%	0.002%
14	2.719	520	522	524	rBV2	413	160	0.01%	0.001%
15	2.751	528	532	533	rBV2	935	638	0.04%	0.006%
16	2.873	567	570	572	rBV2	313	207	0.01%	0.002%
17	2.928	584	587	588	rBV2	417	245	0.02%	0.002%
18	2.937	588	590	591	rVV	235	80	0.01%	0.001%
19	2.966	596	599	604	rVB3	508	431	0.03%	0.004%
20	2.995	604	608	609	rBV2	232	121	0.01%	0.001%
21	3.008	609	612	614	rVB	629	248	0.02%	0.002%
22	3.021	614	616	617	rBV	326	110	0.01%	0.001%
23	3.056	625	627	630	rVB2	681	283	0.02%	0.003%
24	3.076	632	633	634	rBV2	218	49	0.00%	0.000%
25	3.088	635	637	642	rVB4	522	388	0.03%	0.004%
26	3.127	647	649	650	rBV	234	76	0.01%	0.001%
27	3.146	652	655	657	rBV	579	373	0.03%	0.003%
28	3.275	692	695	698	rBV2	531	319	0.02%	0.003%
29	3.542	776	778	780	rBV	595	357	0.02%	0.003%
30	3.638	806	808	809	rBV	538	130	0.01%	0.001%
31	3.703	827	828	832	rVB3	779	360	0.02%	0.003%
32	3.728	832	836	838	rBV2	675	542	0.04%	0.005%
33	3.751	841	843	847	rVB2	964	580	0.04%	0.005%
34	3.876	872	882	914	rBV	125318	363254	24.35%	3.291%
35	4.339	1011	1026	1049	rBV	245607	608486	40.78%	5.513%
36	4.895	1198	1199	1200	rBV	454	153	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027988.D
 Acq On : 21 Sep 2022 02:15
 Operator : SY/MD
 Sample : N4674-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	5.040	1226	1244	1266	rBV2	585990	1491999	100.00%	13.517%
38	5.516	1386	1392	1394	rBV5	974	855	0.06%	0.008%
39	5.548	1401	1402	1405	rBV3	653	335	0.02%	0.003%
40	5.609	1409	1421	1449	rBV	405499	834143	55.91%	7.557%
41	5.915	1501	1516	1534	rBV3	35452	82017	5.50%	0.743%
42	6.063	1550	1562	1587	rBV	335950	687506	46.08%	6.229%
43	6.387	1661	1663	1666	rBV	514	366	0.02%	0.003%
44	6.538	1707	1710	1712	rBV2	851	456	0.03%	0.004%
45	6.629	1736	1738	1741	rBV4	744	541	0.04%	0.005%
46	6.821	1793	1798	1800	rBV3	684	545	0.04%	0.005%
47	6.876	1812	1815	1818	rBV4	727	540	0.04%	0.005%
48	6.940	1834	1835	1837	rVB	858	263	0.02%	0.002%
49	6.982	1837	1848	1865	rBV	166587	310141	20.79%	2.810%
50	7.310	1939	1950	1970	rBV	628359	1104460	74.03%	10.006%
51	7.619	2037	2046	2064	rBV	117959	209549	14.04%	1.898%
52	8.085	2181	2191	2216	rBV	424383	771879	51.73%	6.993%
53	8.458	2305	2307	2309	rBV2	872	446	0.03%	0.004%
54	8.776	2403	2406	2408	rBV3	923	516	0.03%	0.005%
55	8.850	2417	2429	2459	rBV	620607	1021055	68.44%	9.250%
56	9.445	2612	2614	2615	rBV2	397	117	0.01%	0.001%
57	9.538	2640	2643	2644	rBV4	691	424	0.03%	0.004%
58	9.638	2672	2674	2676	rBV3	558	295	0.02%	0.003%
59	9.689	2688	2690	2691	rBV	438	148	0.01%	0.001%
60	9.741	2703	2706	2711	rVB5	798	598	0.04%	0.005%
61	9.831	2731	2734	2736	rBV3	607	406	0.03%	0.004%
62	9.921	2759	2762	2764	rBV3	1024	713	0.05%	0.006%
63	9.960	2773	2774	2778	rVB2	1183	457	0.03%	0.004%
64	10.075	2809	2810	2811	rBV	588	180	0.01%	0.002%
65	10.124	2820	2825	2832	rVB6	2024	2576	0.17%	0.023%
66	10.214	2840	2853	2870	rBV	486949	765893	51.33%	6.939%
67	10.374	2901	2903	2906	rBV2	1767	1360	0.09%	0.012%
68	10.461	2928	2930	2931	rBV2	538	173	0.01%	0.002%
69	10.480	2935	2936	2938	rVB	741	160	0.01%	0.001%
70	10.509	2942	2945	2947	rBV2	1052	599	0.04%	0.005%
71	10.529	2949	2951	2952	rBV2	875	367	0.02%	0.003%
72	10.661	2990	2992	2996	rBV3	850	481	0.03%	0.004%
73	10.680	2996	2998	3002	rVB4	640	288	0.02%	0.003%
74	10.799	3033	3035	3037	rBV2	785	317	0.02%	0.003%
75	10.841	3046	3048	3050	rBV3	1044	640	0.04%	0.006%
76	10.915	3066	3071	3082	rVB9	2361	3508	0.24%	0.032%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027988.D
 Acq On : 21 Sep 2022 02:15
 Operator : SY/MD
 Sample : N4674-01
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 35 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E95

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	11.027	3105	3106	3111	rBV2	410	281	0.02%	0.003%
78	11.059	3115	3116	3118	rBV	363	129	0.01%	0.001%
79	11.101	3123	3129	3131	rBV4	456	404	0.03%	0.004%
80	11.140	3136	3141	3146	rBV5	951	872	0.06%	0.008%
81	11.162	3146	3148	3150	rBV	520	308	0.02%	0.003%
82	11.246	3163	3174	3193	rBV	541916	844704	56.62%	7.653%
83	11.461	3239	3241	3248	rVB4	665	639	0.04%	0.006%
84	11.493	3249	3251	3253	rVV2	640	251	0.02%	0.002%
85	11.535	3262	3264	3265	rBV	468	168	0.01%	0.002%
86	11.622	3279	3291	3313	rBV	578783	915748	61.38%	8.296%
87	11.760	3332	3334	3340	rBV5	702	571	0.04%	0.005%
88	11.892	3372	3375	3376	rBV2	332	207	0.01%	0.002%
89	11.902	3376	3378	3380	rVV2	482	169	0.01%	0.002%
90	11.931	3385	3387	3390	rBV2	357	232	0.02%	0.002%
91	11.950	3390	3393	3396	rBV2	710	450	0.03%	0.004%
92	12.062	3426	3428	3432	rBV3	646	438	0.03%	0.004%
93	12.149	3453	3455	3457	rBV2	480	286	0.02%	0.003%
94	12.471	3553	3555	3558	rBV3	721	410	0.03%	0.004%
95	12.554	3580	3581	3584	rBV	554	331	0.02%	0.003%
96	12.638	3605	3607	3608	rBV	820	444	0.03%	0.004%
97	12.789	3650	3654	3656	rBV	480	393	0.03%	0.004%
98	13.059	3737	3738	3740	rBV	696	240	0.02%	0.002%
99	14.738	4256	4260	4261	rBV3	1041	867	0.06%	0.008%

Sum of corrected areas: 11037867




Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027988.D
Acq On : 21 Sep 2022 02:15
Operator : SY/MD
Sample : N4674-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L

TIC Integration Parameters: LSCINT.P

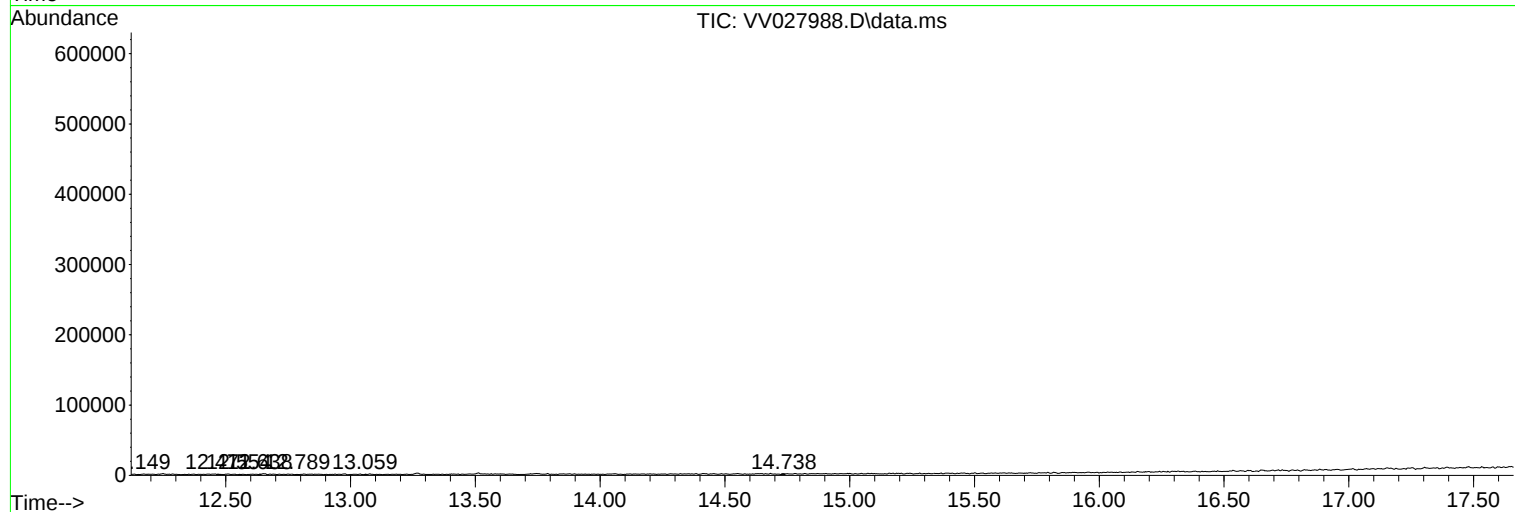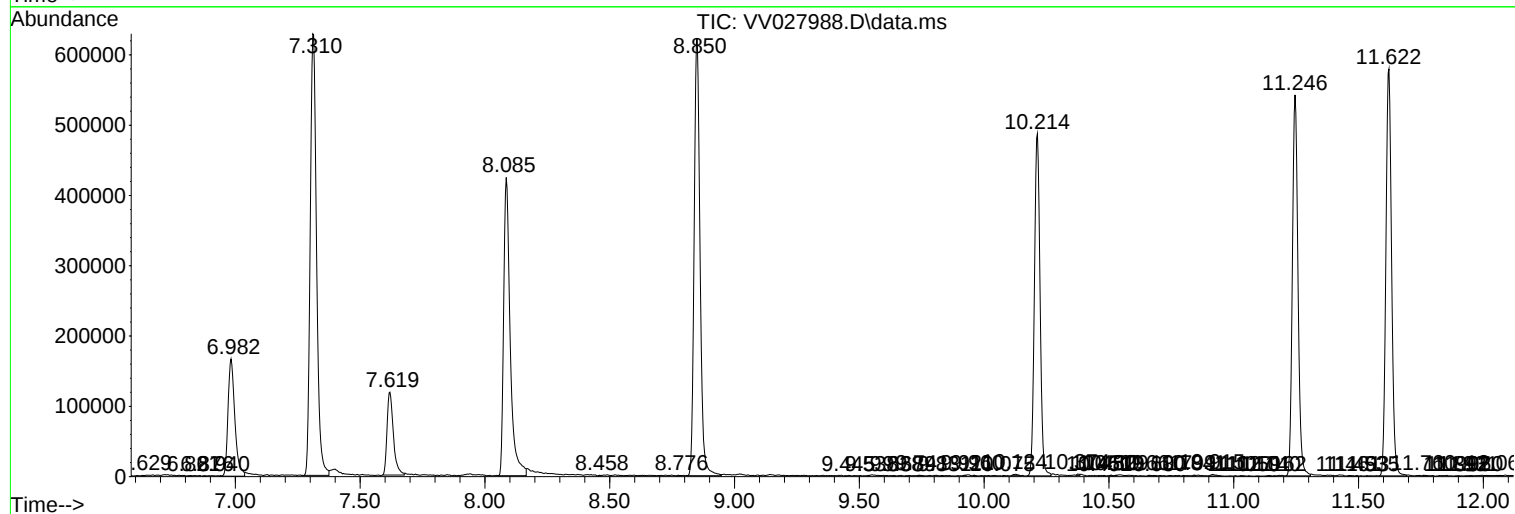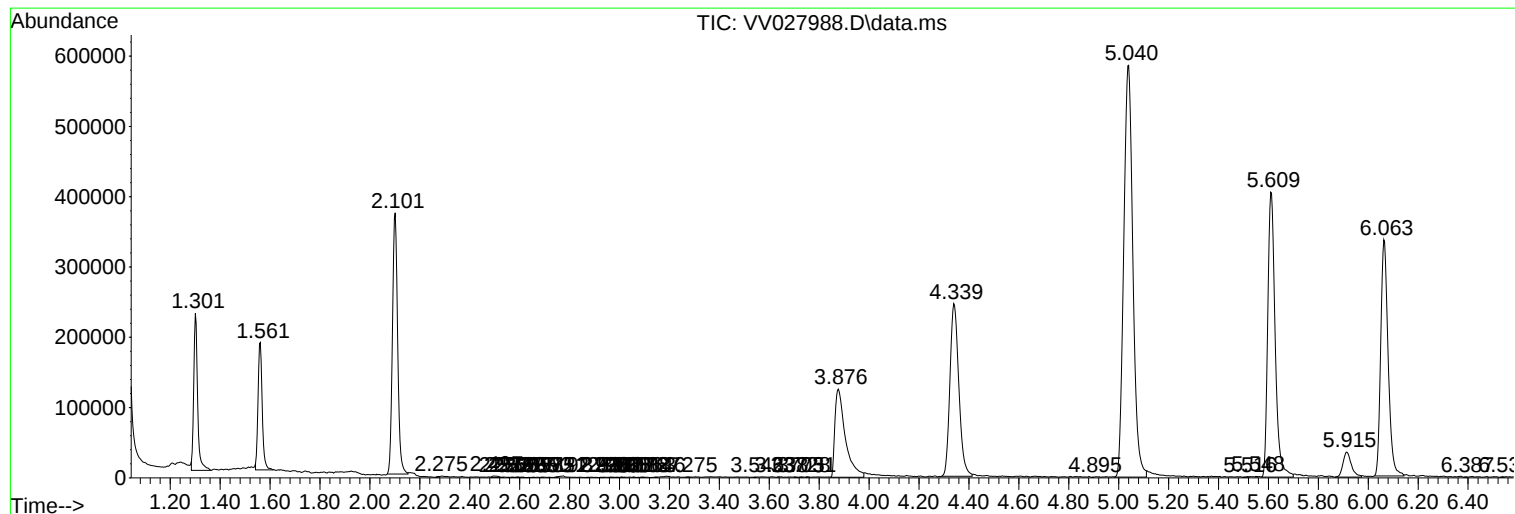

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027988.D
Acq On : 21 Sep 2022 02:15
Operator : SY/MD
Sample : N4674-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027988.D
Acq On : 21 Sep 2022 02:15
Operator : SY/MD
Sample : N4674-01
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 35 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E95

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc