

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027989.D
 Acq On : 21 Sep 2022 02:39
 Operator : SY/MD
 Sample : N4674-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027989.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	95	rVB	217605	222400	15.89%	2.037%
2	1.561	155	162	177	rVB	180672	211542	15.12%	1.938%
3	2.101	320	330	346	rBV	374046	540070	38.60%	4.948%
4	2.500	445	454	461	rBV7	1673	2555	0.18%	0.023%
5	2.574	475	477	479	rVB2	341	118	0.01%	0.001%
6	2.593	482	483	485	rVB2	410	111	0.01%	0.001%
7	2.606	485	487	488	rBV2	300	130	0.01%	0.001%
8	2.645	491	499	505	rBV6	1113	1579	0.11%	0.014%
9	2.735	525	527	528	rBV	110	45	0.00%	0.000%
10	2.741	528	529	530	rBV	223	44	0.00%	0.000%
11	2.754	532	533	535	rBV	283	102	0.01%	0.001%
12	2.786	540	543	545	rBV2	511	356	0.03%	0.003%
13	2.828	554	556	557	rVB2	412	125	0.01%	0.001%
14	2.844	557	561	564	rBV3	366	212	0.02%	0.002%
15	2.892	574	576	578	rBV	352	184	0.01%	0.002%
16	2.908	578	581	584	rVV	343	269	0.02%	0.002%
17	2.928	584	587	589	rVV2	364	267	0.02%	0.002%
18	2.950	591	594	597	rVV2	589	329	0.02%	0.003%
19	2.973	597	601	607	rVV4	378	397	0.03%	0.004%
20	3.002	607	610	612	rBV	278	162	0.01%	0.001%
21	3.076	631	633	635	rVV2	348	127	0.01%	0.001%
22	3.085	635	636	639	rVB2	366	125	0.01%	0.001%
23	3.143	649	654	657	rBV3	326	269	0.02%	0.002%
24	3.169	660	662	664	rVV	371	196	0.01%	0.002%
25	3.220	676	678	679	rBV	234	81	0.01%	0.001%
26	3.314	704	707	708	rBV2	191	111	0.01%	0.001%
27	3.326	708	711	712	rVV	261	109	0.01%	0.001%
28	3.346	715	717	720	rVV2	362	208	0.01%	0.002%
29	3.362	720	722	724	rBV2	252	105	0.01%	0.001%
30	3.387	729	730	731	rBV	168	39	0.00%	0.000%
31	3.413	736	738	739	rBV2	205	67	0.00%	0.001%
32	3.442	744	747	750	rBV3	337	223	0.02%	0.002%
33	3.465	753	754	760	rVB2	593	339	0.02%	0.003%
34	3.490	760	762	764	rBV	240	125	0.01%	0.001%
35	3.503	764	766	768	rBV	428	203	0.01%	0.002%
36	3.532	771	775	777	rBV2	312	227	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027989.D
 Acq On : 21 Sep 2022 02:39
 Operator : SY/MD
 Sample : N4674-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.548	777	780	782	rBV2	477	239	0.02%	0.002%
38	3.587	789	792	794	rBV	283	202	0.01%	0.002%
39	3.703	826	828	829	rBV	180	70	0.01%	0.001%
40	3.715	829	832	836	rVV4	449	379	0.03%	0.003%
41	3.770	847	849	850	rBV	304	83	0.01%	0.001%
42	3.799	857	858	859	rVB	263	51	0.00%	0.000%
43	3.831	864	868	870	rVB2	476	249	0.02%	0.002%
44	3.873	871	881	918	rBV	115378	324321	23.18%	2.971%
45	4.207	984	985	987	rBV	566	217	0.02%	0.002%
46	4.342	1009	1027	1056	rBV2	229726	577716	41.29%	5.293%
47	4.587	1098	1103	1104	rBV2	755	476	0.03%	0.004%
48	4.664	1126	1127	1128	rBV2	360	117	0.01%	0.001%
49	4.719	1142	1144	1149	rVB	499	352	0.03%	0.003%
50	4.767	1158	1159	1160	rBV	319	89	0.01%	0.001%
51	4.780	1161	1163	1165	rVB	515	221	0.02%	0.002%
52	4.825	1171	1177	1179	rBV3	378	411	0.03%	0.004%
53	4.902	1198	1201	1206	rBV3	574	378	0.03%	0.003%
54	4.921	1206	1207	1208	rBV	194	53	0.00%	0.000%
55	4.953	1215	1217	1221	rVB3	481	217	0.02%	0.002%
56	5.040	1227	1244	1272	rBV2	544022	1399207	100.00%	12.819%
57	5.474	1377	1379	1380	rBV	647	214	0.02%	0.002%
58	5.506	1388	1389	1390	rVB	434	84	0.01%	0.001%
59	5.529	1394	1396	1399	rBV3	356	260	0.02%	0.002%
60	5.609	1409	1421	1450	rBV	409589	844310	60.34%	7.735%
61	5.812	1482	1484	1488	rVB5	1297	734	0.05%	0.007%
62	5.985	1535	1538	1540	rBV3	1116	877	0.06%	0.008%
63	6.063	1549	1562	1591	rBV	335637	691816	49.44%	6.338%
64	6.349	1649	1651	1656	rBV5	775	586	0.04%	0.005%
65	6.513	1700	1702	1706	rBV3	659	460	0.03%	0.004%
66	6.587	1724	1725	1727	rBV	352	152	0.01%	0.001%
67	6.802	1790	1792	1793	rBV	894	350	0.03%	0.003%
68	6.860	1807	1810	1814	rBV6	1125	1142	0.08%	0.010%
69	6.982	1837	1848	1867	rBV	164779	308384	22.04%	2.825%
70	7.310	1939	1950	1972	rBV	634636	1105484	79.01%	10.128%
71	7.619	2037	2046	2066	rBV	118393	207651	14.84%	1.902%
72	8.027	2170	2173	2176	rBV5	822	554	0.04%	0.005%
73	8.085	2181	2191	2226	rBV	450459	826355	59.06%	7.570%
74	8.400	2286	2289	2294	rBV4	1486	1354	0.10%	0.012%
75	8.847	2417	2428	2454	rBV	626277	1026868	73.39%	9.407%
76	9.294	2563	2567	2569	rVB2	998	641	0.05%	0.006%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027989.D
 Acq On : 21 Sep 2022 02:39
 Operator : SY/MD
 Sample : N4674-02
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 36 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E97

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.452	2612	2616	2618	rBV2	829	521	0.04%	0.005%
78	9.461	2618	2619	2622	rVB3	741	260	0.02%	0.002%
79	9.599	2660	2662	2665	rBV4	1174	669	0.05%	0.006%
80	9.754	2708	2710	2711	rBV2	561	159	0.01%	0.001%
81	9.905	2753	2757	2758	rBV2	837	526	0.04%	0.005%
82	9.979	2778	2780	2782	rBV	1022	569	0.04%	0.005%
83	10.214	2841	2853	2876	rBV	490259	770298	55.05%	7.057%
84	10.435	2918	2922	2926	rBV4	937	954	0.07%	0.009%
85	11.246	3163	3174	3190	rBV	562538	879649	62.87%	8.059%
86	11.493	3249	3251	3254	rBV3	966	510	0.04%	0.005%
87	11.622	3280	3291	3309	rBV	607447	949169	67.84%	8.696%
88	11.824	3351	3354	3356	rBV2	1075	595	0.04%	0.005%
89	11.847	3359	3361	3362	rBV2	1018	272	0.02%	0.002%
90	11.940	3387	3390	3392	rBV2	1297	710	0.05%	0.007%
91	12.840	3668	3670	3672	rBV	1098	438	0.03%	0.004%
92	12.921	3693	3695	3696	rBV	788	380	0.03%	0.003%
93	12.956	3704	3706	3708	rVB2	765	287	0.02%	0.003%
94	12.972	3708	3711	3714	rBV	954	786	0.06%	0.007%
95	13.082	3742	3745	3749	rVB5	1197	714	0.05%	0.007%
96	13.368	3832	3834	3836	rBV2	525	243	0.02%	0.002%
97	13.728	3945	3946	3947	rBV2	458	133	0.01%	0.001%
98	13.885	3991	3995	3997	rBV4	656	452	0.03%	0.004%
99	14.024	4036	4038	4040	rVB2	823	329	0.02%	0.003%




Sum of corrected areas: 10915498

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027989.D
Acq On : 21 Sep 2022 02:39
Operator : SY/MD
Sample : N4674-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

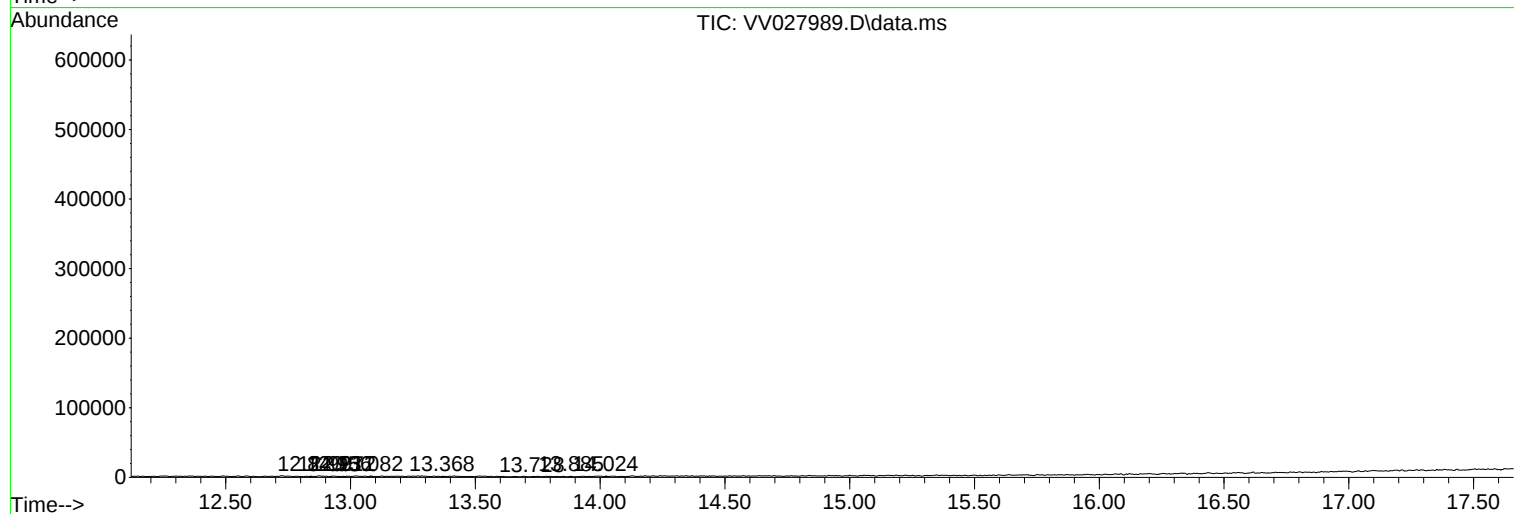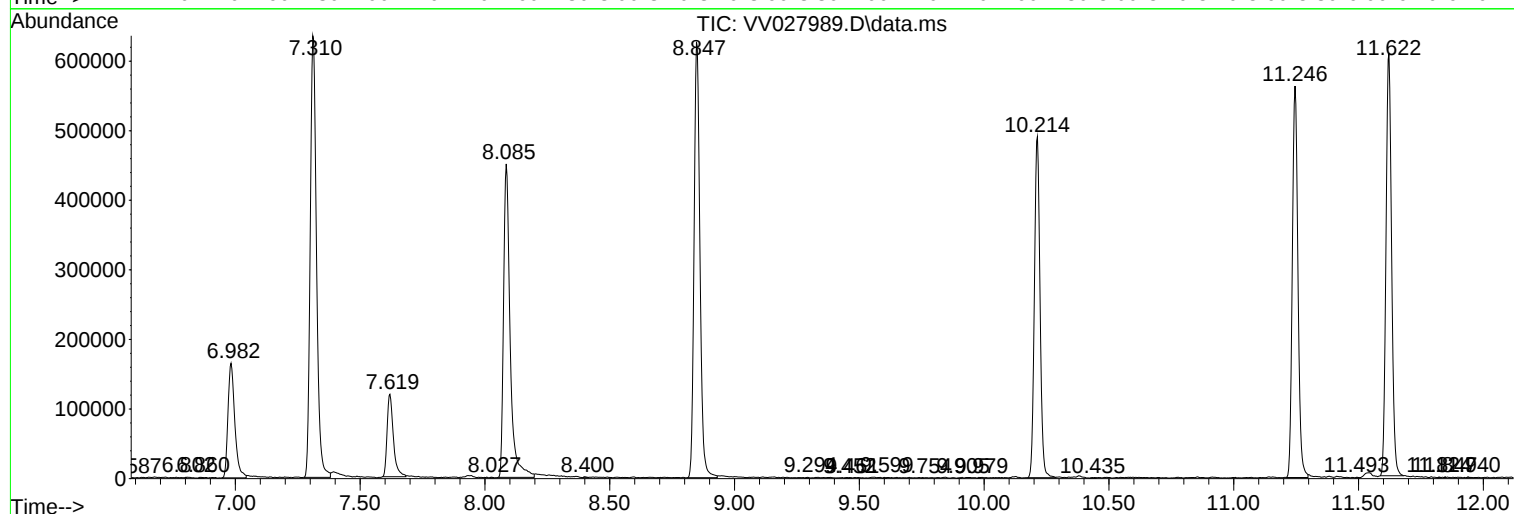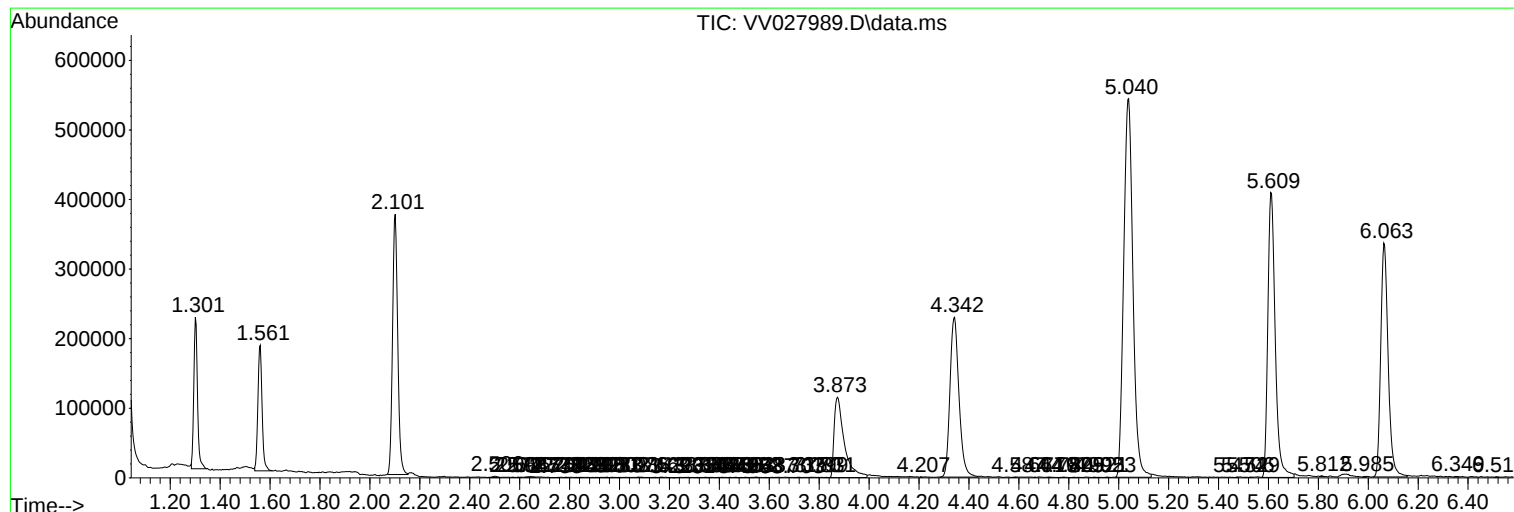

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027989.D
Acq On : 21 Sep 2022 02:39
Operator : SY/MD
Sample : N4674-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027989.D
Acq On : 21 Sep 2022 02:39
Operator : SY/MD
Sample : N4674-02
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 36 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E97

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------