

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027990.D
 Acq On : 21 Sep 2022 03:04
 Operator : SY/MD
 Sample : N4674-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027990.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	75	81	102	rVB	219985	237630	16.65%	2.199%
2	1.558	155	161	175	rVB	184105	208285	14.59%	1.928%
3	2.098	320	329	346	rBV	375878	541386	37.92%	5.010%
4	2.548	466	469	470	rBV	413	175	0.01%	0.002%
5	2.558	470	472	474	rBV2	411	222	0.02%	0.002%
6	2.619	489	491	493	rBV2	371	225	0.02%	0.002%
7	2.690	509	513	516	rBV2	523	383	0.03%	0.004%
8	2.828	551	556	557	rBV	320	219	0.02%	0.002%
9	2.905	578	580	583	rBV2	370	150	0.01%	0.001%
10	2.954	587	595	608	rBV6	1938	4179	0.29%	0.039%
11	2.999	608	609	611	rVV2	677	336	0.02%	0.003%
12	3.027	615	618	621	rVV2	737	402	0.03%	0.004%
13	3.040	621	622	625	rVB2	442	146	0.01%	0.001%
14	3.076	631	633	639	rVB2	571	522	0.04%	0.005%
15	3.114	641	645	649	rVB3	301	265	0.02%	0.002%
16	3.134	649	651	653	rBV2	220	125	0.01%	0.001%
17	3.153	655	657	662	rVB	680	400	0.03%	0.004%
18	3.175	662	664	671	rBV2	357	284	0.02%	0.003%
19	3.211	671	675	677	rBV3	504	390	0.03%	0.004%
20	3.259	687	690	692	rBV2	563	299	0.02%	0.003%
21	3.304	703	704	708	rVB	462	267	0.02%	0.002%
22	3.323	708	710	715	rVB2	420	287	0.02%	0.003%
23	3.349	715	718	720	rBV2	447	187	0.01%	0.002%
24	3.388	727	730	733	rVB2	393	229	0.02%	0.002%
25	3.433	740	744	748	rBV2	474	338	0.02%	0.003%
26	3.471	752	756	761	rBV2	424	486	0.03%	0.004%
27	3.503	761	766	769	rBV2	342	275	0.02%	0.003%
28	3.519	769	771	775	rBV2	334	269	0.02%	0.002%
29	3.613	795	800	805	rBV	305	370	0.03%	0.003%
30	3.674	816	819	821	rVV	343	202	0.01%	0.002%
31	3.683	821	822	827	rVV2	252	183	0.01%	0.002%
32	3.703	827	828	832	rVB	337	146	0.01%	0.001%
33	3.728	832	836	841	rBV2	383	264	0.02%	0.002%
34	3.757	841	845	849	rBB2	334	235	0.02%	0.002%
35	3.876	872	882	907	rBV	116718	317782	22.26%	2.941%
36	4.207	983	985	988	rBV4	729	356	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027990.D
 Acq On : 21 Sep 2022 03:04
 Operator : SY/MD
 Sample : N4674-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	4.339	1010	1026	1050	rBV	232481	576883	40.41%	5.339%
38	4.593	1102	1105	1108	rVB3	584	377	0.03%	0.003%
39	4.690	1132	1135	1136	rBV	389	185	0.01%	0.002%
40	4.709	1139	1141	1145	rVB2	827	509	0.04%	0.005%
41	4.735	1145	1149	1151	rBV	634	479	0.03%	0.004%
42	4.847	1182	1184	1185	rBV2	399	168	0.01%	0.002%
43	4.947	1213	1215	1219	rBV2	359	253	0.02%	0.002%
44	4.979	1224	1225	1227	rBV2	369	191	0.01%	0.002%
45	5.037	1227	1243	1269	rBV2	558170	1427567	100.00%	13.212%
46	5.278	1315	1318	1321	rBV4	685	450	0.03%	0.004%
47	5.423	1360	1363	1365	rVB3	874	500	0.04%	0.005%
48	5.468	1373	1377	1379	rVV5	499	284	0.02%	0.003%
49	5.481	1379	1381	1382	rBV	478	136	0.01%	0.001%
50	5.561	1402	1406	1407	rBV3	617	374	0.03%	0.003%
51	5.609	1410	1421	1454	rVV	377197	780199	54.65%	7.221%
52	5.982	1535	1537	1538	rBV2	361	186	0.01%	0.002%
53	6.063	1548	1562	1589	rBV	321800	654658	45.86%	6.059%
54	6.301	1635	1636	1637	rBV	547	190	0.01%	0.002%
55	6.346	1648	1650	1654	rVB3	770	432	0.03%	0.004%
56	6.362	1654	1655	1660	rBV4	874	874	0.06%	0.008%
57	6.410	1668	1670	1674	rBV4	836	517	0.04%	0.005%
58	6.445	1680	1681	1684	rBV3	664	364	0.03%	0.003%
59	6.513	1698	1702	1704	rBV4	1346	1133	0.08%	0.010%
60	6.590	1722	1726	1727	rBV2	756	504	0.04%	0.005%
61	6.815	1794	1796	1798	rBV2	723	403	0.03%	0.004%
62	6.924	1828	1830	1833	rBV	478	292	0.02%	0.003%
63	6.982	1837	1848	1872	rVV	168670	311263	21.80%	2.881%
64	7.310	1939	1950	1970	rBV	631821	1111567	77.86%	10.287%
65	7.619	2036	2046	2071	rBV	119111	216720	15.18%	2.006%
66	7.934	2138	2144	2153	rVB8	2408	4087	0.29%	0.038%
67	8.085	2181	2191	2223	rBV	450661	831069	58.22%	7.691%
68	8.400	2287	2289	2293	rBV5	1280	1045	0.07%	0.010%
69	8.741	2394	2395	2397	rVB	607	169	0.01%	0.002%
70	8.847	2417	2428	2454	rBV	603614	980280	68.67%	9.072%
71	9.410	2600	2603	2608	rBV4	1078	1084	0.08%	0.010%
72	9.500	2630	2631	2634	rVB2	488	235	0.02%	0.002%
73	9.516	2634	2636	2638	rBV4	725	251	0.02%	0.002%
74	9.529	2638	2640	2641	rBV3	792	266	0.02%	0.002%
75	9.635	2670	2673	2674	rBV	758	373	0.03%	0.003%
76	9.728	2697	2702	2705	rBV4	960	830	0.06%	0.008%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027990.D
 Acq On : 21 Sep 2022 03:04
 Operator : SY/MD
 Sample : N4674-03
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0E98

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.931	2761	2765	2766	rBV4	643	438	0.03%	0.004%
78	9.982	2778	2781	2784	rBV3	1090	764	0.05%	0.007%
79	10.066	2805	2807	2809	rBV2	771	284	0.02%	0.003%
80	10.114	2820	2822	2823	rBV2	1028	447	0.03%	0.004%
81	10.210	2840	2852	2873	rBV	483140	768710	53.85%	7.114%
82	10.683	2995	2999	3002	rBV2	924	806	0.06%	0.007%
83	10.866	3054	3056	3060	rBV4	616	372	0.03%	0.003%
84	11.098	3126	3128	3131	rBV	273	176	0.01%	0.002%
85	11.117	3131	3134	3136	rBV3	858	486	0.03%	0.004%
86	11.246	3163	3174	3198	rBV	548914	837967	58.70%	7.755%
87	11.622	3280	3291	3312	rVB	610600	961698	67.37%	8.900%
88	12.017	3411	3414	3418	rBV3	655	593	0.04%	0.005%
89	12.943	3700	3702	3707	rBV	846	713	0.05%	0.007%
90	13.050	3732	3735	3738	rVB3	1551	766	0.05%	0.007%
91	13.088	3744	3747	3750	rBV2	612	426	0.03%	0.004%
92	13.255	3794	3799	3801	rBV3	904	838	0.06%	0.008%
93	13.352	3826	3829	3830	rBV	846	430	0.03%	0.004%
94	13.619	3909	3912	3917	rBV5	1320	961	0.07%	0.009%
95	13.673	3927	3929	3931	rBV2	797	423	0.03%	0.004%
96	13.699	3935	3937	3939	rBV2	660	290	0.02%	0.003%
97	13.969	4019	4021	4023	rBV3	824	312	0.02%	0.003%
98	14.095	4058	4060	4063	rVB3	1101	460	0.03%	0.004%
99	14.342	4133	4137	4139	rBV3	1264	960	0.07%	0.009%
100	15.111	4374	4376	4378	rBV2	1168	555	0.04%	0.005%




Sum of corrected areas: 10805121

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027990.D
Acq On : 21 Sep 2022 03:04
Operator : SY/MD
Sample : N4674-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

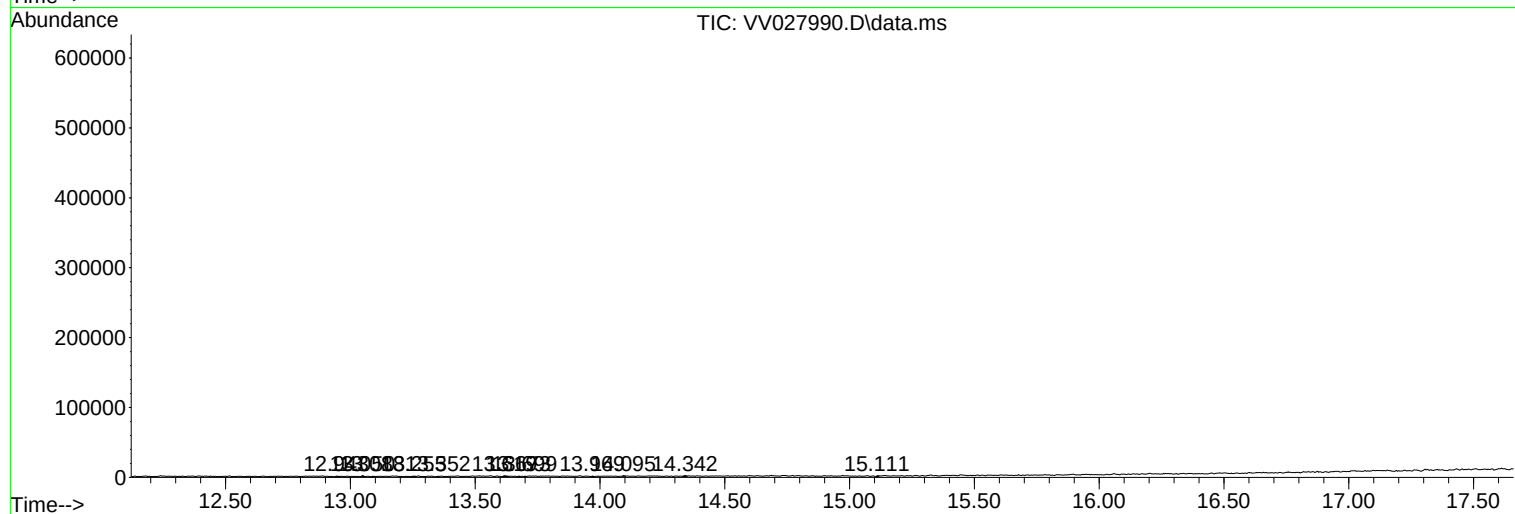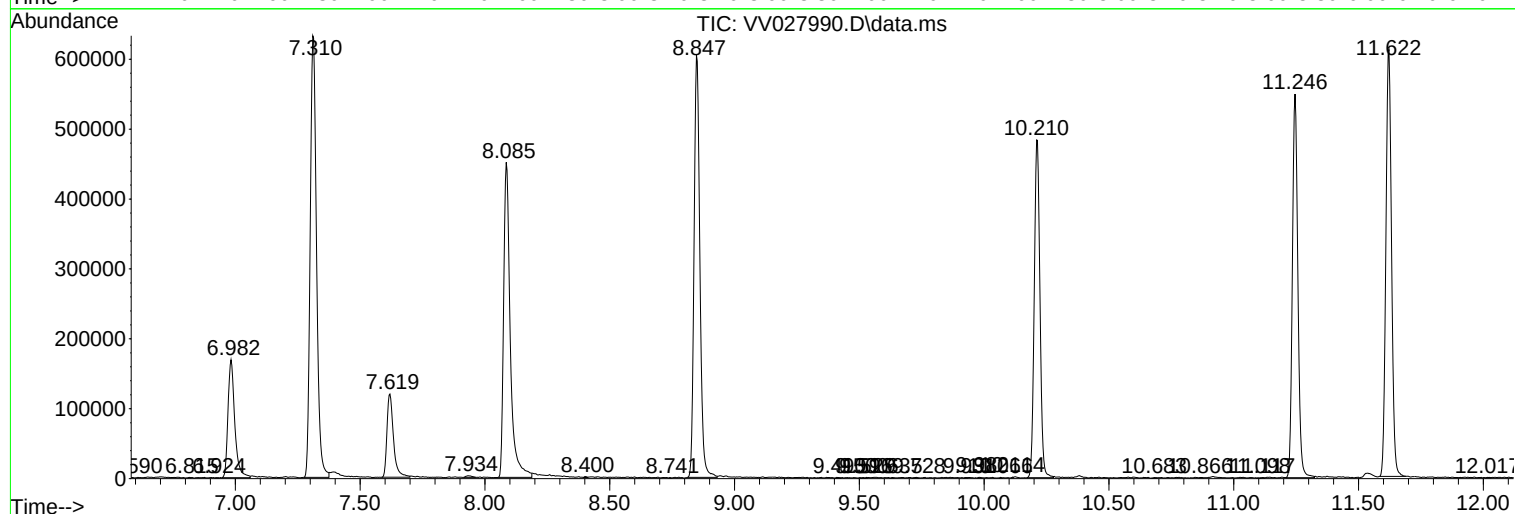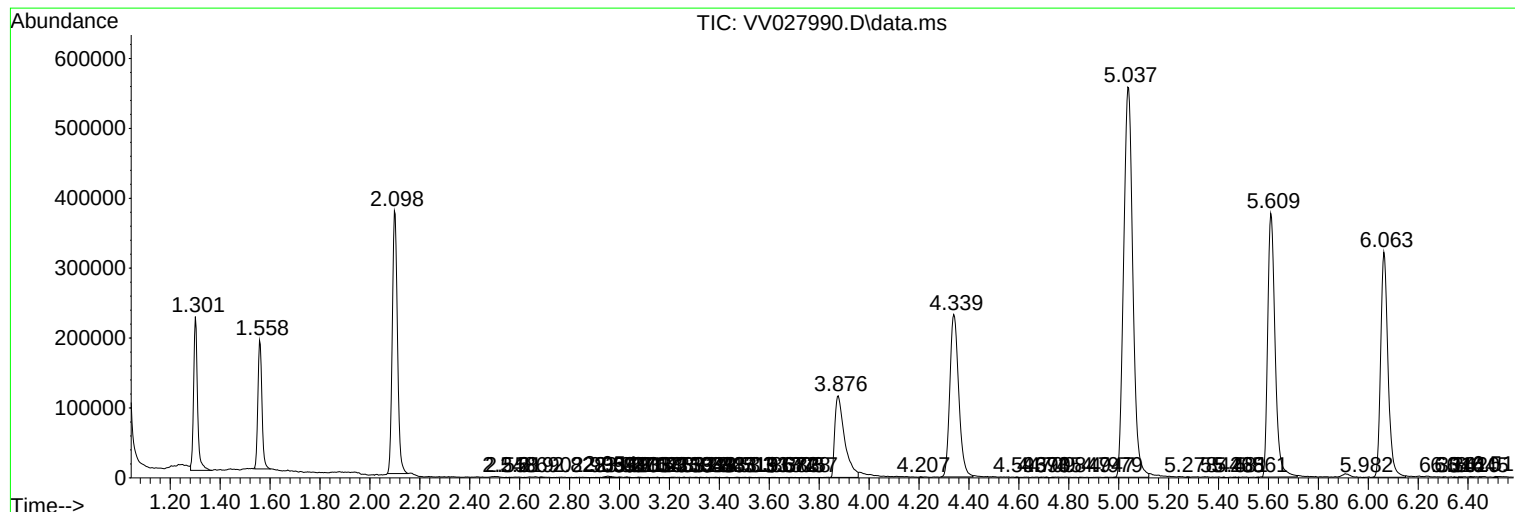

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027990.D
Acq On : 21 Sep 2022 03:04
Operator : SY/MD
Sample : N4674-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027990.D
Acq On : 21 Sep 2022 03:04
Operator : SY/MD
Sample : N4674-03
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 37 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0E98

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	#	RT	Resp	Conc
------------------	----	---------	-------	----------	---	----	------	------