

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027992.D
 Acq On : 21 Sep 2022 03:54
 Operator : SY/MD
 Sample : N4674-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027992.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	102	rVB	217653	229855	15.67%	2.095%
2	1.561	156	162	182	rVB	182285	212743	14.50%	1.939%
3	2.102	320	330	345	rBV	362588	527485	35.96%	4.807%
4	2.574	475	477	480	rBV	266	169	0.01%	0.002%
5	2.658	501	503	505	rBV2	694	324	0.02%	0.003%
6	2.706	516	518	521	rBV	379	254	0.02%	0.002%
7	2.754	528	533	534	rBV2	513	296	0.02%	0.003%
8	2.774	537	539	540	rVV	572	315	0.02%	0.003%
9	2.793	544	545	547	rVB	480	120	0.01%	0.001%
10	2.815	547	552	555	rBV3	516	417	0.03%	0.004%
11	2.831	555	557	561	rVB3	299	176	0.01%	0.002%
12	2.857	564	565	569	rVB2	343	171	0.01%	0.002%
13	2.886	569	574	576	rBV4	602	460	0.03%	0.004%
14	2.896	576	577	579	rVB4	307	94	0.01%	0.001%
15	2.915	579	583	584	rBV2	274	194	0.01%	0.002%
16	2.954	586	595	604	rBV6	1988	3707	0.25%	0.034%
17	3.040	620	622	626	rVB2	463	207	0.01%	0.002%
18	3.073	630	632	635	rVB3	549	242	0.02%	0.002%
19	3.089	635	637	639	rBV2	431	252	0.02%	0.002%
20	3.127	647	649	652	rBV3	325	209	0.01%	0.002%
21	3.163	659	660	663	rVB	208	104	0.01%	0.001%
22	3.179	663	665	670	rVB2	291	156	0.01%	0.001%
23	3.198	670	671	673	rBV2	237	87	0.01%	0.001%
24	3.237	679	683	686	rVB3	511	386	0.03%	0.004%
25	3.256	686	689	691	rBV	494	250	0.02%	0.002%
26	3.285	694	698	700	rBV2	341	237	0.02%	0.002%
27	3.307	703	705	706	rBV	359	142	0.01%	0.001%
28	3.330	710	712	716	rBV2	203	188	0.01%	0.002%
29	3.349	716	718	719	rBV	198	93	0.01%	0.001%
30	3.407	731	736	741	rBV3	405	326	0.02%	0.003%
31	3.442	745	747	750	rVB2	331	156	0.01%	0.001%
32	3.462	750	753	755	rVB2	544	304	0.02%	0.003%
33	3.481	758	759	761	rBV	169	75	0.01%	0.001%
34	3.497	761	764	766	rVB3	359	178	0.01%	0.002%
35	3.513	766	769	771	rBV	272	180	0.01%	0.002%
36	3.523	771	772	773	rBV	372	97	0.01%	0.001%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027992.D
 Acq On : 21 Sep 2022 03:54
 Operator : SY/MD
 Sample : N4674-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	3.564	782	785	787	rVB	298	173	0.01%	0.002%
38	3.574	787	788	792	rVB2	264	127	0.01%	0.001%
39	3.593	792	794	795	rBV2	205	100	0.01%	0.001%
40	3.603	795	797	798	rBV	205	67	0.00%	0.001%
41	3.629	803	805	808	rVB	470	252	0.02%	0.002%
42	3.664	813	816	817	rBV	445	220	0.01%	0.002%
43	3.696	824	826	828	rBB2	302	125	0.01%	0.001%
44	3.716	828	832	836	rVB3	401	324	0.02%	0.003%
45	3.738	836	839	842	rBV	262	166	0.01%	0.002%
46	3.790	854	855	858	rBV	161	88	0.01%	0.001%
47	3.806	858	860	863	rBV	308	197	0.01%	0.002%
48	3.876	873	882	930	rBV	116227	344481	23.49%	3.139%
49	4.269	1003	1004	1007	rBV	612	392	0.03%	0.004%
50	4.339	1012	1026	1050	rVV2	236324	579833	39.53%	5.284%
51	4.580	1100	1101	1104	rBV2	589	309	0.02%	0.003%
52	4.593	1104	1105	1106	rBV	469	135	0.01%	0.001%
53	4.699	1136	1138	1141	rVB2	448	216	0.01%	0.002%
54	4.716	1141	1143	1146	rBV2	447	247	0.02%	0.002%
55	4.735	1146	1149	1151	rVV2	446	267	0.02%	0.002%
56	4.757	1155	1156	1158	rVB2	462	115	0.01%	0.001%
57	4.806	1169	1171	1172	rBV2	534	175	0.01%	0.002%
58	4.863	1187	1189	1191	rBV2	434	213	0.01%	0.002%
59	4.896	1196	1199	1200	rBV2	421	219	0.01%	0.002%
60	4.905	1200	1202	1203	rBV	284	89	0.01%	0.001%
61	4.915	1203	1205	1208	rBV	513	318	0.02%	0.003%
62	4.957	1215	1218	1219	rBV2	372	222	0.02%	0.002%
63	5.040	1227	1244	1270	rBV2	572526	1466780	100.00%	13.367%
64	5.346	1337	1339	1342	rBV4	674	474	0.03%	0.004%
65	5.490	1382	1384	1386	rVB2	962	418	0.03%	0.004%
66	5.503	1386	1388	1392	rBV5	1185	727	0.05%	0.007%
67	5.609	1409	1421	1452	rBV	407720	845106	57.62%	7.701%
68	6.063	1550	1562	1584	rBV	334006	681448	46.46%	6.210%
69	6.510	1698	1701	1702	rBV	743	467	0.03%	0.004%
70	6.642	1739	1742	1744	rBV3	1102	832	0.06%	0.008%
71	6.667	1749	1750	1751	rBV	787	195	0.01%	0.002%
72	6.982	1837	1848	1874	rBV	161343	303159	20.67%	2.763%
73	7.310	1939	1950	1969	rBV	629538	1096994	74.79%	9.997%
74	7.619	2036	2046	2064	rBV	118270	207362	14.14%	1.890%
75	8.085	2181	2191	2222	rBV	451439	827863	56.44%	7.544%
76	8.847	2418	2428	2457	rBV	634943	1020616	69.58%	9.301%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027992.D
 Acq On : 21 Sep 2022 03:54
 Operator : SY/MD
 Sample : N4674-05
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA1

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.204	2536	2539	2542	rBV3	840	508	0.03%	0.005%
78	9.355	2584	2586	2587	rBV	553	207	0.01%	0.002%
79	9.384	2592	2595	2596	rBV	982	587	0.04%	0.005%
80	9.632	2670	2672	2675	rBV4	588	374	0.03%	0.003%
81	9.751	2705	2709	2711	rBV2	895	774	0.05%	0.007%
82	9.818	2728	2730	2731	rBV	690	192	0.01%	0.002%
83	9.902	2754	2756	2758	rBV2	321	127	0.01%	0.001%
84	10.027	2793	2795	2799	rBV3	746	525	0.04%	0.005%
85	10.092	2810	2815	2816	rBV2	772	556	0.04%	0.005%
86	10.214	2840	2853	2873	rBV	484300	767059	52.30%	6.990%
87	10.667	2989	2994	2999	rVB5	513	545	0.04%	0.005%
88	11.146	3141	3143	3145	rBV2	1099	562	0.04%	0.005%
89	11.246	3163	3174	3193	rBV	570480	875387	59.68%	7.977%
90	11.622	3279	3291	3314	rBV	617673	959967	65.45%	8.748%
91	12.281	3494	3496	3498	rVB3	790	267	0.02%	0.002%
92	12.297	3498	3501	3504	rBV4	873	775	0.05%	0.007%
93	12.429	3541	3542	3546	rBV3	661	411	0.03%	0.004%
94	12.561	3581	3583	3585	rBV2	516	255	0.02%	0.002%
95	12.696	3624	3625	3629	rVB4	793	340	0.02%	0.003%
96	13.072	3739	3742	3744	rBV2	499	339	0.02%	0.003%
97	13.185	3775	3777	3778	rBV	573	203	0.01%	0.002%
98	13.921	4004	4006	4007	rBV	1039	373	0.03%	0.003%
99	13.966	4019	4020	4025	rVB3	1076	449	0.03%	0.004%
100	14.368	4142	4145	4146	rBV	873	498	0.03%	0.005%




Sum of corrected areas: 10973440

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027992.D
Acq On : 21 Sep 2022 03:54
Operator : SY/MD
Sample : N4674-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

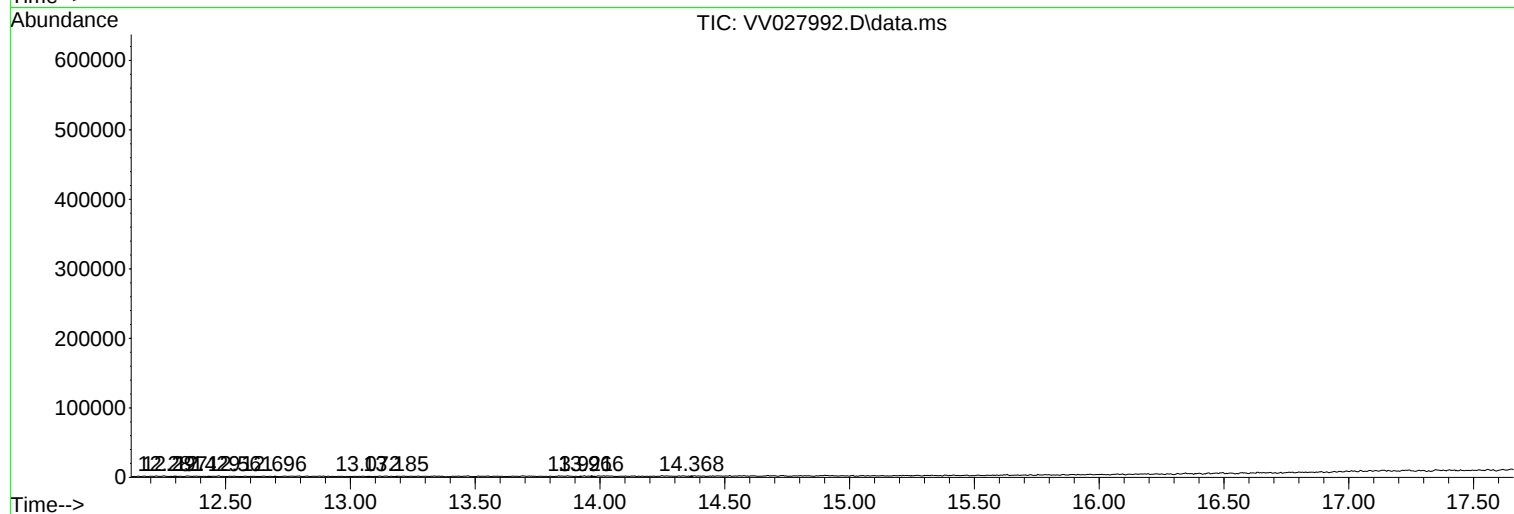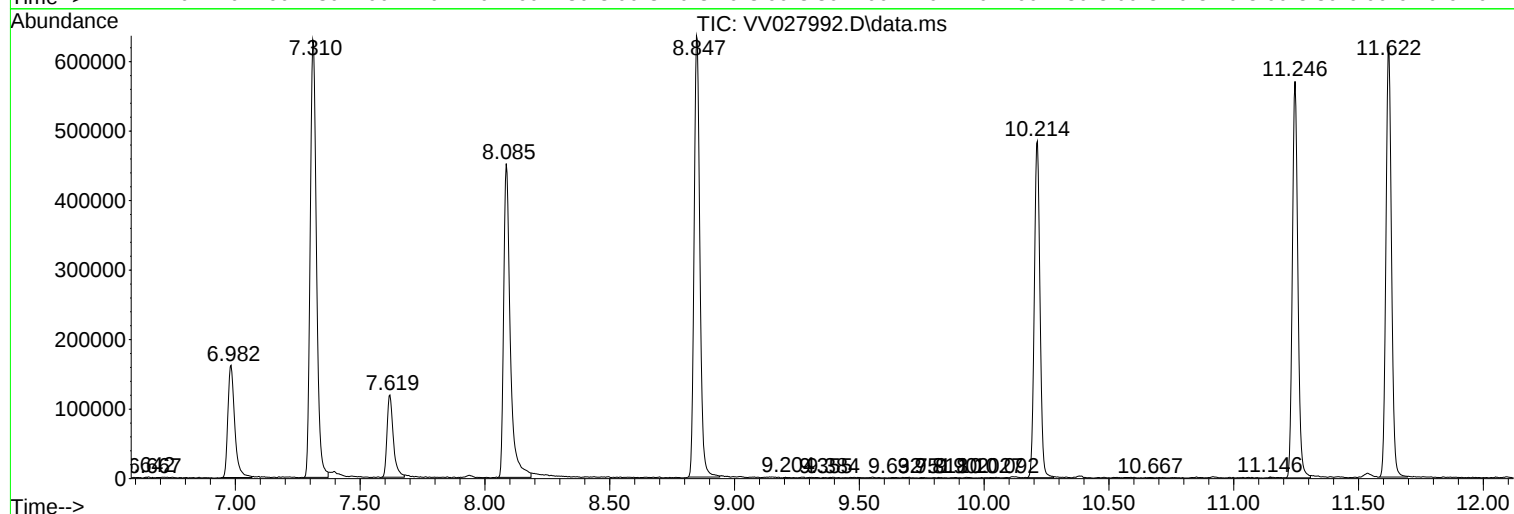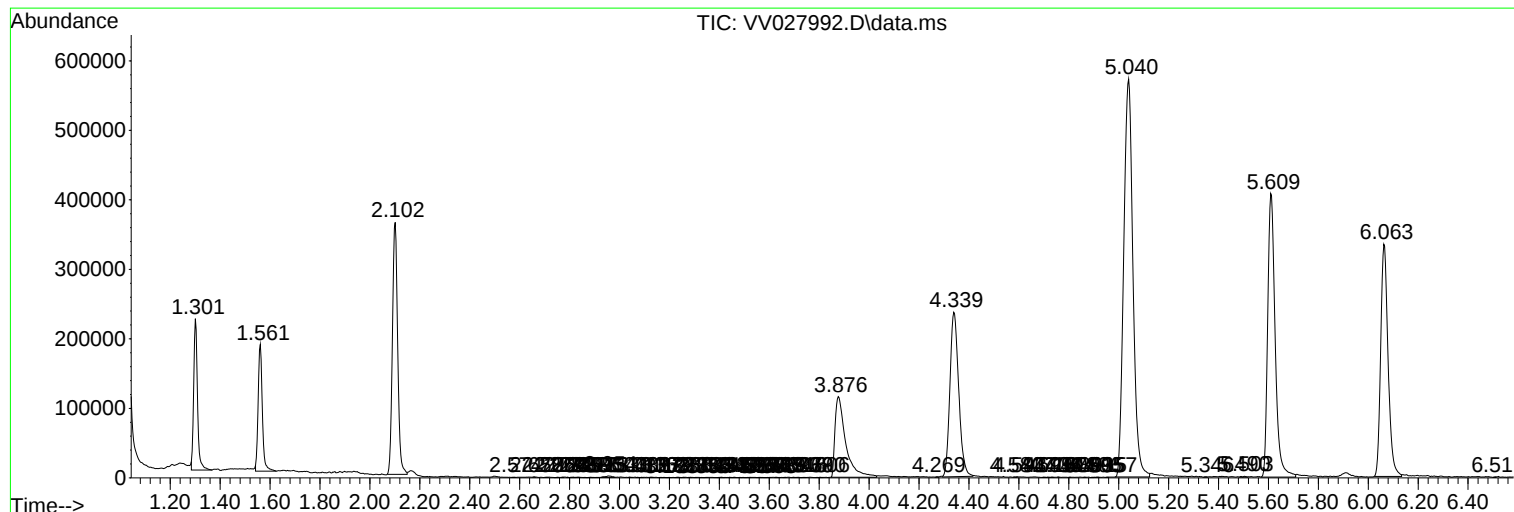

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027992.D
Acq On : 21 Sep 2022 03:54
Operator : SY/MD
Sample : N4674-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027992.D
Acq On : 21 Sep 2022 03:54
Operator : SY/MD
Sample : N4674-05
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 39 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA1

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc