

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027993.D
 Acq On : 21 Sep 2022 04:18
 Operator : SY/MD
 Sample : N4674-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027993.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	211829	221894	16.49%	2.142%
2	1.561	156	162	177	rVB	176989	200176	14.88%	1.932%
3	2.101	321	330	346	rVB	352882	509195	37.85%	4.915%
4	2.400	419	423	428	rVB6	445	441	0.03%	0.004%
5	2.484	446	449	451	rBV3	514	373	0.03%	0.004%
6	2.754	531	533	540	rBV2	473	640	0.05%	0.006%
7	2.818	550	553	556	rBV2	594	480	0.04%	0.005%
8	2.960	595	597	600	rVB	559	190	0.01%	0.002%
9	2.989	603	606	607	rBV	261	137	0.01%	0.001%
10	3.079	632	634	636	rBV	319	137	0.01%	0.001%
11	3.137	649	652	653	rBV	315	138	0.01%	0.001%
12	3.185	665	667	670	rBV2	319	179	0.01%	0.002%
13	3.223	677	679	682	rBV2	336	192	0.01%	0.002%
14	3.272	687	694	700	rBV2	506	552	0.04%	0.005%
15	3.317	702	708	710	rBV2	563	291	0.02%	0.003%
16	3.336	710	714	716	rBV2	258	176	0.01%	0.002%
17	3.355	716	720	722	rBV	291	140	0.01%	0.001%
18	3.375	724	726	729	rBV	331	197	0.01%	0.002%
19	3.391	729	731	734	rBV	299	163	0.01%	0.002%
20	3.503	760	766	771	rVB4	422	383	0.03%	0.004%
21	3.548	778	780	781	rBV	462	185	0.01%	0.002%
22	3.584	788	791	794	rBV	231	135	0.01%	0.001%
23	3.606	794	798	799	rBV2	429	288	0.02%	0.003%
24	3.680	819	821	826	rVB2	264	186	0.01%	0.002%
25	3.719	831	833	835	rBV2	276	143	0.01%	0.001%
26	3.802	856	859	861	rBV2	403	247	0.02%	0.002%
27	3.876	872	882	915	rBV	108849	310222	23.06%	2.994%
28	4.339	1012	1026	1054	rBV2	219739	543144	40.37%	5.242%
29	4.561	1093	1095	1098	rBV4	298	194	0.01%	0.002%
30	4.609	1108	1110	1115	rVB3	832	518	0.04%	0.005%
31	4.635	1115	1118	1119	rBV	354	146	0.01%	0.001%
32	4.719	1140	1144	1150	rBV3	368	444	0.03%	0.004%
33	4.773	1159	1161	1164	rBV	328	177	0.01%	0.002%
34	4.789	1164	1166	1168	rBV	359	189	0.01%	0.002%
35	4.825	1172	1177	1181	rVB3	469	531	0.04%	0.005%
36	4.847	1181	1184	1186	rBV	362	205	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027993.D
 Acq On : 21 Sep 2022 04:18
 Operator : SY/MD
 Sample : N4674-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	4.960	1214	1219	1221	rBV3	460	306	0.02%	0.003%
38	5.040	1226	1244	1282	rBV2	522101	1345324	100.00%	12.984%
39	5.349	1336	1340	1342	rBV4	581	478	0.04%	0.005%
40	5.362	1342	1344	1348	rVV3	604	322	0.02%	0.003%
41	5.384	1348	1351	1355	rVB3	605	435	0.03%	0.004%
42	5.529	1394	1396	1399	rBV2	326	176	0.01%	0.002%
43	5.548	1400	1402	1404	rVB	565	202	0.02%	0.002%
44	5.609	1404	1421	1449	rBV	400690	809525	60.17%	7.813%
45	5.863	1496	1500	1502	rVV4	668	401	0.03%	0.004%
46	5.908	1505	1514	1530	rVB7	3923	8638	0.64%	0.083%
47	6.063	1549	1562	1583	rBV	291100	602388	44.78%	5.814%
48	6.284	1629	1631	1633	rVB2	429	181	0.01%	0.002%
49	6.342	1645	1649	1651	rVB2	304	195	0.01%	0.002%
50	6.362	1652	1655	1656	rVV	372	175	0.01%	0.002%
51	6.374	1656	1659	1660	rVV3	628	411	0.03%	0.004%
52	6.397	1663	1666	1670	rVB3	732	404	0.03%	0.004%
53	6.461	1684	1686	1688	rVB	295	154	0.01%	0.001%
54	6.493	1694	1696	1703	rVB3	725	585	0.04%	0.006%
55	6.526	1703	1706	1707	rBV	368	158	0.01%	0.002%
56	6.561	1715	1717	1720	rVB	487	169	0.01%	0.002%
57	6.574	1720	1721	1726	rVB2	570	338	0.03%	0.003%
58	6.596	1726	1728	1730	rBV2	505	332	0.02%	0.003%
59	6.628	1735	1738	1741	rBV3	471	352	0.03%	0.003%
60	6.693	1756	1758	1763	rBV2	935	746	0.06%	0.007%
61	6.776	1781	1784	1786	rVB3	577	296	0.02%	0.003%
62	6.857	1807	1809	1811	rVB2	490	152	0.01%	0.001%
63	6.870	1811	1813	1816	rVB	319	141	0.01%	0.001%
64	6.924	1828	1830	1832	rVB	367	189	0.01%	0.002%
65	6.937	1832	1834	1836	rBV	422	184	0.01%	0.002%
66	6.982	1836	1848	1870	rBV	149827	279321	20.76%	2.696%
67	7.310	1938	1950	1971	rBV	579482	1021035	75.90%	9.855%
68	7.619	2035	2046	2066	rBV	109569	194381	14.45%	1.876%
69	7.834	2112	2113	2114	rBV	573	169	0.01%	0.002%
70	7.934	2136	2144	2145	rBV4	2738	3268	0.24%	0.032%
71	8.085	2181	2191	2222	rBV	394058	732681	54.46%	7.072%
72	8.513	2322	2324	2326	rBV3	551	306	0.02%	0.003%
73	8.789	2407	2410	2412	rBV2	689	378	0.03%	0.004%
74	8.802	2412	2414	2417	rBV4	591	330	0.02%	0.003%
75	8.847	2417	2428	2456	rBV	611408	995949	74.03%	9.612%
76	9.191	2533	2535	2536	rBV2	746	273	0.02%	0.003%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027993.D
 Acq On : 21 Sep 2022 04:18
 Operator : SY/MD
 Sample : N4674-06
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 40 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA3

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	9.278	2559	2562	2564	rBV4	957	708	0.05%	0.007%
78	9.307	2569	2571	2574	rVV	788	341	0.03%	0.003%
79	9.471	2620	2622	2625	rBV3	818	457	0.03%	0.004%
80	9.712	2695	2697	2701	rVB4	889	440	0.03%	0.004%
81	9.757	2707	2711	2713	rBV2	713	549	0.04%	0.005%
82	9.879	2748	2749	2750	rBV2	405	137	0.01%	0.001%
83	9.918	2758	2761	2764	rBV3	756	624	0.05%	0.006%
84	10.005	2784	2788	2790	rBV2	868	592	0.04%	0.006%
85	10.017	2790	2792	2796	rVV4	738	607	0.05%	0.006%
86	10.214	2839	2853	2871	rBV	468827	741030	55.08%	7.152%
87	10.381	2898	2905	2910	rBV5	3040	4371	0.32%	0.042%
88	10.506	2941	2944	2947	rBV4	986	776	0.06%	0.007%
89	10.551	2954	2958	2961	rBV3	783	686	0.05%	0.007%
90	11.030	3104	3107	3109	rBV4	1071	735	0.05%	0.007%
91	11.246	3162	3174	3192	rBV	570746	892257	66.32%	8.612%
92	11.622	3280	3291	3313	rVB	581723	919238	68.33%	8.872%
93	11.840	3357	3359	3360	rBV	563	323	0.02%	0.003%
94	11.898	3375	3377	3379	rBV3	660	302	0.02%	0.003%
95	11.992	3404	3406	3409	rBV3	770	403	0.03%	0.004%
96	12.181	3463	3465	3466	rBV	418	154	0.01%	0.001%
97	12.673	3616	3618	3621	rVB2	682	282	0.02%	0.003%
98	12.705	3627	3628	3633	rBV4	616	485	0.04%	0.005%
99	13.156	3766	3768	3770	rBV2	1269	717	0.05%	0.007%
100	14.082	4054	4056	4057	rBV	811	347	0.03%	0.003%




Sum of corrected areas: 10361037

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027993.D
Acq On : 21 Sep 2022 04:18
Operator : SY/MD
Sample : N4674-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

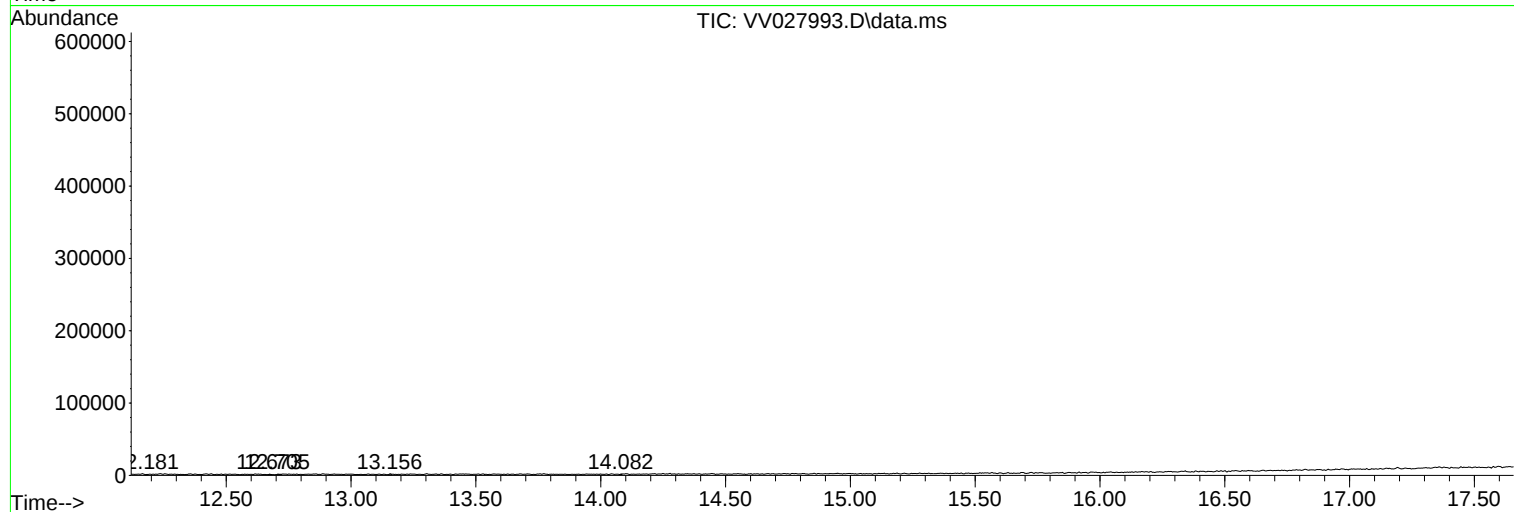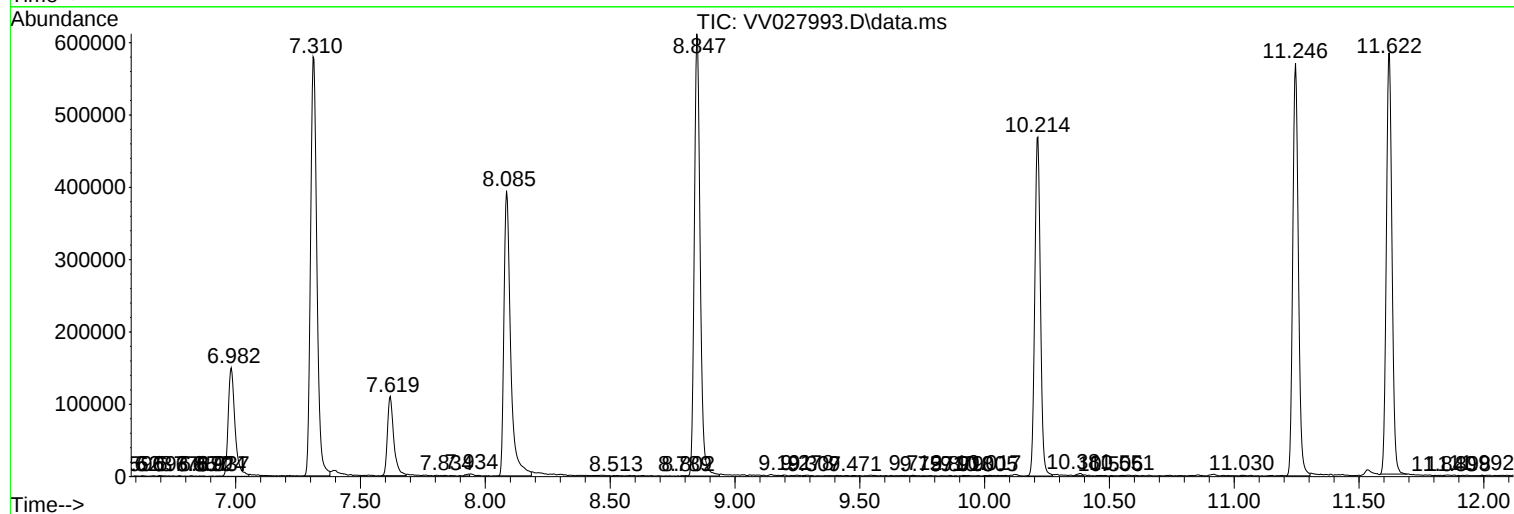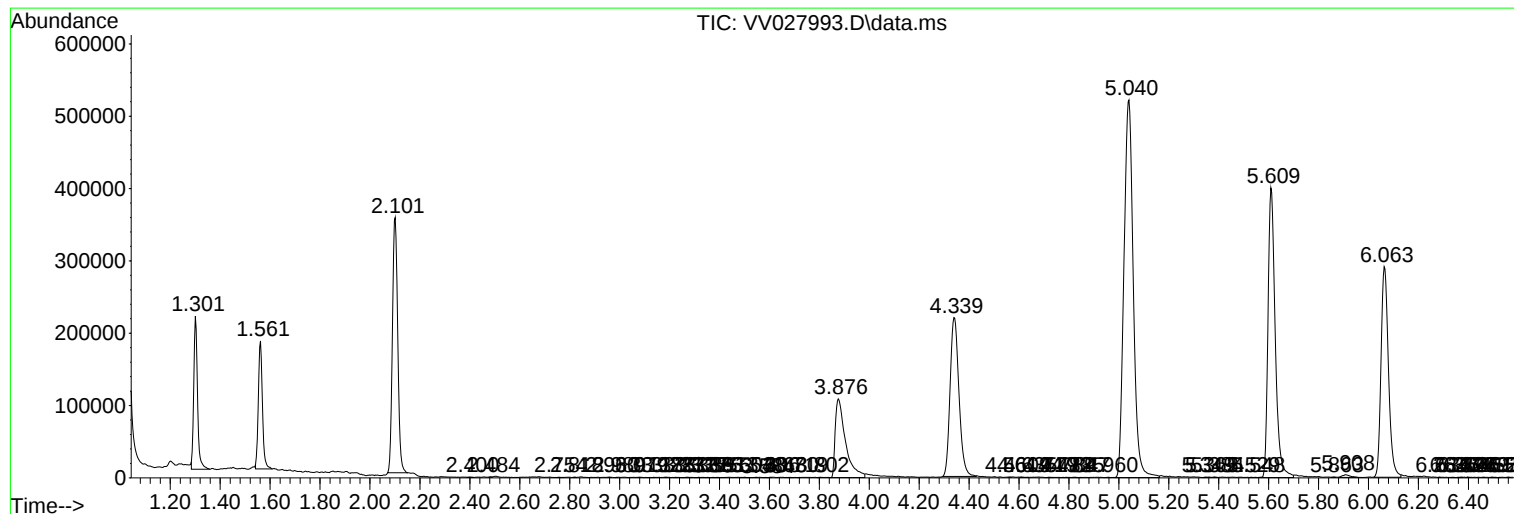

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027993.D
Acq On : 21 Sep 2022 04:18
Operator : SY/MD
Sample : N4674-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027993.D
Acq On : 21 Sep 2022 04:18
Operator : SY/MD
Sample : N4674-06
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 40 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA3

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--			
					#	RT	Resp	Conc