

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027994.D
 Acq On : 21 Sep 2022 04:43
 Operator : SY/MD
 Sample : N4674-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

Signal : TIC: VV027994.D\data.ms

peak #	R.T. min	first scan	max scan	last scan	PK TY	peak height	corr. area	corr. % max.	% of total
1	1.301	76	81	99	rVB	210073	221078	15.14%	2.028%
2	1.558	155	161	179	rVB	177563	204047	13.97%	1.871%
3	2.101	320	330	359	rVB	353103	523879	35.87%	4.805%
4	2.590	479	482	483	rBV	802	347	0.02%	0.003%
5	2.712	516	520	522	rVB4	1020	679	0.05%	0.006%
6	2.873	567	570	573	rBV2	782	621	0.04%	0.006%
7	2.896	573	577	579	rVB4	826	573	0.04%	0.005%
8	3.002	607	610	611	rBV2	823	278	0.02%	0.003%
9	3.063	627	629	630	rBV	680	313	0.02%	0.003%
10	3.089	635	637	639	rBV	789	363	0.02%	0.003%
11	3.195	668	670	672	rBV2	543	302	0.02%	0.003%
12	3.230	679	681	686	rVB4	744	329	0.02%	0.003%
13	3.291	698	700	706	rVB3	640	416	0.03%	0.004%
14	3.330	709	712	714	rBV3	838	555	0.04%	0.005%
15	3.404	733	735	736	rBV2	553	253	0.02%	0.002%
16	3.516	767	770	771	rBV2	427	263	0.02%	0.002%
17	3.590	790	793	798	rVV5	696	671	0.05%	0.006%
18	3.629	803	805	809	rVV2	636	458	0.03%	0.004%
19	3.716	829	832	834	rVB2	751	514	0.04%	0.005%
20	3.735	834	838	844	rBV4	643	723	0.05%	0.007%
21	3.818	861	864	865	rBV	873	489	0.03%	0.004%
22	3.873	871	881	915	rBV	126883	358777	24.57%	3.290%
23	4.339	1012	1026	1054	rVB	238796	582046	39.86%	5.338%
24	4.529	1082	1085	1087	rBV3	1127	829	0.06%	0.008%
25	4.625	1112	1115	1117	rBV4	1150	581	0.04%	0.005%
26	4.722	1143	1145	1148	rBV3	715	412	0.03%	0.004%
27	4.738	1148	1150	1152	rVB	1075	373	0.03%	0.003%
28	4.806	1168	1171	1173	rBV2	783	440	0.03%	0.004%
29	4.847	1182	1184	1188	rBV2	518	489	0.03%	0.004%
30	4.908	1201	1203	1206	rVB3	935	397	0.03%	0.004%
31	5.040	1227	1244	1275	rBV2	566331	1460354	100.00%	13.393%
32	5.323	1330	1332	1335	rBV3	1061	459	0.03%	0.004%
33	5.609	1410	1421	1447	rBV	412434	837636	57.36%	7.682%
34	5.863	1498	1500	1504	rBV3	750	488	0.03%	0.004%
35	5.915	1504	1516	1530	rVV7	14427	32326	2.21%	0.296%
36	6.063	1548	1562	1593	rBV2	326059	676555	46.33%	6.205%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027994.D
 Acq On : 21 Sep 2022 04:43
 Operator : SY/MD
 Sample : N4674-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

37	6.371	1654	1658	1659	rBV4	764	549	0.04%	0.005%
38	6.381	1659	1661	1664	rVB3	1244	581	0.04%	0.005%
39	6.449	1679	1682	1683	rBV2	606	282	0.02%	0.003%
40	6.503	1696	1699	1700	rBV2	941	448	0.03%	0.004%
41	6.529	1705	1707	1710	rBV3	450	305	0.02%	0.003%
42	6.622	1734	1736	1738	rBV2	933	488	0.03%	0.004%
43	6.773	1781	1783	1788	rVB5	903	692	0.05%	0.006%
44	6.825	1797	1799	1800	rBV	650	286	0.02%	0.003%
45	6.905	1817	1824	1827	rBV4	990	1010	0.07%	0.009%
46	6.937	1833	1834	1837	rBV3	554	308	0.02%	0.003%
47	6.982	1837	1848	1869	rBV2	157775	297057	20.34%	2.724%
48	7.310	1935	1950	1970	rBV	584131	1035821	70.93%	9.500%
49	7.551	2023	2025	2026	rBV2	598	248	0.02%	0.002%
50	7.619	2034	2046	2072	rBV	106892	194858	13.34%	1.787%
51	7.793	2098	2100	2104	rVB2	820	427	0.03%	0.004%
52	7.850	2116	2118	2124	rVB5	1059	685	0.05%	0.006%
53	7.876	2124	2126	2127	rBV	629	293	0.02%	0.003%
54	7.937	2140	2145	2147	rBV4	1613	1668	0.11%	0.015%
55	7.989	2159	2161	2163	rBV	633	293	0.02%	0.003%
56	8.024	2170	2172	2174	rVB3	689	264	0.02%	0.002%
57	8.085	2181	2191	2223	rBV	438894	808158	55.34%	7.412%
58	8.641	2362	2364	2365	rBV2	672	374	0.03%	0.003%
59	8.677	2372	2375	2376	rBV2	957	466	0.03%	0.004%
60	8.741	2391	2395	2400	rBV5	830	1078	0.07%	0.010%
61	8.847	2416	2428	2450	rBV	627420	1030928	70.59%	9.455%
62	9.227	2541	2546	2548	rBV4	1201	1003	0.07%	0.009%
63	9.272	2556	2560	2565	rVB5	1237	1079	0.07%	0.010%
64	9.490	2624	2628	2633	rVB3	768	536	0.04%	0.005%
65	9.738	2701	2705	2706	rBV	693	342	0.02%	0.003%
66	9.747	2706	2708	2711	rBV3	802	468	0.03%	0.004%
67	9.844	2734	2738	2743	rVB6	752	553	0.04%	0.005%
68	9.902	2752	2756	2758	rBV3	734	521	0.04%	0.005%
69	9.940	2764	2768	2772	rBV3	1034	1125	0.08%	0.010%
70	9.973	2776	2778	2780	rBV2	661	380	0.03%	0.003%
71	10.063	2801	2806	2809	rBV3	666	649	0.04%	0.006%
72	10.079	2809	2811	2813	rBV3	685	398	0.03%	0.004%
73	10.210	2841	2852	2874	rBV	474996	750414	51.39%	6.882%
74	10.468	2929	2932	2936	rBV3	784	614	0.04%	0.006%
75	10.484	2936	2937	2941	rBV3	510	355	0.02%	0.003%
76	10.526	2948	2950	2951	rBV	644	249	0.02%	0.002%

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
 Data File : VV027994.D
 Acq On : 21 Sep 2022 04:43
 Operator : SY/MD
 Sample : N4674-07
 Misc : 5.0mL/MSVOA_V/WATER
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 MSVOA_V
 ClientSampleId :
 C0EA4

Integration Parameters: LSCINT.P

Integrator: RTE

Smoothing : OFF

Filtering: 5

Sampling : 1

Min Area: 0 % of largest Peak

Start Thrs: 0.2

Max Peaks: 100

Stop Thrs : 0

Peak Location: TOP

If leading or trailing edge < 100 prefer < Baseline drop else tangent >

Peak separation: 5

Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
 Title : VOC Analysis

77	10.715	3005	3009	3011	rBV4	973	622	0.04%	0.006%
78	10.818	3039	3041	3044	rBV4	740	325	0.02%	0.003%
79	10.834	3044	3046	3048	rVB2	769	289	0.02%	0.003%
80	10.857	3048	3053	3056	rBV5	720	763	0.05%	0.007%
81	10.982	3088	3092	3095	rBV2	644	398	0.03%	0.004%
82	11.001	3095	3098	3099	rVB2	492	294	0.02%	0.003%
83	11.111	3129	3132	3133	rBV2	594	270	0.02%	0.002%
84	11.136	3136	3140	3142	rBV2	760	618	0.04%	0.006%
85	11.201	3158	3160	3162	rBV2	775	445	0.03%	0.004%
86	11.246	3162	3174	3204	rVV	576188	887984	60.81%	8.144%
87	11.535	3254	3264	3276	rVV6	8611	18694	1.28%	0.171%
88	11.619	3280	3290	3314	rVB	586214	939279	64.32%	8.614%
89	11.944	3389	3391	3396	rVB4	753	505	0.03%	0.005%
90	12.014	3409	3413	3415	rBV4	1037	810	0.06%	0.007%
91	12.040	3419	3421	3426	rBV4	1013	887	0.06%	0.008%
92	12.226	3476	3479	3482	rBV2	1072	840	0.06%	0.008%
93	12.503	3563	3565	3568	rBV2	634	422	0.03%	0.004%
94	13.140	3761	3763	3765	rBV3	868	471	0.03%	0.004%
95	13.371	3831	3835	3837	rBV5	920	713	0.05%	0.007%
96	13.435	3850	3855	3862	rBV6	964	1407	0.10%	0.013%
97	13.471	3862	3866	3868	rBV5	861	651	0.04%	0.006%
98	13.722	3940	3944	3945	rBV3	591	462	0.03%	0.004%
99	13.963	4017	4019	4022	rBV2	1125	472	0.03%	0.004%
100	14.355	4138	4141	4142	rBV2	776	449	0.03%	0.004%




Sum of corrected areas: 10903636

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027994.D
Acq On : 21 Sep 2022 04:43
Operator : SY/MD
Sample : N4674-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

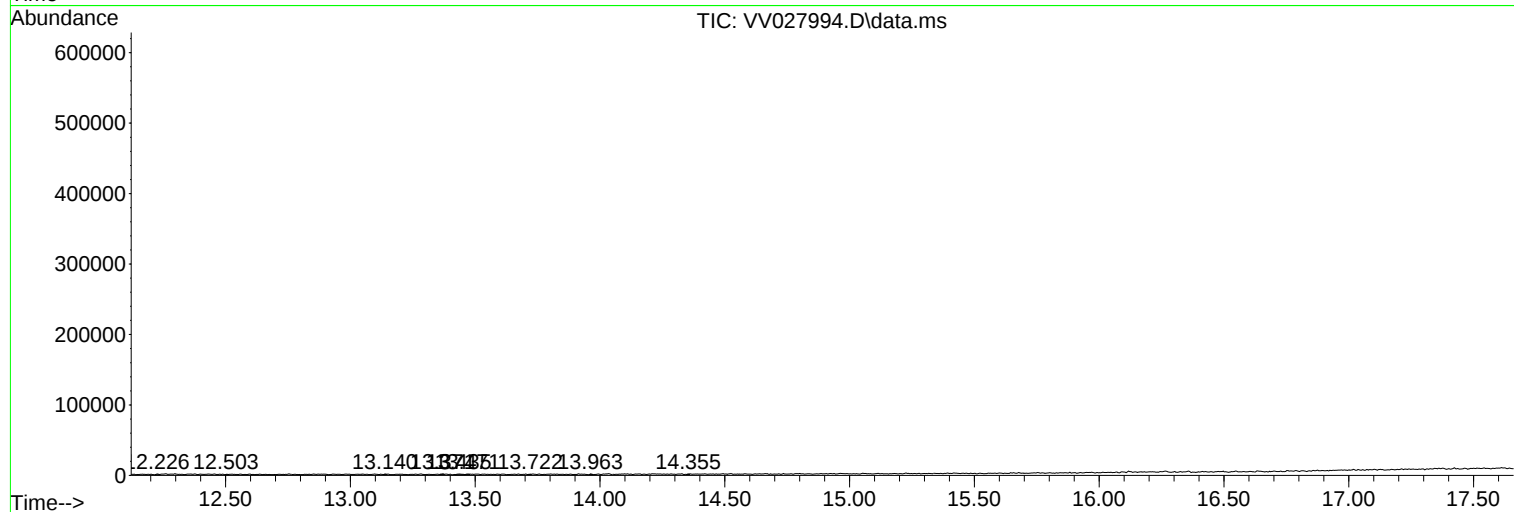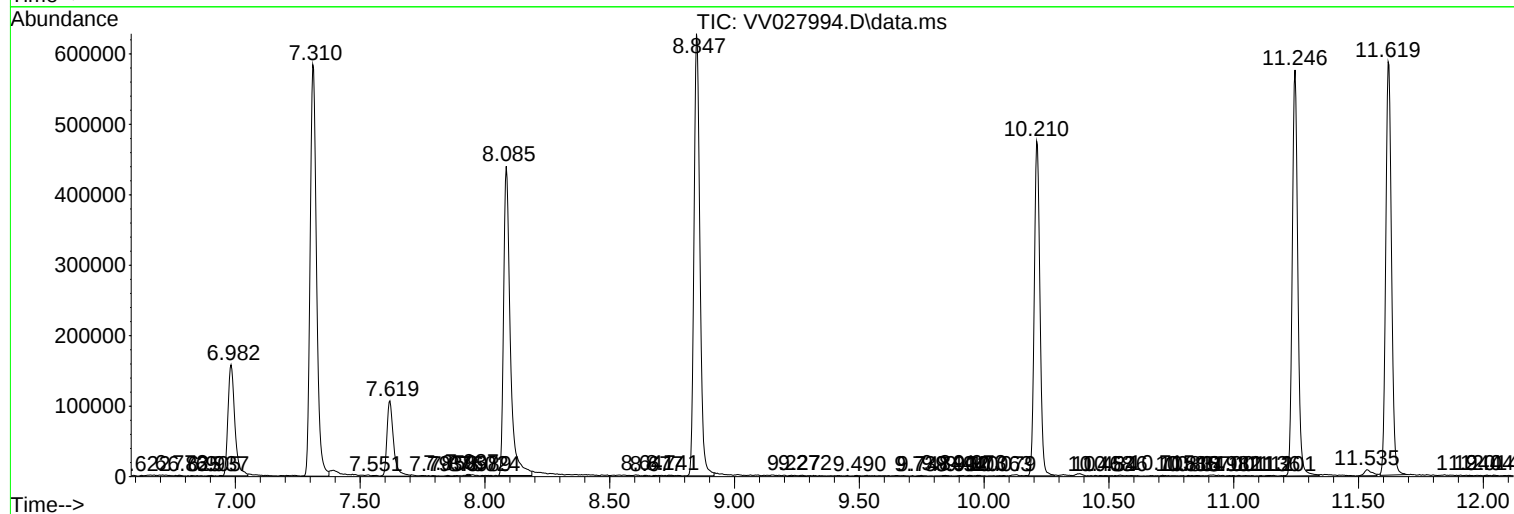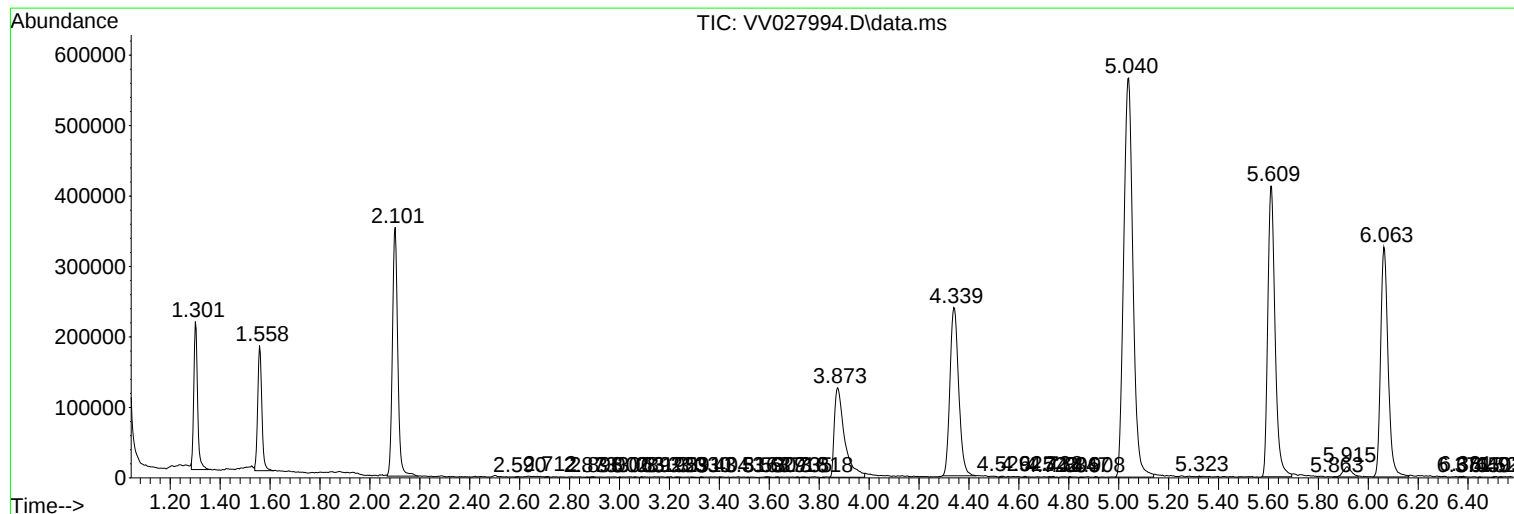

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027994.D
Acq On : 21 Sep 2022 04:43
Operator : SY/MD
Sample : N4674-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

No Library Search Compounds Detected

Data Path : Z:\voasrv\HPCHEM1\MSVOA_V\Data\VV092022\
Data File : VV027994.D
Acq On : 21 Sep 2022 04:43
Operator : SY/MD
Sample : N4674-07
Misc : 5.0mL/MSVOA_V/WATER
ALS Vial : 41 Sample Multiplier: 1

Instrument :
MSVOA_V
ClientSampleId :
C0EA4

Quant Method : Z:\voasrv\HPCHEM1\MSVOA_V\Method\SFAMVLM092022WMA.M
Quant Title : VOC Analysis

TIC Library : C:\Database\NIST11.L
TIC Integration Parameters: LSCINT.P

TIC Top Hit name	RT	EstConc	Units	Response	--Internal Standard--
				#	RT Resp Conc